

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
 Data File : VU046607.D
 Acq On : 27 Dec 2021 18:39
 Operator : SY/MD
 Sample : M5126-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J21

Quant Time: Dec 28 04:58:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 28 04:55:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	69246	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	73077	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	34004	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	3798	0.696	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	14.000%#
7) Chloroethane-d5	1.919	69	5536	1.289	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	25.800%#
11) 1,1-Dichloroethene-d2	2.572	65	1284	0.558	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	11.200%#
20) 2-Butanone-d5	4.645	46	93211	58.916	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.840%
24) Chloroform-d	5.067	84	22497	2.251	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	45.000%#
26) 1,2-Dichloroethane-d4	5.707	65	15468	2.707	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	54.200%#
32) Benzene-d6	5.729	84	25078	1.231	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	24.600%#
36) 1,2-Dichloropropane-d6	6.694	67	12947	2.115	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	42.400%#
41) Toluene-d8	7.899	98	13731	0.743	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	14.800%#
43) trans-1,3-Dichloroprop...	8.182	79	4612	1.629	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	32.600%#
46) 2-Hexanone-d5	8.636	63	78155	47.020	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.040%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	25159	4.005	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.000%
66) 1,2-Dichlorobenzene-d4	12.192	152	16101	2.571	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	51.400%#
Target Compounds						
					Qvalue	
35) Methylcyclohexane	6.694	83	3343	0.310	ug/L #	17
37) 1,2-Dichloropropane	6.687	63	1292	0.174	ug/L #	88
61) 1,2,3-Trichloropropane	11.812	75	3937	0.697	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046607.D
Acq On : 27 Dec 2021 18:39
Operator : SY/MD
Sample : M5126-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J21

Quant Time: Dec 28 04:58:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 28 04:55:25 2021
Response via : Initial Calibration




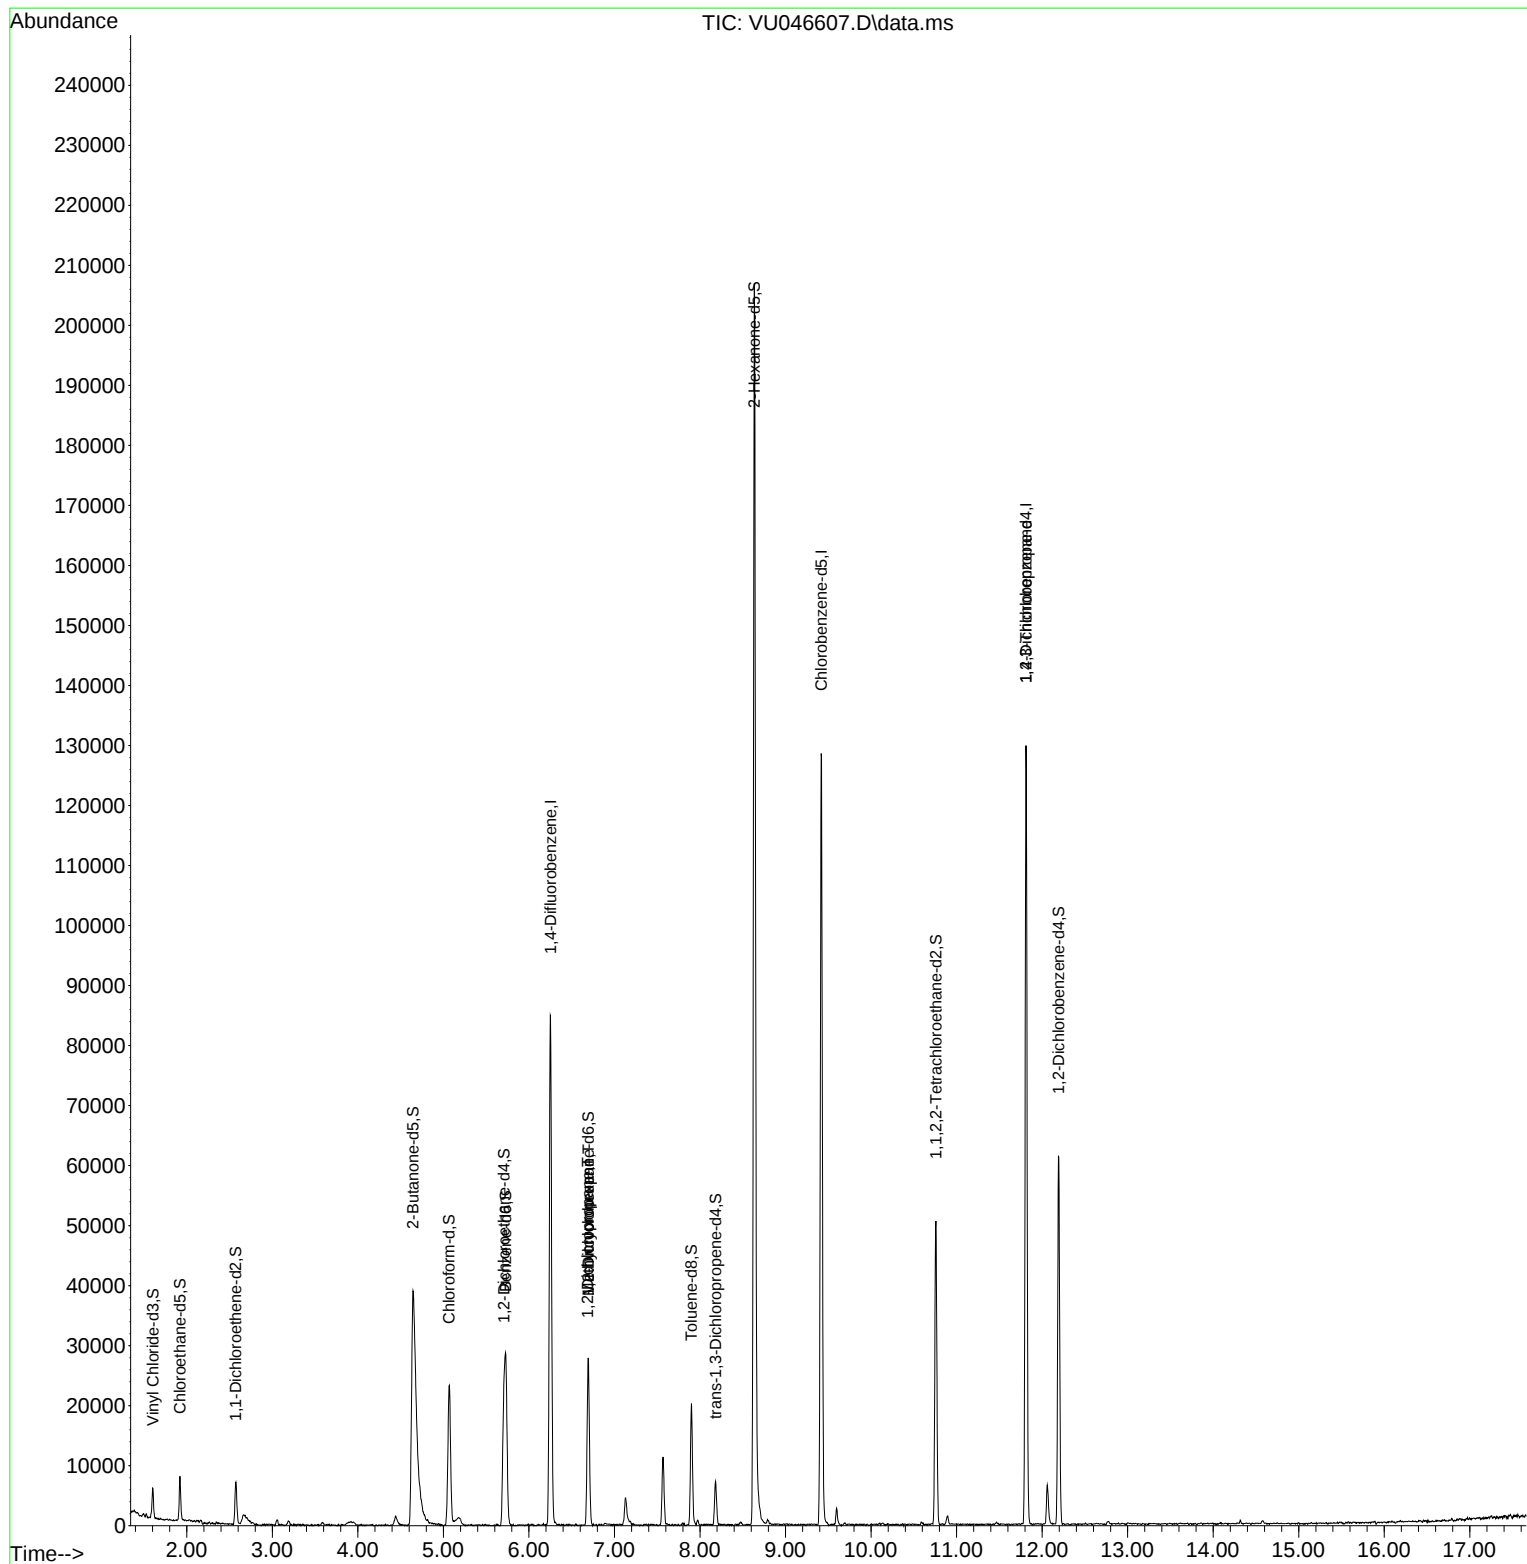


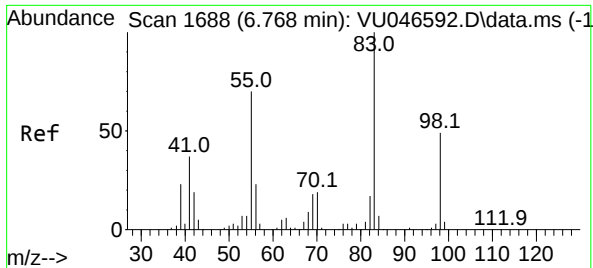

#35
Methylcyclohexane
Concen: 0.310 ug/L
RT: 6.694 min Scan# 1665
Delta R.T. -0.074 min
Lab File: VU046607.D
Acq: 27 Dec 2021 18:39




Instrument :
MSVOA_U
ClientSampleId :
C0J21


Tgt Ion: 83 Resp: 3343
Ion Ratio Lower Upper
83 100
55 0.0 61.9 92.9#
98 0.0 39.0 58.6#

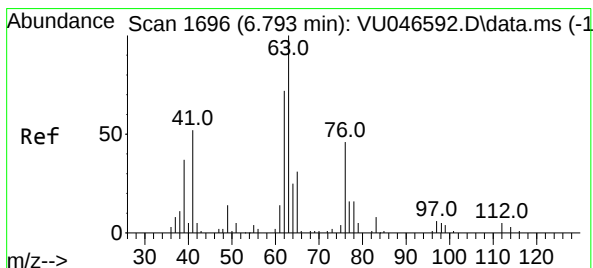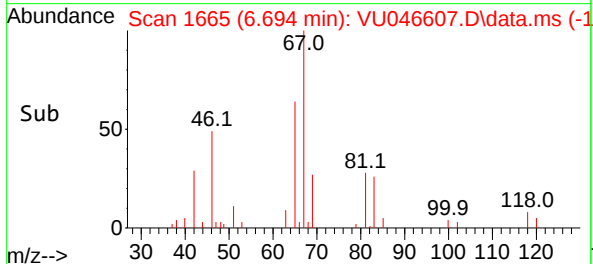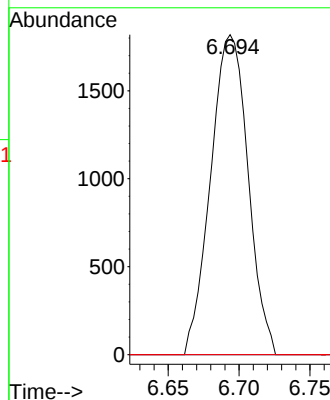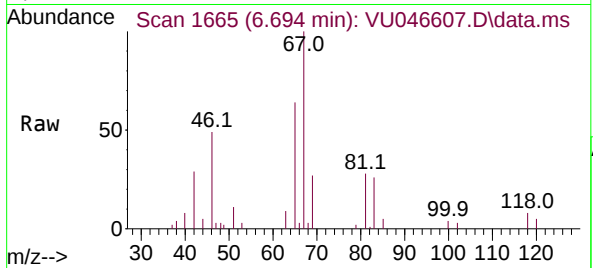

#37
1,2-Dichloropropane
Concen: 0.174 ug/L
RT: 6.687 min Scan# 1663
Delta R.T. -0.106 min
Lab File: VU046607.D
Acq: 27 Dec 2021 18:39


Tgt Ion: 63 Resp: 1292
Ion Ratio Lower Upper
63 100
112 0.0 3.2 4.8#

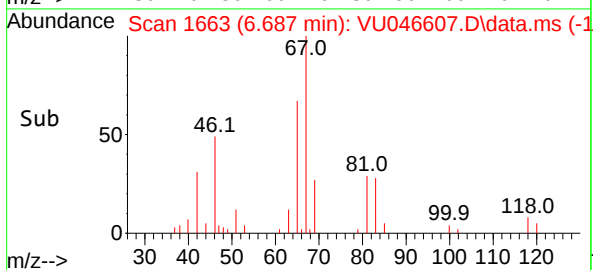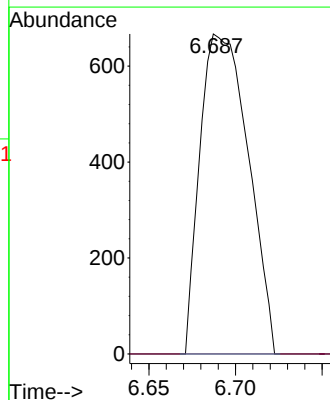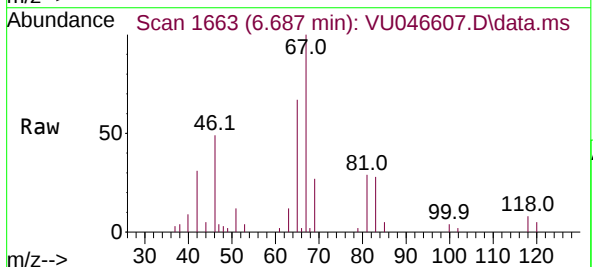

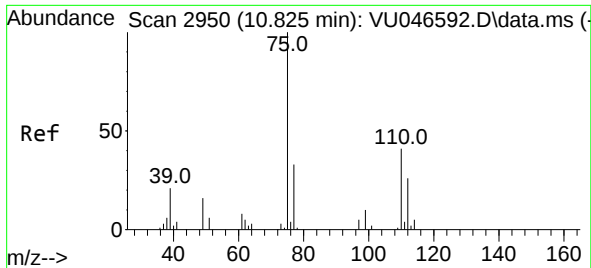

#61
 1,2,3-Trichloropropane
 Concen: 0.697 ug/L
 RT: 11.812 min Scan# 31
 Delta R.T. 0.987 min
 Lab File: VU046607.D
 Acq: 27 Dec 2021 18:39

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J21

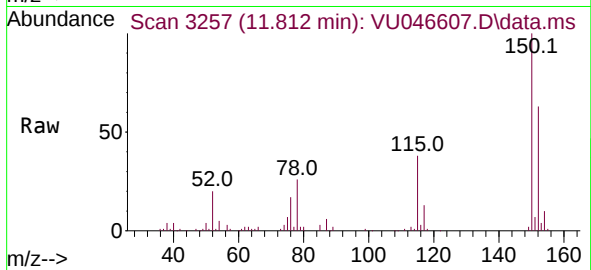

Tgt Ion: 75 Resp: 3937
 Ion Ratio Lower Upper
 75 100
 110 0.0 29.9 44.9#
 77 31.8 25.5 38.3

