

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
 Data File : VU046598.D
 Acq On : 27 Dec 2021 15:01
 Operator : SY/MD
 Sample : M5201-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 P035-TW001-A-01

Quant Time: Dec 28 04:57:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 28 04:55:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	73889	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	73953	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	37197	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	0.000	65	0	0.000	ug/L	
Spiked Amount	5.000	Range	40 - 130	Recovery	=	0.000%#
7) Chloroethane-d5	1.919	69	26685	5.823	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.400%
11) 1,1-Dichloroethene-d2	2.572	65	9793	3.990	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.800%
20) 2-Butanone-d5	4.646	46	103096	61.069	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.140%
24) Chloroform-d	5.067	84	62949	5.903	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	118.000%
26) 1,2-Dichloroethane-d4	5.707	65	37437	6.141	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.800%
32) Benzene-d6	5.732	84	123236	5.978	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	119.600%
36) 1,2-Dichloropropane-d6	6.694	67	37648	6.077	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	121.600%
41) Toluene-d8	7.899	98	64460	3.445	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.000%#
43) trans-1,3-Dichloroprop...	8.182	79	10442	3.645	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.800%
46) 2-Hexanone-d5	8.636	63	87836	52.218	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.440%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	36009	5.664	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	41881	6.112	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.200%#
Target Compounds					Qvalue	
25) Chloroform	5.092	83	18992	1.376	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046598.D
Acq On : 27 Dec 2021 15:01
Operator : SY/MD
Sample : M5201-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
P035-TW001-A-01

Quant Time: Dec 28 04:57:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 28 04:55:25 2021
Response via : Initial Calibration

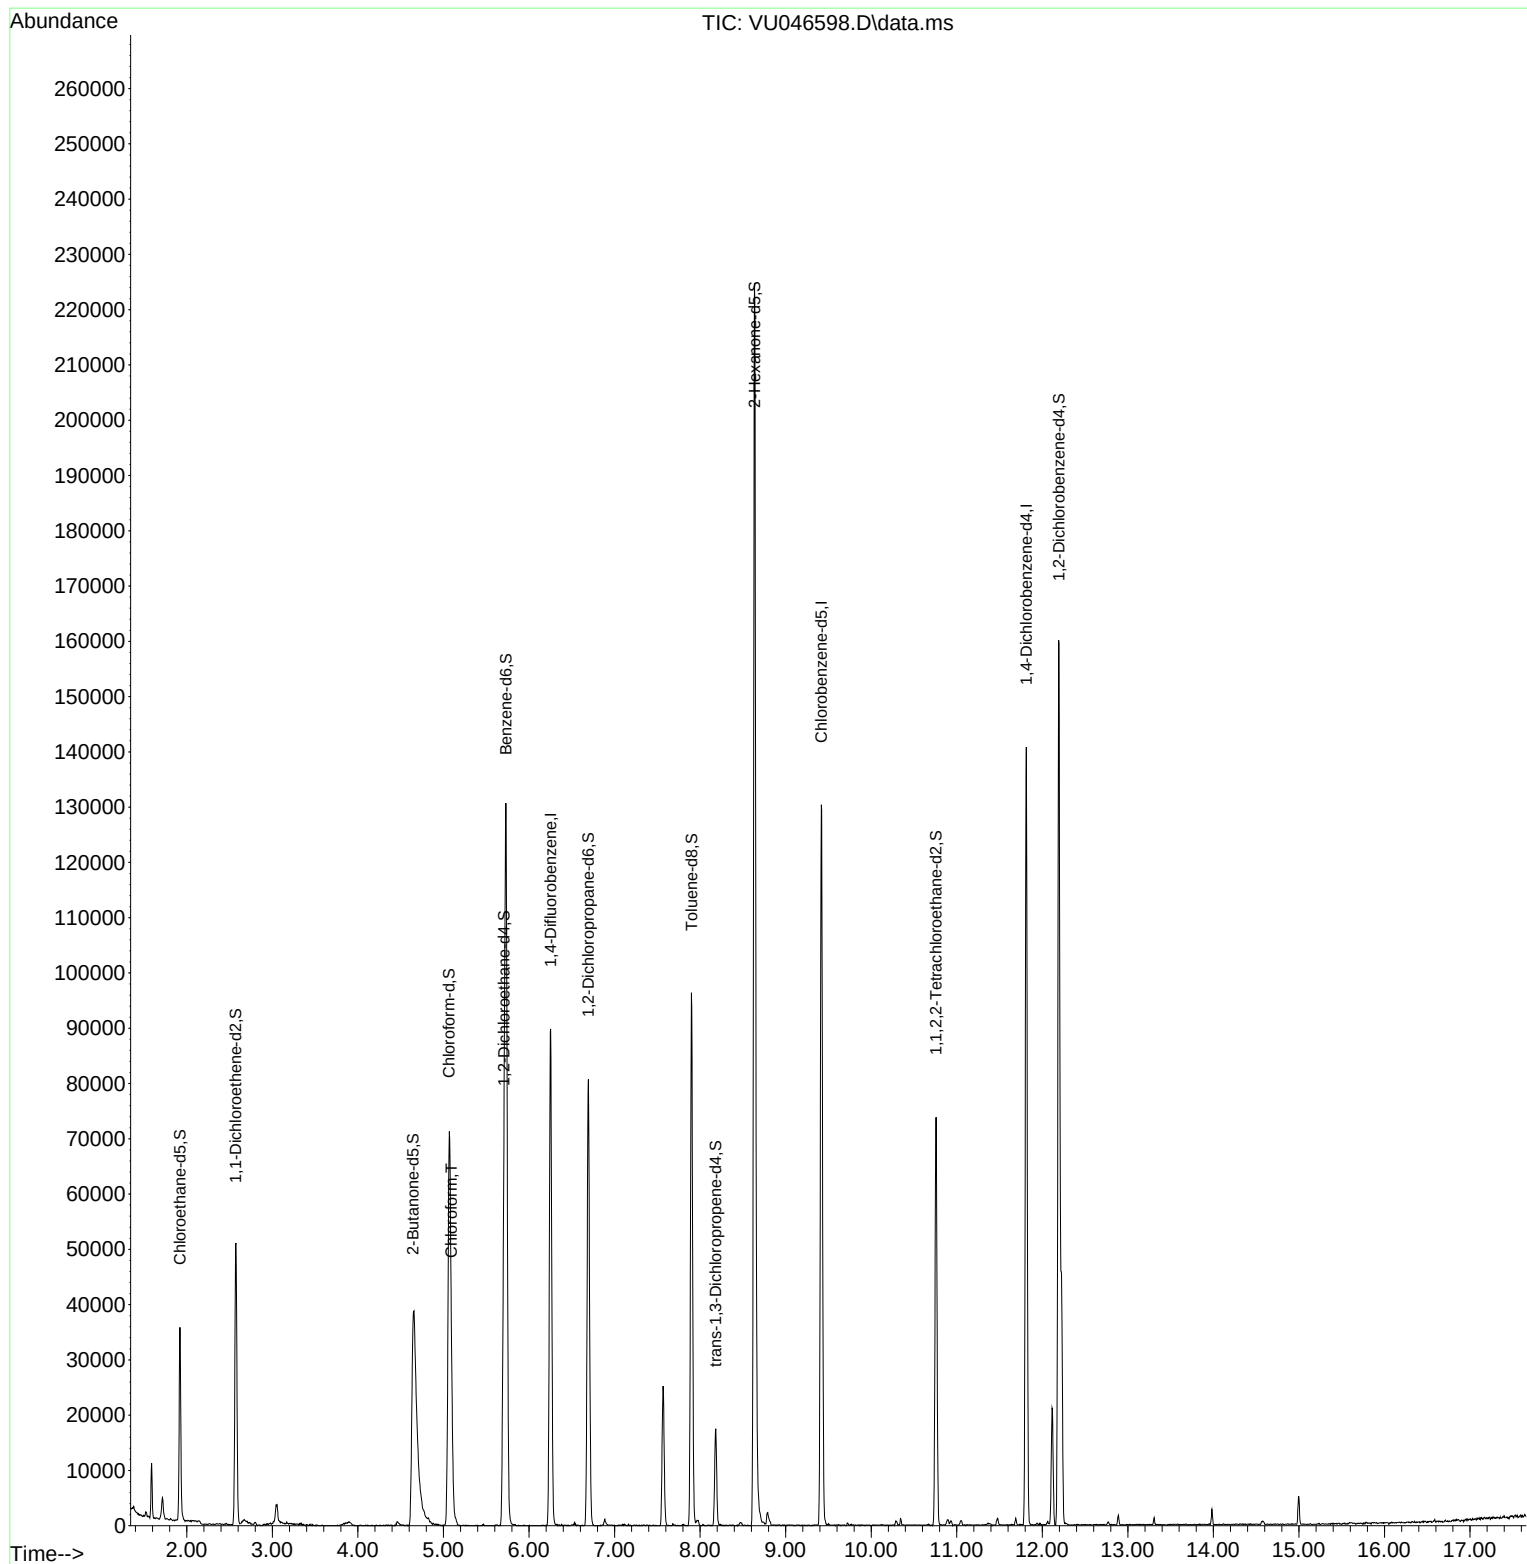

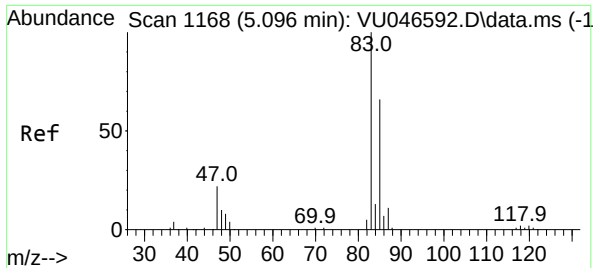

#25
 Chloroform
 Concen: 1.376 ug/L
 RT: 5.092 min Scan# 11
 Delta R.T. -0.003 min
 Lab File: VU046598.D
 Acq: 27 Dec 2021 15:01

Instrument :
 MSVOA_U
 ClientSampleId :
 P035-TW001-A-01

Tgt Ion: 83 Resp: 18992
 Ion Ratio Lower Upper
 83 100
 85 66.3 46.9 87.1

