

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
 Data File : VU046605.D
 Acq On : 27 Dec 2021 17:51
 Operator : SY/MD
 Sample : M5126-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	76	82	92	rBV	4498	5387	1.49%	0.313%
2	1.919	173	180	190	rBV	7074	8652	2.40%	0.503%
3	2.147	242	251	263	rVB2	3882	6539	1.81%	0.380%
4	2.575	375	384	394	rBV2	7203	11803	3.27%	0.687%
5	3.870	776	787	802	rVB2	2285	5907	1.64%	0.344%
6	4.665	1014	1034	1076	rBV2	44131	184165	51.06%	10.715%
7	5.070	1146	1160	1177	rBV	22592	52490	14.55%	3.054%
8	5.321	1226	1238	1251	rBV2	5794	12303	3.41%	0.716%
9	5.722	1344	1363	1382	rVB3	26792	81120	22.49%	4.720%
10	6.253	1513	1528	1552	rVB	93667	175954	48.78%	10.237%
11	6.546	1605	1619	1632	rBB3	22652	41737	11.57%	2.428%
12	6.693	1653	1665	1679	rBV	25626	48088	13.33%	2.798%
13	7.568	1926	1937	1951	rBV3	10296	18125	5.02%	1.055%
14	7.899	2027	2040	2056	rBB	18919	31847	8.83%	1.853%
15	8.182	2118	2128	2141	rVB2	7097	11806	3.27%	0.687%
16	8.555	2234	2244	2254	rVB3	16132	26582	7.37%	1.547%
17	8.635	2254	2269	2301	rBV	200062	360707	100.00%	20.986%
18	9.420	2500	2513	2531	rBV	143258	232665	64.50%	13.537%
19	10.758	2918	2929	2945	rVB	49901	79081	21.92%	4.601%
20	11.812	3245	3257	3272	rBV	142210	226887	62.90%	13.200%
21	12.063	3328	3335	3343	rBV3	3228	4515	1.25%	0.263%
22	12.195	3364	3376	3389	rBV	58977	92420	25.62%	5.377%




Sum of corrected areas: 1718780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046605.D
Acq On : 27 Dec 2021 17:51
Operator : SY/MD
Sample : M5126-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

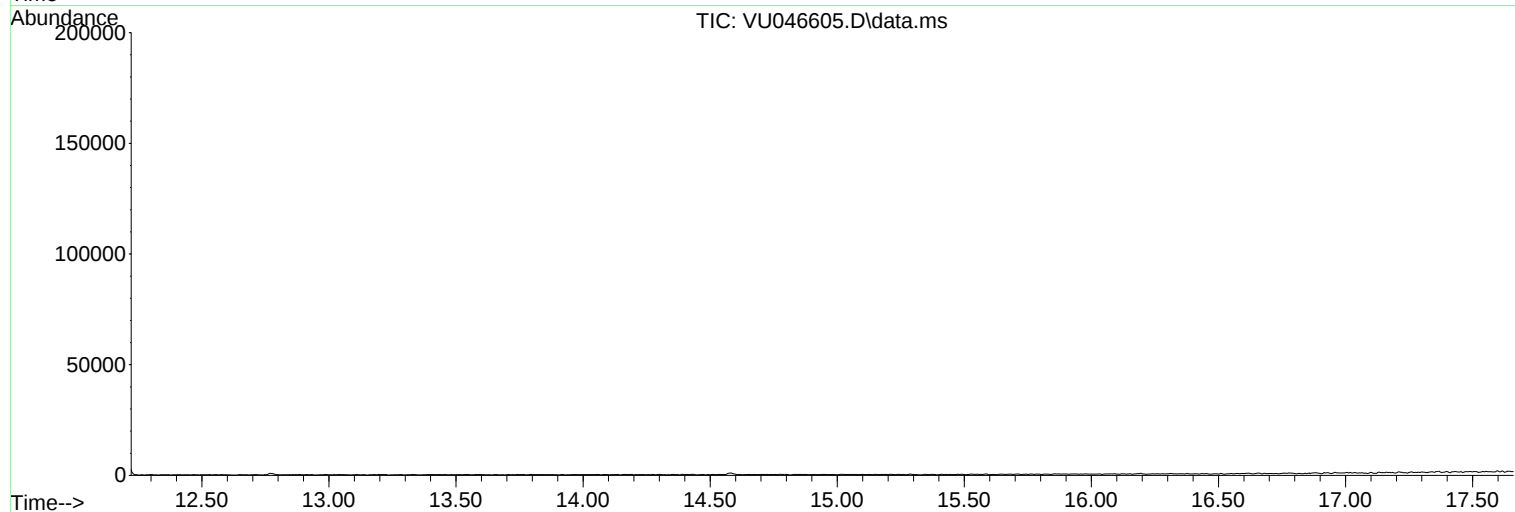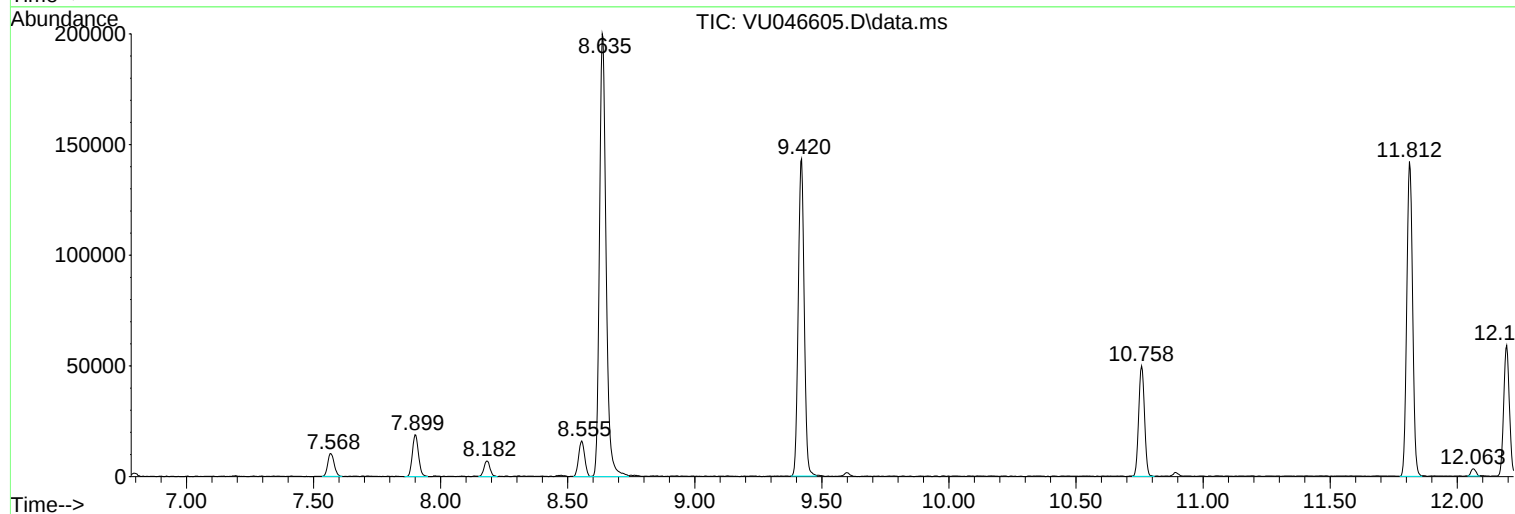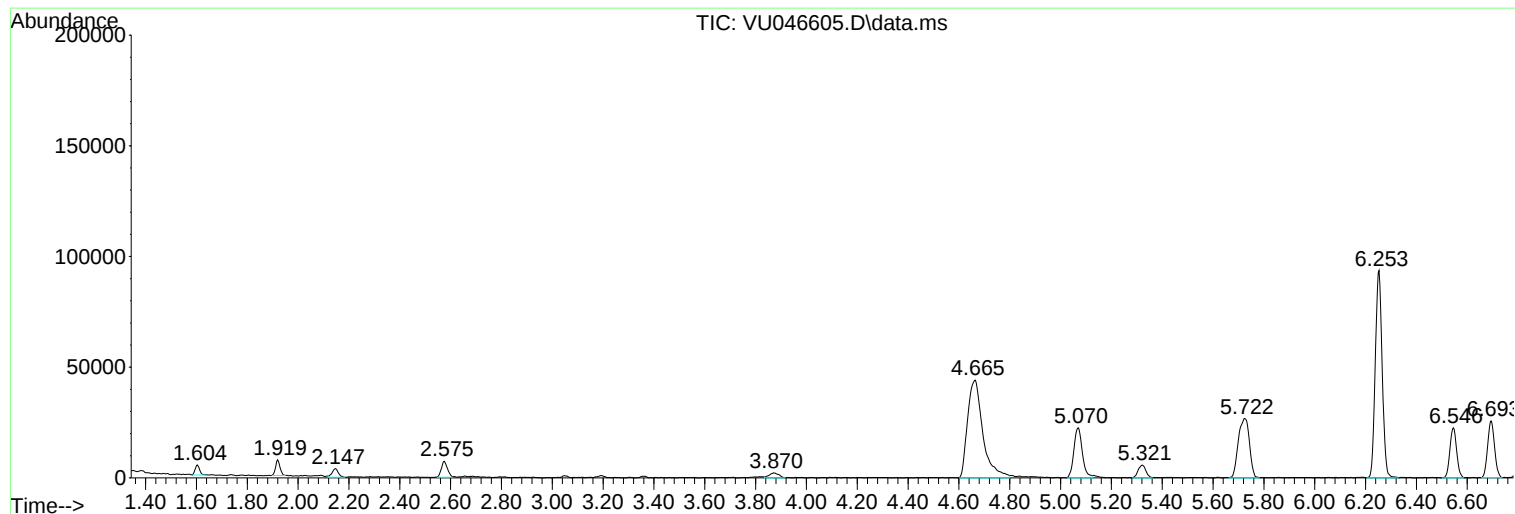

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046605.D
Acq On : 27 Dec 2021 17:51
Operator : SY/MD
Sample : M5126-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046605.D
Acq On : 27 Dec 2021 17:51
Operator : SY/MD
Sample : M5126-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
