

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
 Data File : VU046606.D
 Acq On : 27 Dec 2021 18:15
 Operator : SY/MD
 Sample : M5126-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J17

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.494	42	48	57	rVB	15134	15063	4.14%	0.933%
2	1.604	73	82	90	rVB3	4922	6959	1.91%	0.431%
3	1.919	173	180	189	rVB	6745	7890	2.17%	0.489%
4	2.575	372	384	393	rBV2	6761	10817	2.97%	0.670%
5	3.054	524	533	543	rVB5	2043	3866	1.06%	0.239%
6	4.648	1013	1029	1071	rBV	38331	159264	43.79%	9.864%
7	5.066	1146	1159	1179	rBV2	23103	52069	14.32%	3.225%
8	5.726	1345	1364	1381	rBV3	27854	83204	22.88%	5.153%
9	6.253	1515	1528	1544	rBV	87112	162027	44.55%	10.035%
10	6.693	1653	1665	1678	rBV	25894	49596	13.64%	3.072%
11	7.568	1926	1937	1947	rBV2	10393	17867	4.91%	1.107%
12	7.902	2030	2041	2053	rBV	18788	32575	8.96%	2.017%
13	7.970	2053	2062	2076	rVB2	10293	16993	4.67%	1.052%
14	8.182	2119	2128	2142	rVB2	7587	12874	3.54%	0.797%
15	8.635	2257	2269	2300	rBV	204115	363733	100.00%	22.527%
16	9.420	2501	2513	2531	rBV	129478	217799	59.88%	13.489%
17	9.597	2561	2568	2579	rVB2	2990	4282	1.18%	0.265%
18	10.758	2916	2929	2946	rBV	50388	81042	22.28%	5.019%
19	11.812	3246	3257	3273	rBV	133425	209923	57.71%	13.001%
20	12.063	3326	3335	3349	rVB	6521	10419	2.86%	0.645%
21	12.195	3363	3376	3388	rBV2	59252	96394	26.50%	5.970%




Sum of corrected areas: 1614656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046606.D
Acq On : 27 Dec 2021 18:15
Operator : SY/MD
Sample : M5126-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

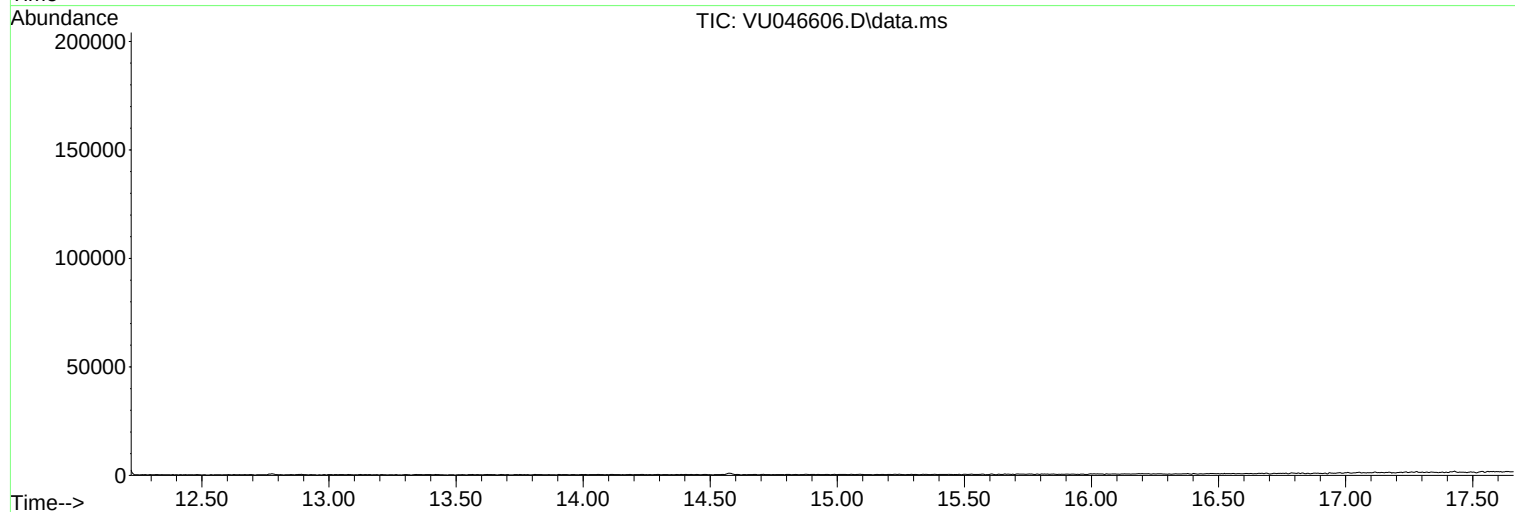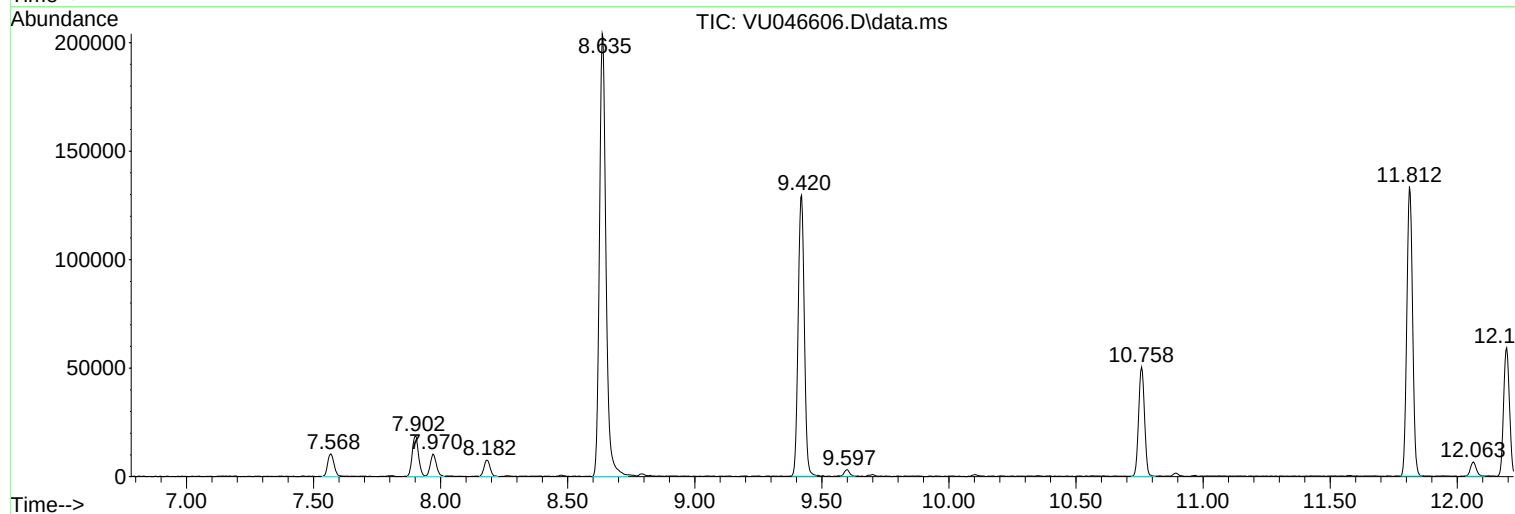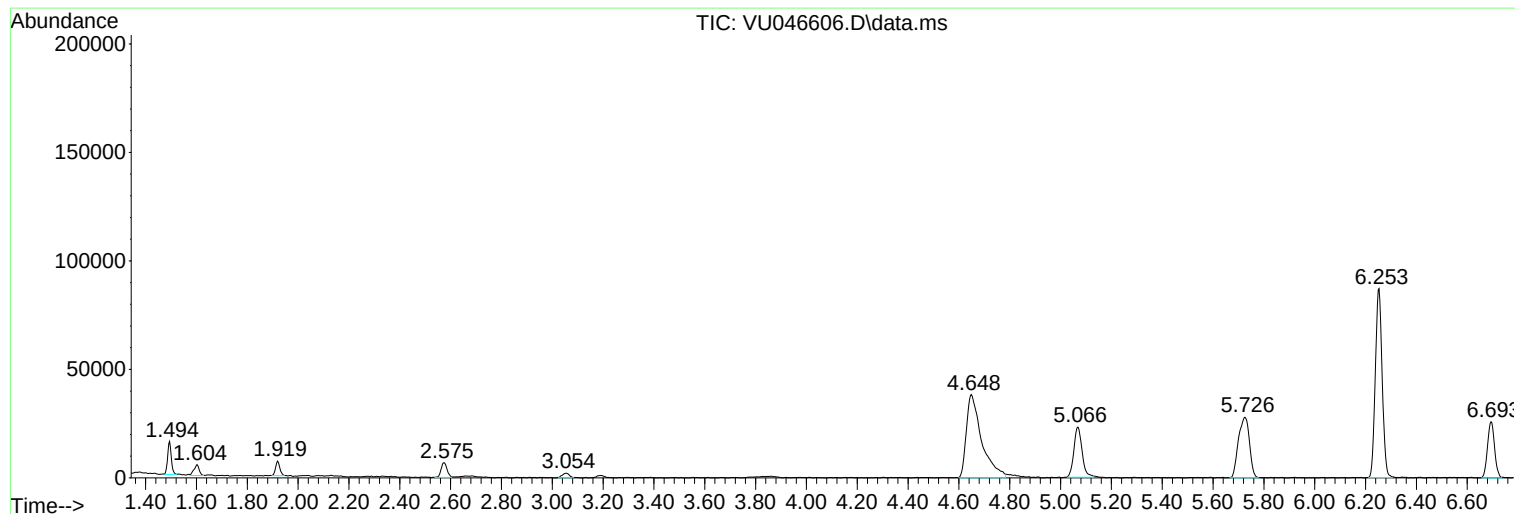

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046606.D
Acq On : 27 Dec 2021 18:15
Operator : SY/MD
Sample : M5126-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
Data File : VU046606.D
Acq On : 27 Dec 2021 18:15
Operator : SY/MD
Sample : M5126-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc