


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122721\
 Data File : VU046591.D
 Acq On : 27 Dec 2021 09:26
 Operator : SY/MD
 Sample : BFB036
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB036

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 30 04:21:35 2021

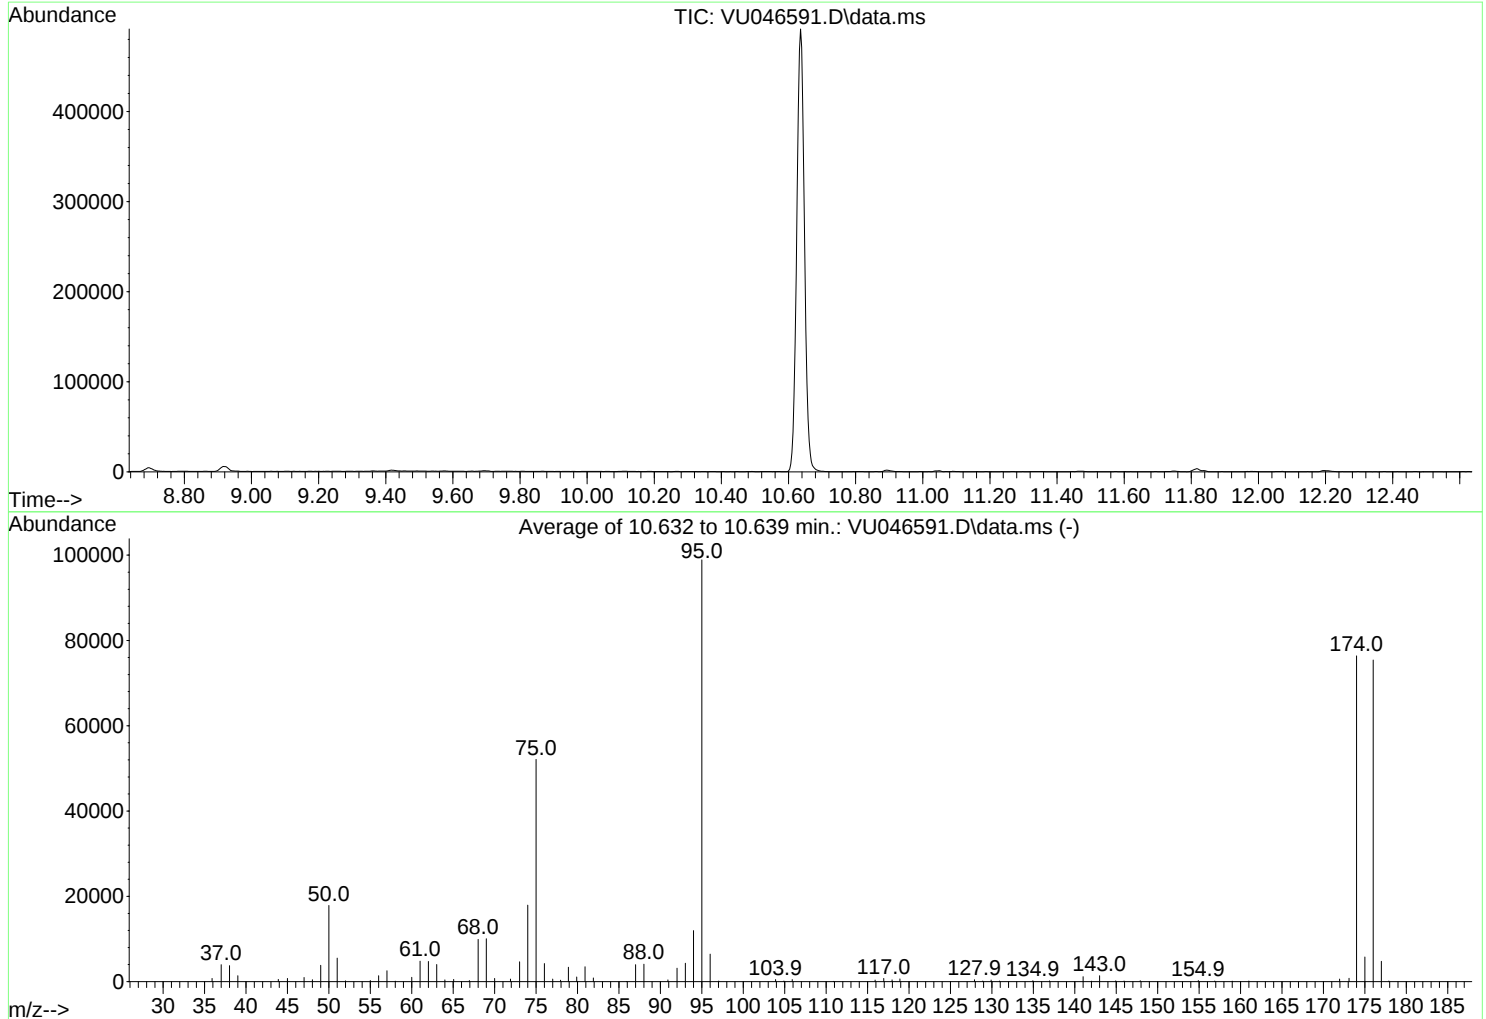

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	17877	PASS
75	95	30	80	52.7	52107	PASS
95	95	100	100	100.0	98899	PASS
96	95	5	9	6.5	6445	PASS
173	174	0.00	2	1.0	801	PASS
174	95	50	120	77.3	76403	PASS
175	174	5	9	7.6	5771	PASS
176	174	95	101	98.7	75424	PASS
177	176	5	9	6.3	4773	PASS

m/z	Abundance
35.90	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.90	995.0
37.00	4031.0
38.00	3735.0
39.00	1388.0
43.90	497.0
45.00	720.0
47.00	967.0
48.00	446.0
49.00	3740.0
50.00	17576.0
51.00	5420.0
52.00	187.0
55.00	253.0
56.00	1394.0
57.00	2616.0
57.90	104.0
60.00	997.0
61.00	4980.0
62.00	4755.0
63.00	4113.0
64.00	372.0
65.00	594.0
67.00	250.0
68.00	9676.0
69.00	10095.0
70.00	868.0
71.90	601.0
73.00	4535.0
74.00	18000.0
75.00	51512.0
76.00	4262.0
77.00	573.0
78.00	306.0
78.90	3336.0
79.90	1015.0
80.90	3508.0
81.90	888.0
85.90	112.0
87.00	4005.0
88.00	3975.0
90.90	394.0
92.00	3219.0
93.00	4225.0
94.00	12036.0
95.00	97128.0
96.00	6405.0
97.10	165.0
103.90	457.0
104.90	136.0
105.90	485.0
110.90	119.0
115.90	356.0
116.90	731.0
117.90	449.0
118.90	674.0
127.90	400.0
128.90	153.0
129.90	362.0
130.90	137.0
134.90	227.0
136.90	167.0
141.00	1072.0
142.00	108.0
143.00	1328.0
145.00	223.0
145.90	170.0
147.90	213.0
154.90	270.0
156.90	182.0
161.00	153.0
172.00	635.0
173.10	773.0
174.00	73576.0
175.00	5538.0
176.00	72488.0
177.00	4580.0
177.90	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
36.00	993.0
37.00	4058.0
38.00	3890.0
39.00	1453.0
43.90	560.0
45.00	779.0
47.00	1011.0
48.00	463.0
49.00	3988.0
50.00	18504.0
51.00	5696.0
52.00	183.0
55.00	289.0
56.00	1412.0
57.00	2666.0
58.00	125.0
60.00	1065.0
61.00	4901.0
62.00	4885.0
63.00	4197.0
64.00	426.0
65.10	504.0
67.00	258.0
68.00	10205.0
69.00	10298.0
70.00	786.0
71.90	605.0
73.00	4834.0
74.00	18592.0
75.00	53688.0
76.00	4350.0
77.00	619.0
78.00	345.0
78.90	3475.0
79.90	1127.0
80.90	3563.0
81.90	908.0
87.00	4121.0
88.00	4245.0
90.90	435.0
92.00	3241.0
93.00	4460.0
94.00	12322.0
95.00	102120.0
96.00	6649.0
97.00	169.0
103.90	497.0
104.90	151.0
105.90	532.0
110.90	120.0
115.90	396.0
117.00	763.0
117.90	436.0
118.90	669.0
127.90	463.0
128.90	180.0
129.90	392.0
130.90	143.0
134.90	258.0
136.90	174.0
141.00	1220.0
142.00	105.0
143.00	1409.0
144.90	207.0
146.00	165.0
147.90	224.0
154.90	271.0
156.90	142.0
159.00	144.0
161.00	161.0
172.00	614.0
173.10	843.0
174.00	78728.0
175.00	5959.0
176.00	77608.0
177.00	4886.0
177.90	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036

m/z	Abundance
35.90	882.0
37.00	3817.0
38.00	3669.0
39.00	1351.0
43.90	577.0
45.00	764.0
47.00	928.0
48.00	439.0
49.00	3789.0
50.00	17552.0
51.00	5450.0
52.00	179.0
55.00	278.0
56.00	1389.0
57.00	2371.0
58.10	120.0
60.00	981.0
61.00	4492.0
62.00	4514.0
63.00	3752.0
64.00	405.0
65.00	426.0
66.90	276.0
68.00	9872.0
69.00	9802.0
70.00	641.0
71.90	553.0
73.00	4585.0
74.00	17248.0
75.00	51120.0
76.00	4116.0
77.00	597.0
77.90	364.0
78.90	3329.0
79.90	1101.0
80.90	3432.0
81.90	843.0
87.00	3754.0
88.00	4057.0
90.90	461.0
92.00	3020.0
93.00	4275.0
94.00	11564.0
95.00	97448.0
96.00	6280.0
97.00	163.0
103.90	534.0
104.90	152.0
105.90	471.0
115.90	396.0
117.00	753.0
118.00	406.0
118.90	599.0
127.90	463.0
128.90	178.0
129.90	403.0
130.90	132.0
135.00	241.0
137.00	187.0
141.00	1237.0
142.00	109.0
143.00	1415.0
144.90	182.0
146.00	119.0
147.90	227.0
154.90	245.0
156.90	103.0
159.00	178.0
161.00	147.0
171.90	550.0
173.10	786.0
174.00	76904.0
175.00	5817.0
176.00	76176.0
177.00	4853.0
177.90	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB036