

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122722\
 Data File : VU052556.D
 Acq On : 27 Dec 2022 11:59
 Operator : JC/MD
 Sample : N6170-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBQB5

Quant Time: Dec 28 01:19:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 28 01:18:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	159041	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	152539	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	67738	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	56037	3.478	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.600%
7) Chloroethane-d5	1.916	69	55215	3.974	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.400%
11) 1,1-Dichloroethene-d2	2.568	65	25395	3.663	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	4.629	46	287509	57.542	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.080%
24) Chloroform-d	5.060	84	118447	4.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
26) 1,2-Dichloroethane-d4	5.697	65	74040	4.695	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.722	84	234512	4.484	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	6.687	67	83957	4.664	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.896	98	177413	4.041	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.800%
43) trans-1,3-Dichloroprop...	8.176	79	29478	4.782	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.600%
46) 2-Hexanone-d5	8.629	63	198751	58.930	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.860%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	78970	5.167	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.400%
66) 1,2-Dichlorobenzene-d4	12.188	152	68782	4.988	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						Qvalue
5) Vinyl chloride	1.607	62	5708	0.308	ug/L	84
13) Acetone	2.649	43	19688	5.345	ug/L	95
14) Carbon disulfide	2.797	76	16794	0.438	ug/L	98
15) Methyl Acetate	2.960	43	3820	0.471	ug/L #	55
16) Methylene chloride	3.044	84	8258	0.491	ug/L	93
18) trans-1,2-Dichloroethene	3.353	96	10502	0.856	ug/L	94
22) cis-1,2-Dichloroethene	4.665	96	83332	6.186	ug/L	96
33) Benzene	5.777	78	10944	0.199	ug/L	100
37) 1,2-Dichloropropane	6.687	63	8524	0.556	ug/L #	88
47) Tetrachloroethene	8.549	164	1289	0.144	ug/L	86
53) m,p-Xylene	9.690	106	2873	0.143	ug/L	82
54) o-Xylene	10.095	106	3429	0.178	ug/L	90
61) 1,2,3-Trichloropropane	11.806	75	9468	0.975	ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122722\
Data File : VU052556.D
Acq On : 27 Dec 2022 11:59
Operator : JC/MD
Sample : N6170-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQB5

Quant Time: Dec 28 01:19:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 28 01:18:16 2022
Response via : Initial Calibration




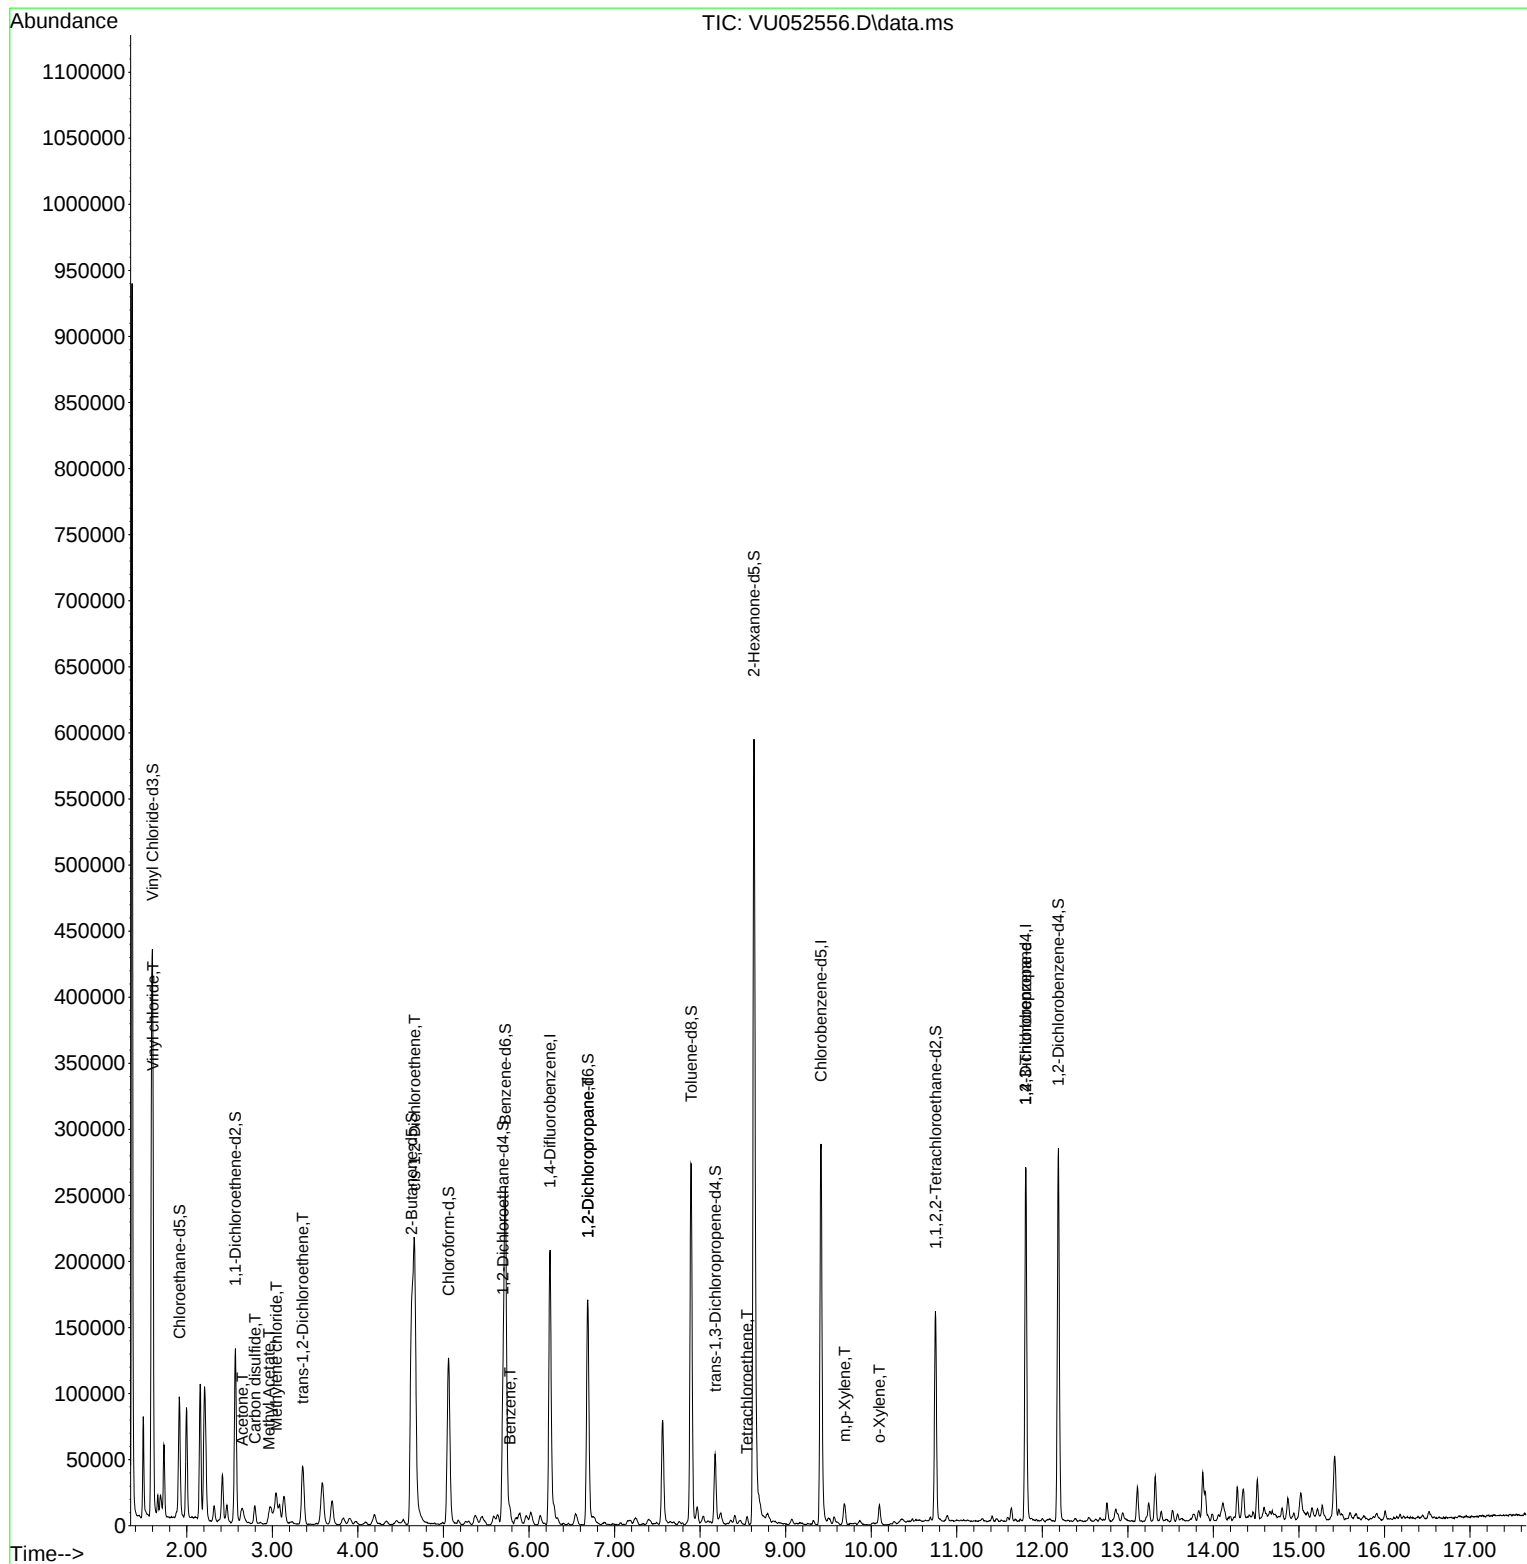


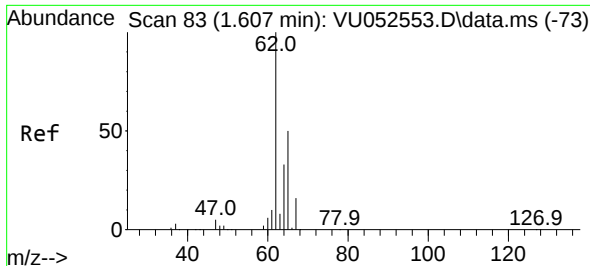

#5
 Vinyl chloride
 Concen: 0.308 ug/L
 RT: 1.607 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VU052556.D
 Acq: 27 Dec 2022 11:59




Instrument :
 MSVOA_U
 ClientSampleId :
 GBQB5


Tgt Ion: 62 Resp: 5708
 Ion Ratio Lower Upper
 62 100
 64 44.0 24.4 45.4

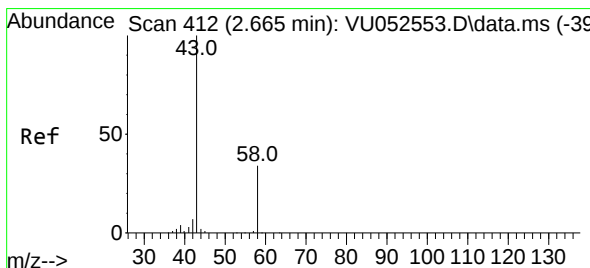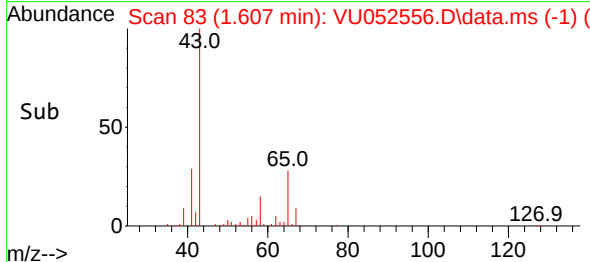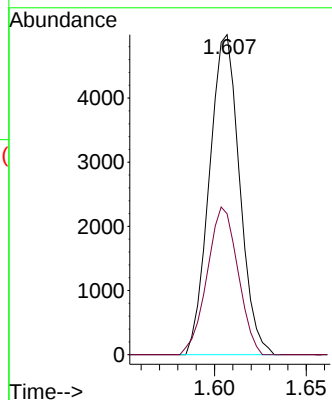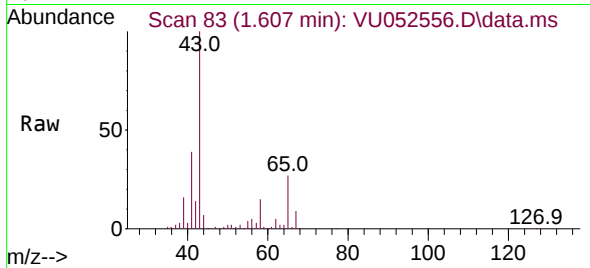

#13
 Acetone
 Concen: 5.345 ug/L
 RT: 2.649 min Scan# 407
 Delta R.T. -0.016 min
 Lab File: VU052556.D
 Acq: 27 Dec 2022 11:59

Tgt Ion: 43 Resp: 19688
 Ion Ratio Lower Upper
 43 100
 58 35.8 0.0 65.4


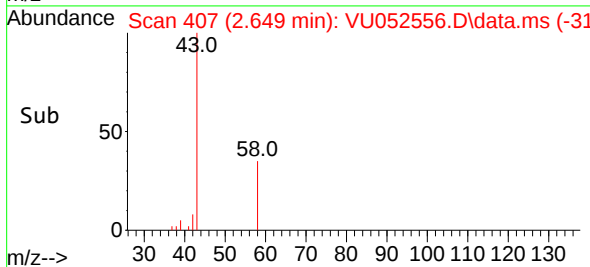
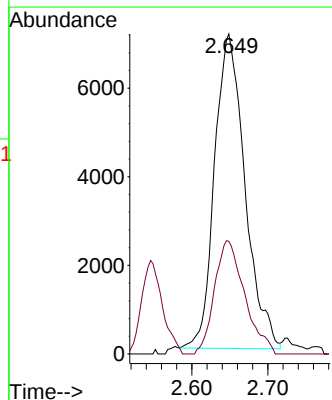
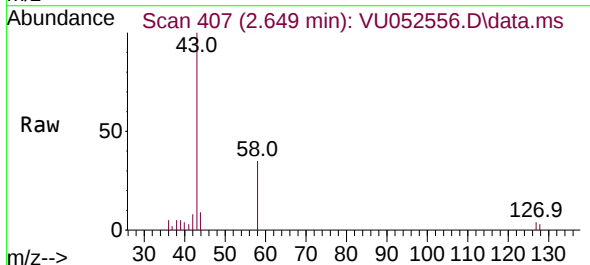


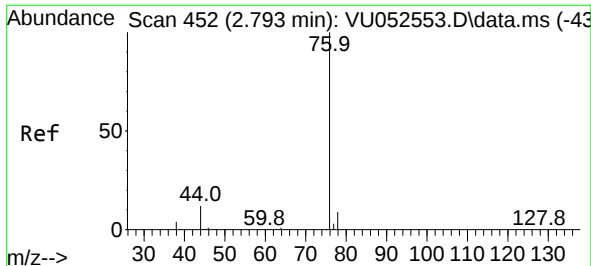

#14
Carbon disulfide
Concen: 0.438 ug/L
RT: 2.797 min Scan# 41
Delta R.T. 0.003 min
Lab File: VU052556.D
Acq: 27 Dec 2022 11:59




Instrument :
MSVOA_U
ClientSampleId :
GBQB5


Tgt Ion: 76 Resp: 16794
Ion Ratio Lower Upper
76 100
78 8.1 7.1 10.7

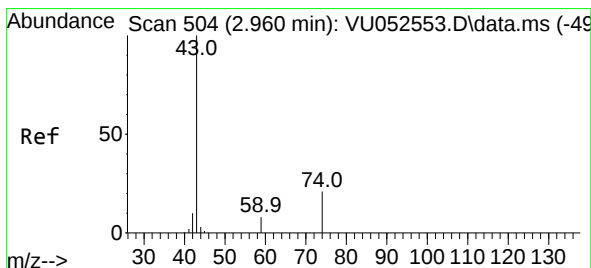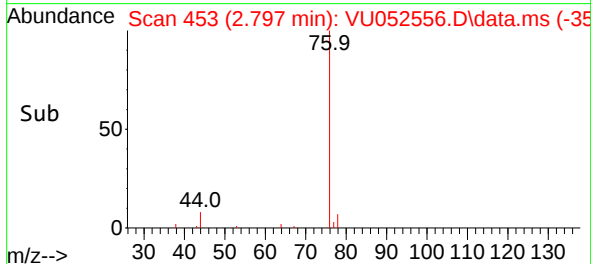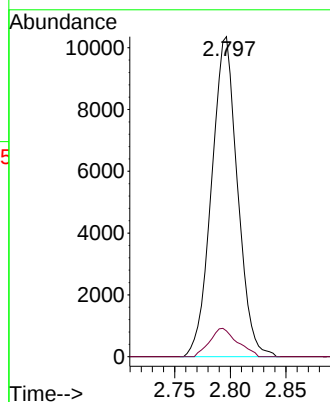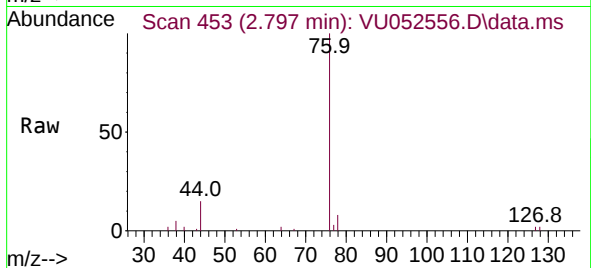

#15
Methyl Acetate
Concen: 0.471 ug/L
RT: 2.960 min Scan# 504
Delta R.T. 0.000 min
Lab File: VU052556.D
Acq: 27 Dec 2022 11:59

Tgt Ion: 43 Resp: 3820
Ion Ratio Lower Upper
43 100
74 0.0 16.9 25.3#


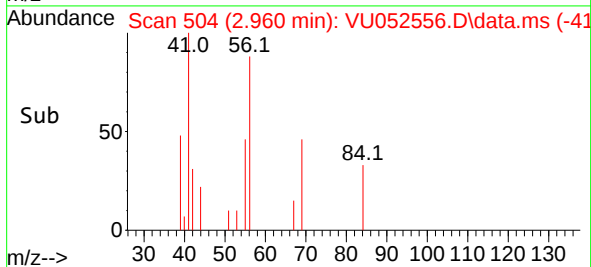
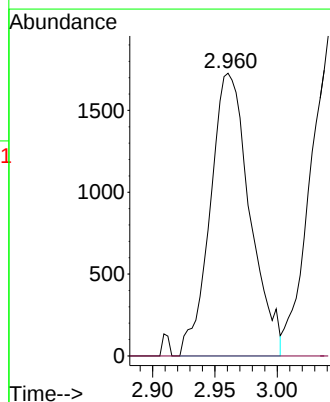
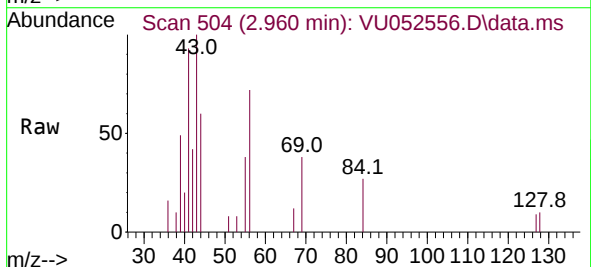


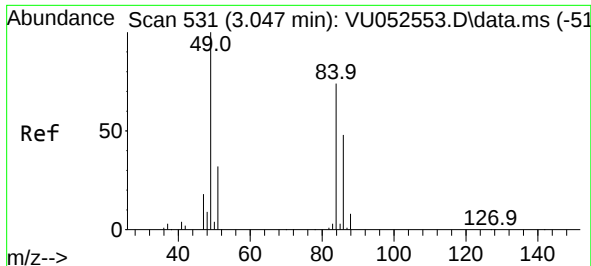

#16
Methylene chloride
Concen: 0.491 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU052556.D
Acq: 27 Dec 2022 11:59




Instrument :
MSVOA_U
ClientSampleId :
GBQB5


Tgt Ion: 84 Resp: 8258
Ion Ratio Lower Upper
84 100
86 61.9 44.7 83.1
49 143.7 93.3 173.3

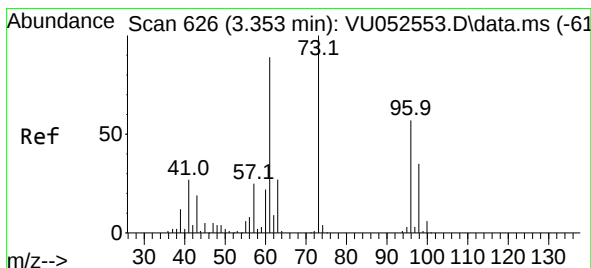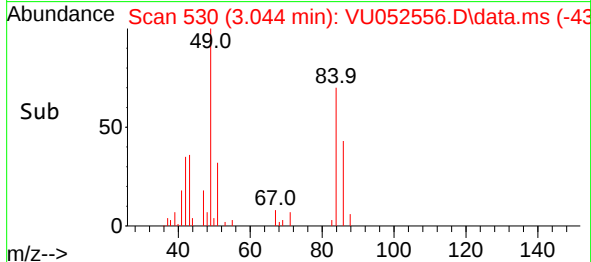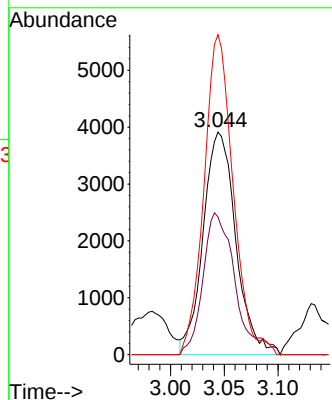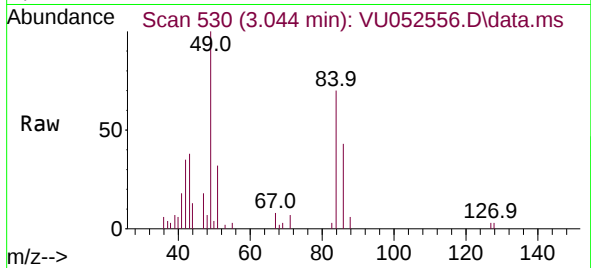

#18
trans-1,2-Dichloroethene
Concen: 0.856 ug/L
RT: 3.353 min Scan# 626
Delta R.T. 0.000 min
Lab File: VU052556.D
Acq: 27 Dec 2022 11:59

Tgt Ion: 96 Resp: 10502
Ion Ratio Lower Upper
96 100
61 161.3 108.3 201.1
98 69.4 44.0 81.6


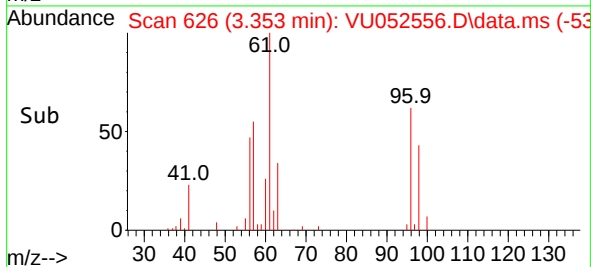
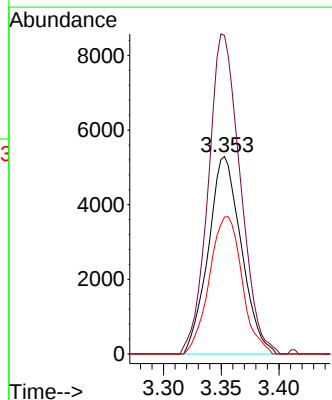
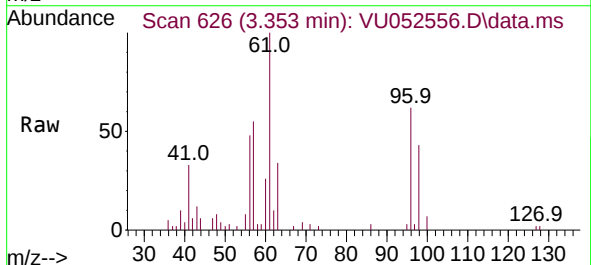


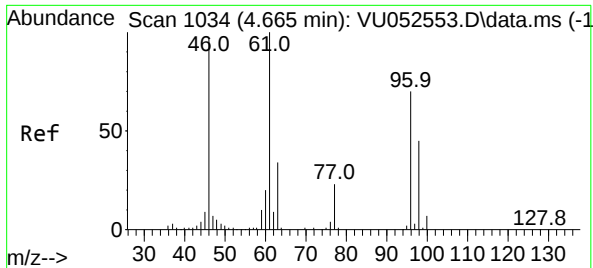

#22
 cis-1,2-Dichloroethene
 Concen: 6.186 ug/L
 RT: 4.665 min Scan# 1034
 Delta R.T. 0.000 min
 Lab File: VU052556.D
 Acq: 27 Dec 2022 11:59




Instrument :
 MSVOA_U
 ClientSampleId :
 GBQB5


Tgt Ion: 96 Resp: 83332
 Ion Ratio Lower Upper
 96 100
 61 145.4 96.9 180.1
 98 65.3 44.7 83.1

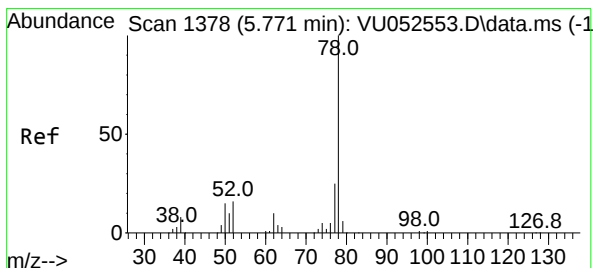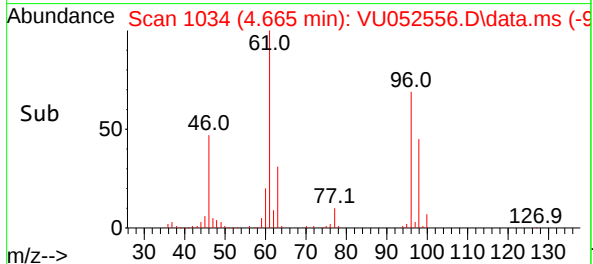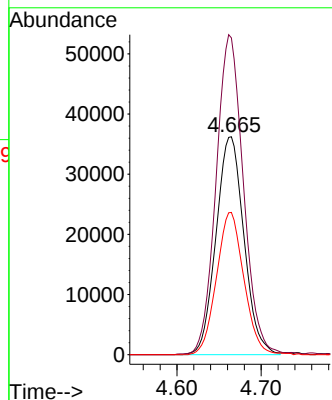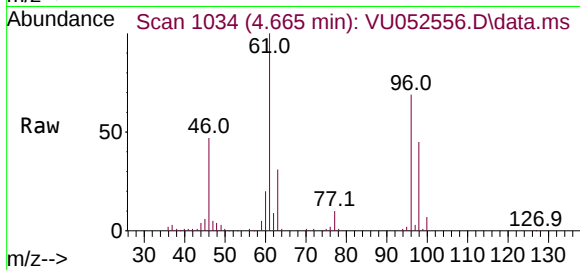

#33
 Benzene
 Concen: 0.199 ug/L
 RT: 5.777 min Scan# 1380
 Delta R.T. 0.006 min
 Lab File: VU052556.D
 Acq: 27 Dec 2022 11:59

Tgt Ion: 78 Resp: 10944

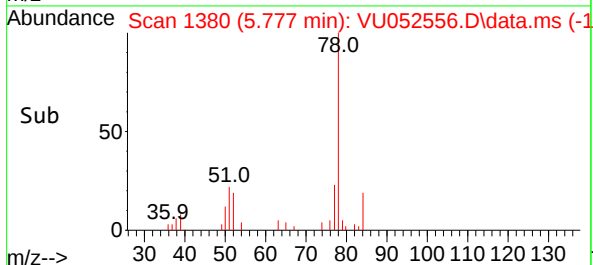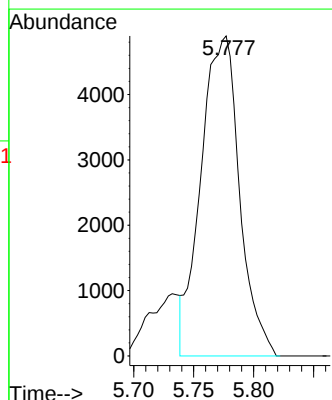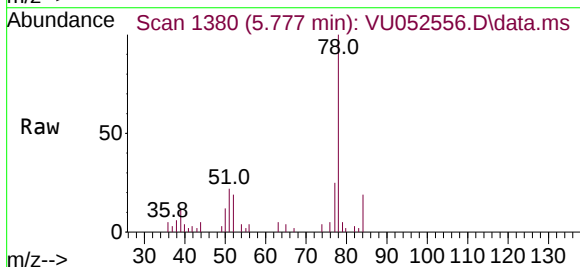

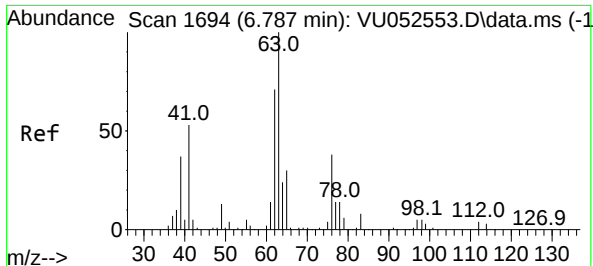

#37

1,2-Dichloropropane

Concen: 0.556 ug/L

RT: 6.687 min Scan# 1

Delta R.T. -0.100 min

Lab File: VU052556.D

Acq: 27 Dec 2022 11:59

Instrument :

MSVOA_U

ClientSampleId :





GBQB5

Tgt Ion: 63 Resp: 8524

Ion Ratio Lower Upper

63 100

112 0.0 3.0 4.6#

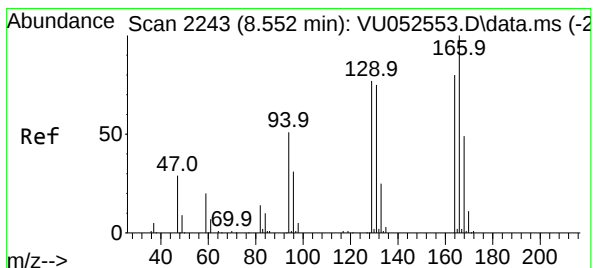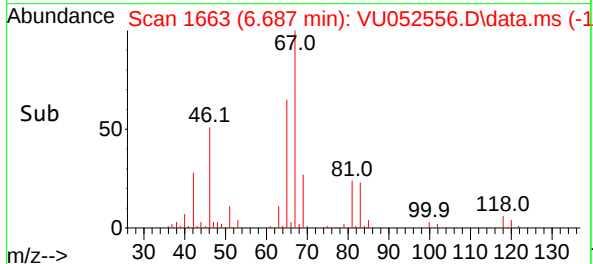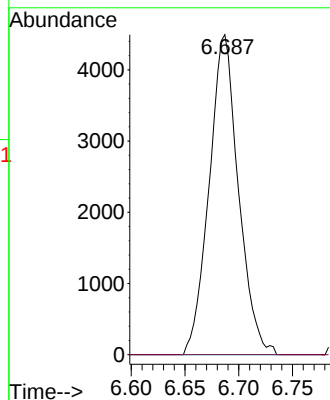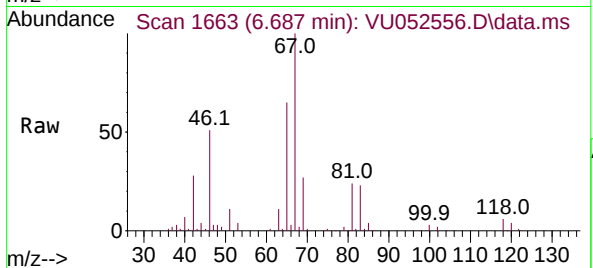

#47

Tetrachloroethene

Concen: 0.144 ug/L

RT: 8.549 min Scan# 2242

Delta R.T. -0.003 min

Lab File: VU052556.D

Acq: 27 Dec 2022 11:59

Tgt Ion: 164 Resp: 1289




Ion Ratio Lower Upper


164 100

129 112.7 68.1 126.5

131 89.1 66.5 123.5

166 146.4 87.9 163.3


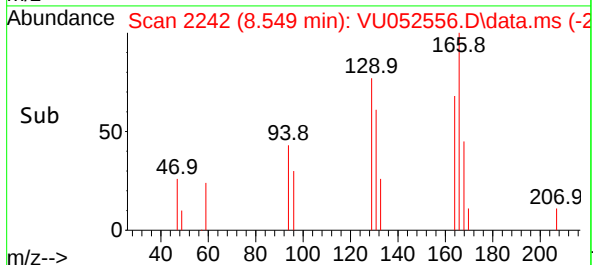
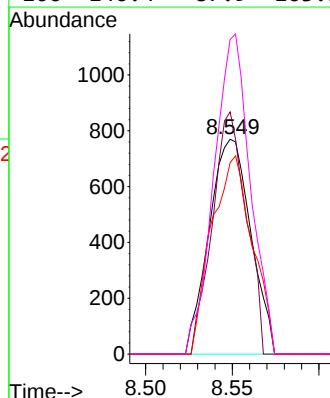
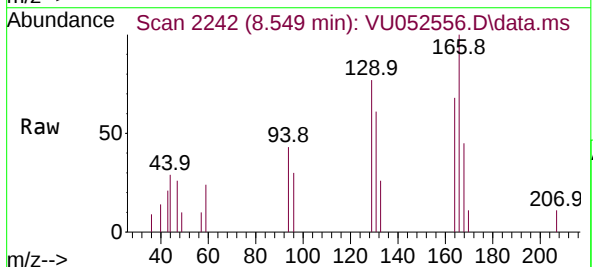


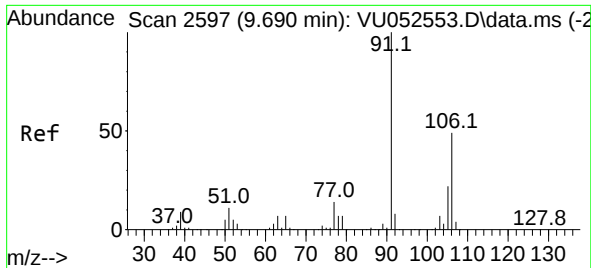

#53
m,p-Xylene
Concen: 0.143 ug/L
RT: 9.690 min Scan# 2597
Delta R.T. 0.000 min
Lab File: VU052556.D
Acq: 27 Dec 2022 11:59




Instrument :
MSVOA_U
ClientSampleId :
GBQB5


Tgt Ion:106 Resp: 2873
Ion Ratio Lower Upper
106 100
91 182.7 148.2 275.2

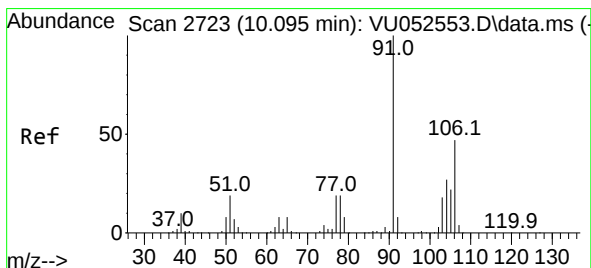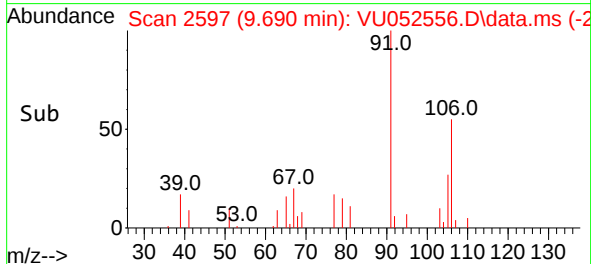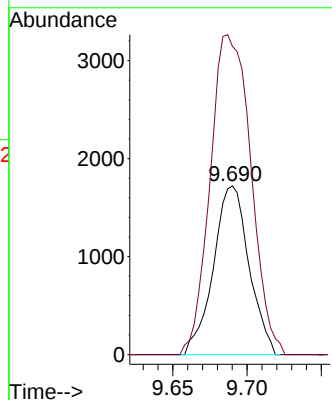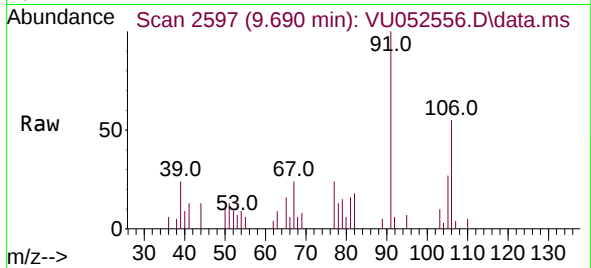

#54
o-Xylene
Concen: 0.178 ug/L
RT: 10.095 min Scan# 2723
Delta R.T. 0.000 min
Lab File: VU052556.D
Acq: 27 Dec 2022 11:59

Tgt Ion:106 Resp: 3429
Ion Ratio Lower Upper
106 100
91 234.5 153.2 284.4

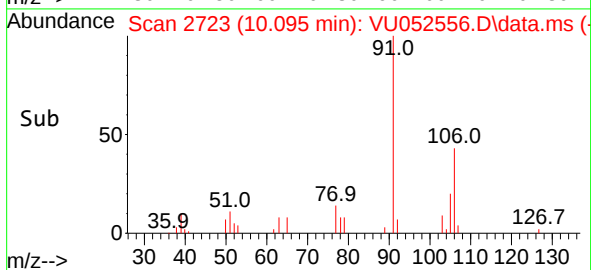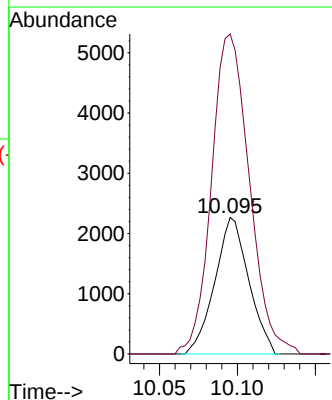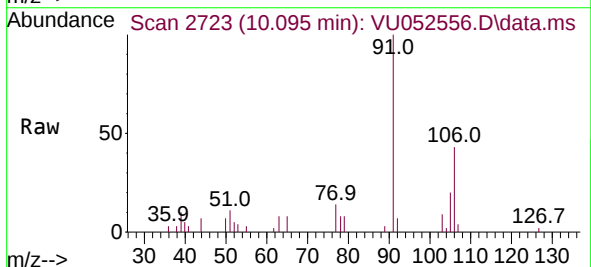

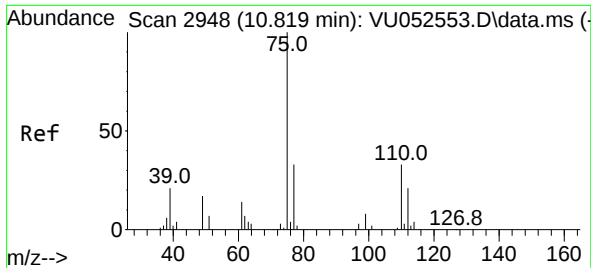

#61

1,2,3-Trichloropropane

Concen: 0.975 ug/L

RT: 11.806 min Scan# 31

Delta R.T. 0.987 min

Lab File: VU052556.D


Acq: 27 Dec 2022 11:59

Instrument :

MSVOA_U

ClientSampleId :

GBQB5

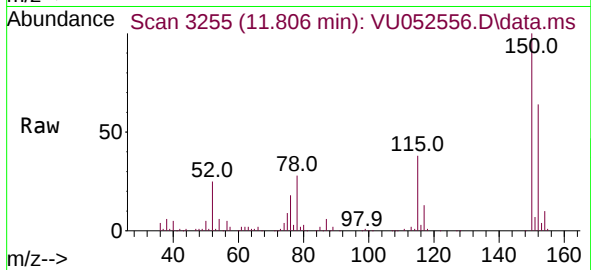

Tgt Ion: 75 Resp: 9468

Ion Ratio Lower Upper

75 100

110 0.0 27.9 41.9#

77 32.5 25.9 38.9

