

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122722\
 Data File : VU052554.D
 Acq On : 27 Dec 2022 11:08
 Operator : JC/MD
 Sample : VU1227WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK166

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	91	rVB	82542	93348	9.26%	1.514%
2	1.916	170	179	192	rBV	82199	110345	10.95%	1.789%
3	2.568	371	382	397	rVB	138799	233158	23.13%	3.781%
4	3.047	519	531	543	rVB2	13227	24977	2.48%	0.405%
5	4.642	1011	1027	1071	rBV	123242	450867	44.72%	7.311%
6	5.060	1141	1157	1178	rVB	142607	315399	31.29%	5.114%
7	5.723	1341	1363	1395	rBV2	281171	761814	75.57%	12.353%
8	6.247	1512	1526	1543	rBV	200628	381625	37.86%	6.188%
9	6.533	1605	1615	1633	rVB10	4970	10884	1.08%	0.176%
10	6.687	1648	1663	1679	rBV	191327	376926	37.39%	6.112%
11	7.562	1919	1935	1956	rBV	75394	137322	13.62%	2.227%
12	7.896	2025	2039	2054	rBV	297028	517987	51.38%	8.400%
13	8.176	2115	2126	2144	rBV	50501	87667	8.70%	1.422%
14	8.632	2254	2268	2308	rBV	526528	1008111	100.00%	16.347%
15	9.414	2498	2511	2535	rBV	292632	492680	48.87%	7.989%
16	10.105	2716	2726	2741	rVB6	6196	13187	1.31%	0.214%
17	10.751	2915	2927	2942	rBV	154240	254491	25.24%	4.127%
18	11.806	3244	3255	3274	rVV	257436	416963	41.36%	6.761%
19	12.189	3362	3374	3395	rBV	295445	479063	47.52%	7.768%




Sum of corrected areas: 6166814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122722\
Data File : VU052554.D
Acq On : 27 Dec 2022 11:08
Operator : JC/MD
Sample : VU1227WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

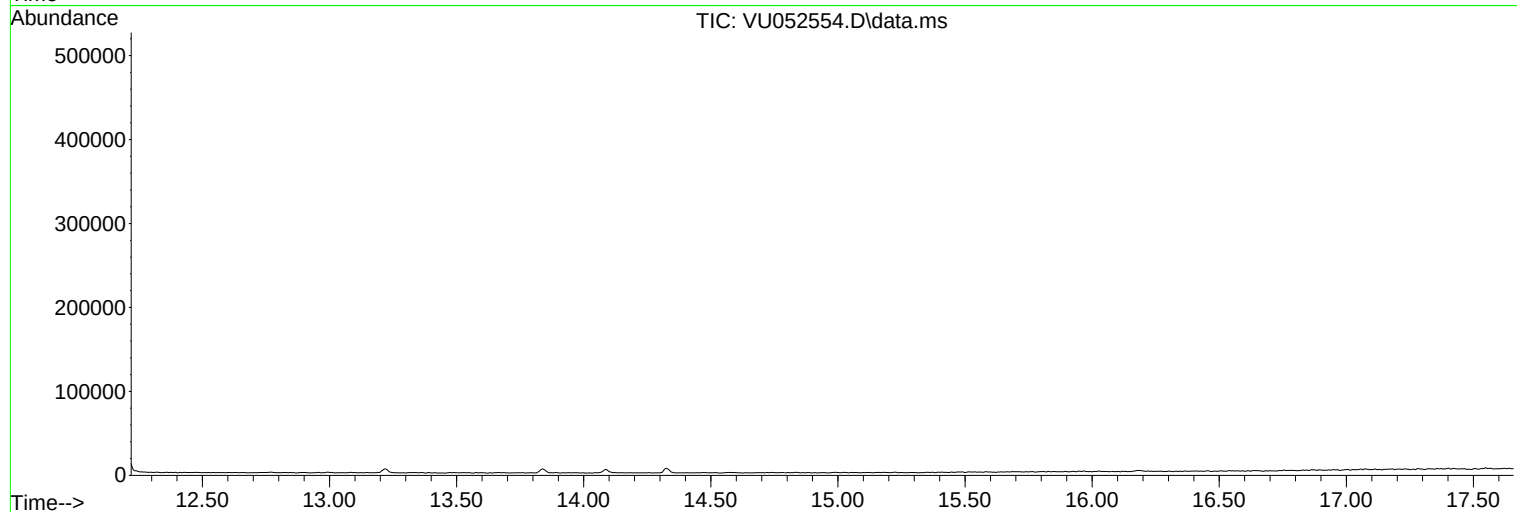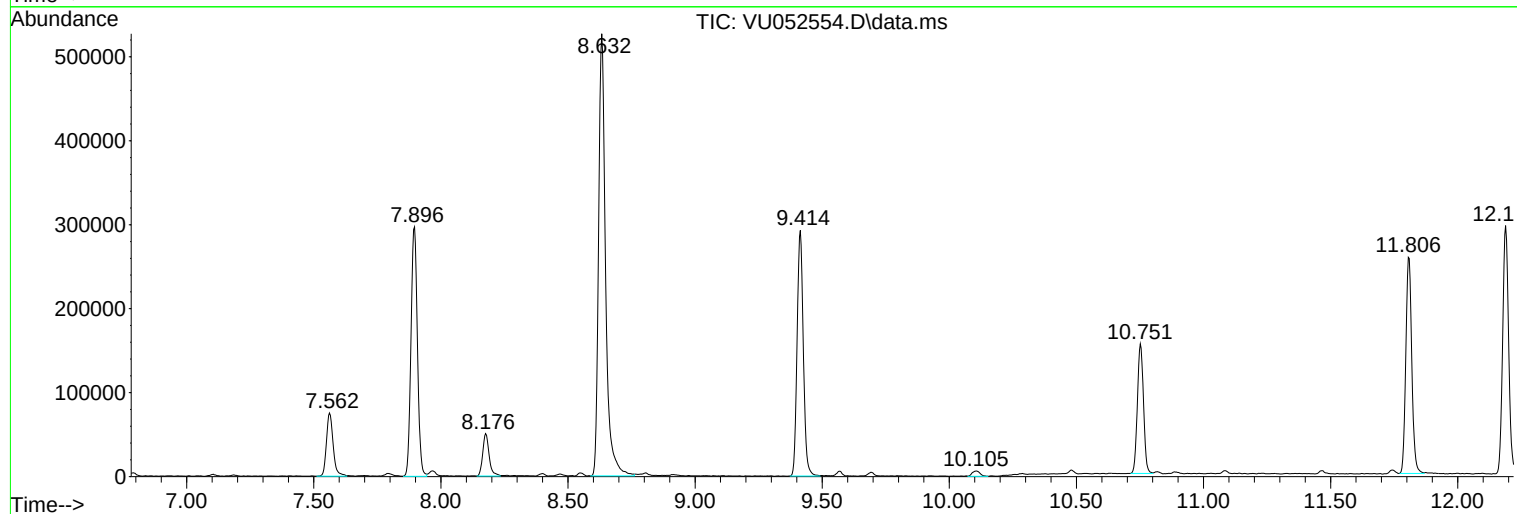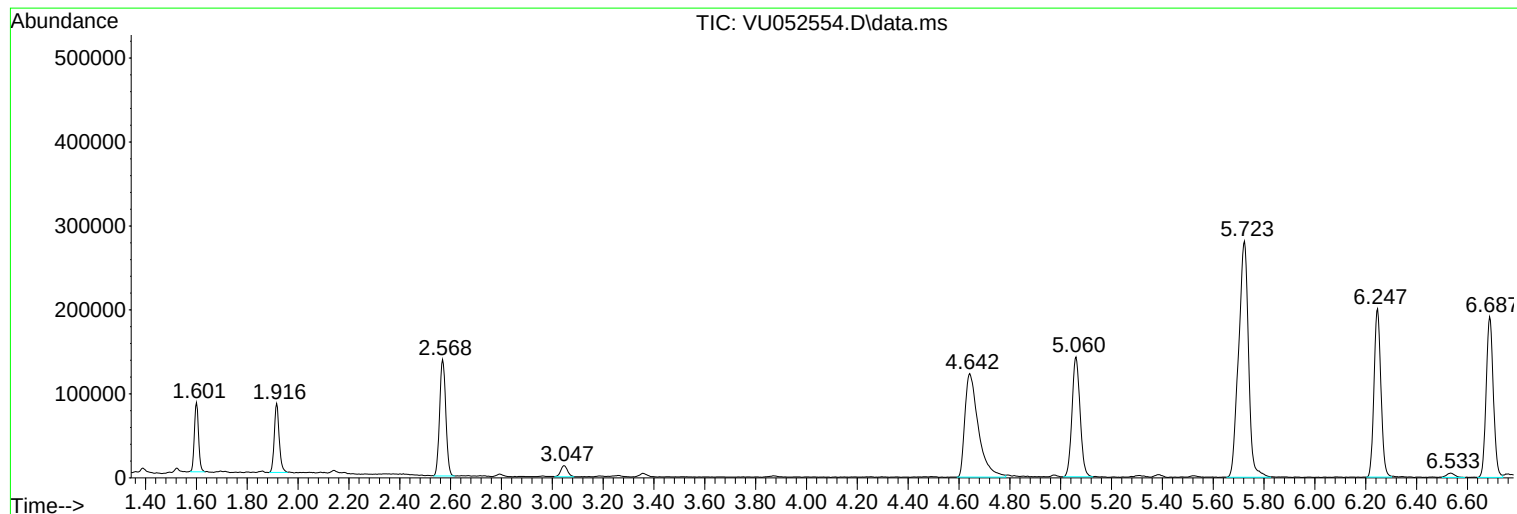

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122722\
Data File : VU052554.D
Acq On : 27 Dec 2022 11:08
Operator : JC/MD
Sample : VU1227WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122722\
Data File : VU052554.D
Acq On : 27 Dec 2022 11:08
Operator : JC/MD
Sample : VU1227WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK166

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc