
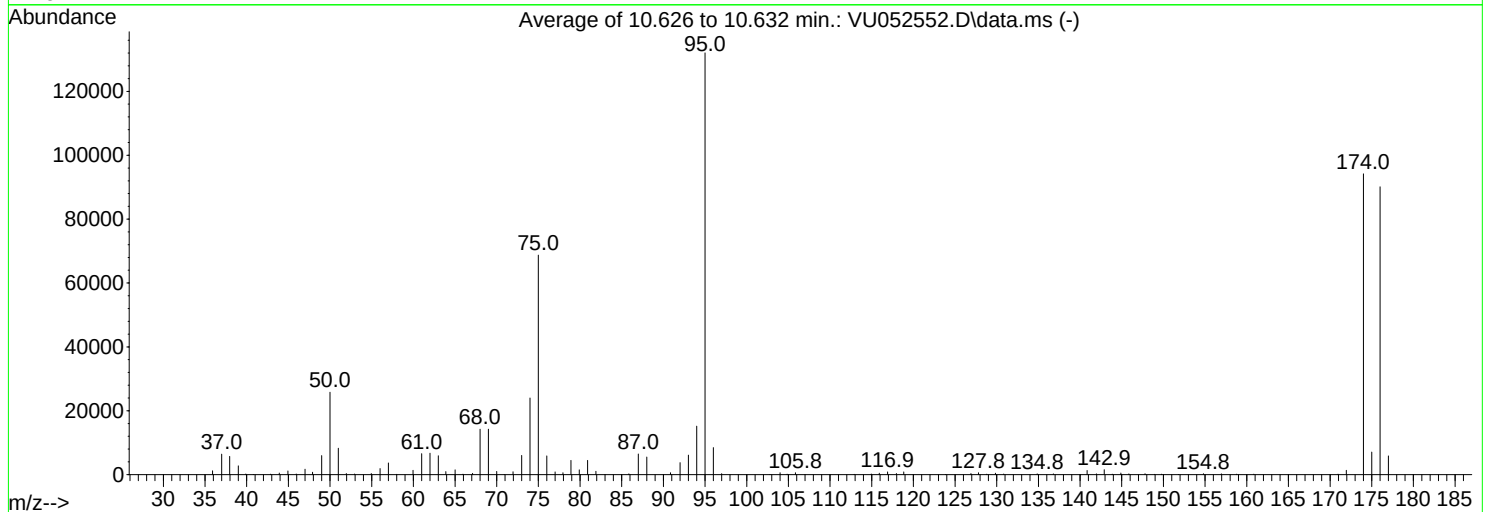


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122722\
 Data File : VU052552.D
 Acq On : 27 Dec 2022 09:49
 Operator : JC/MD
 Sample : BFB185
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB185

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 29 00:24:48 2022

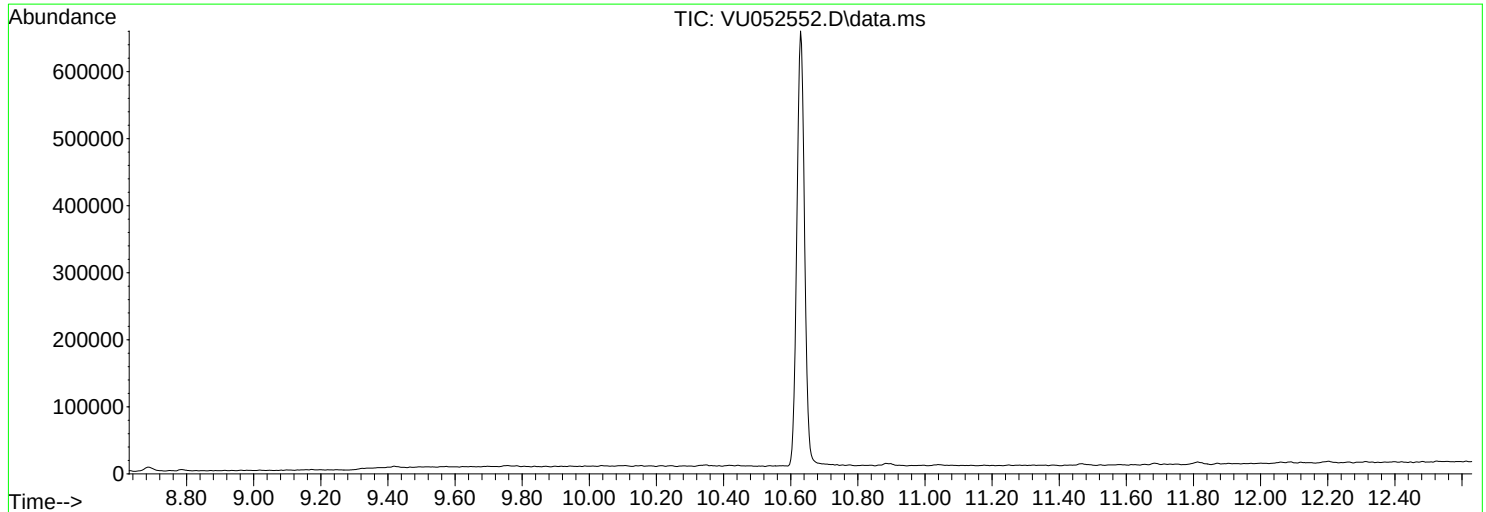

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	25827	PASS
75	95	30	80	52.1	68739	PASS
95	95	100	100	100.0	132061	PASS
96	95	5	9	6.4	8464	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.3	94200	PASS
175	174	5	9	7.5	7090	PASS
176	174	95	101	95.7	90139	PASS
177	176	5	9	6.5	5858	PASS

m/z	Abundance
35.90	1743.0
37.00	169.0
37.90	754.0
39.90	139.0
43.90	428.0
63.40	453.0
126.90	4040.0
127.80	915.0
253.80	3336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
35.90	3036.0
37.00	6521.0
38.00	6178.0
39.00	2706.0
39.90	325.0
42.80	162.0
43.90	923.0
44.90	1168.0
45.90	260.0
47.00	1800.0
47.90	761.0
49.00	5830.0
50.00	25232.0
51.00	8101.0
51.90	379.0
52.90	252.0
54.90	359.0
56.00	1918.0
57.00	3760.0
58.00	184.0
59.90	1368.0
61.00	6477.0
62.00	6673.0
63.00	5931.0
64.00	958.0
65.00	1470.0
65.90	211.0
67.10	371.0
68.00	13407.0
69.00	14169.0
70.00	1060.0
70.90	110.0
71.90	831.0
73.00	5856.0
74.00	23672.0
75.00	66384.0
76.00	5792.0
77.00	782.0
77.90	587.0
78.90	4344.0
79.90	1444.0
80.90	4329.0
81.90	978.0
85.90	224.0
87.00	6340.0
88.00	5116.0
90.90	499.0
92.00	3686.0
93.00	5912.0
94.00	14732.0
95.00	128344.0
96.00	8457.0
97.00	292.0
102.80	126.0
104.00	568.0
104.80	185.0
105.80	607.0
107.00	117.0
115.00	166.0
115.90	428.0
116.90	854.0
117.90	378.0
118.80	840.0
123.90	100.0
126.90	4455.0
127.90	1562.0
128.80	102.0
129.80	485.0
130.80	177.0
134.80	225.0
136.80	270.0
140.80	1246.0
141.90	213.0
142.90	1410.0
143.90	126.0
144.90	496.0
145.80	282.0
147.80	271.0
148.90	117.0
149.80	125.0
151.80	103.0
154.80	280.0
156.90	220.0
158.80	156.0
160.90	162.0
170.90	205.0
171.90	1207.0
174.00	89288.0
175.00	6877.0
176.00	85040.0
177.00	5727.0
253.80	3314.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
35.90	2989.0
37.00	6783.0
38.00	6763.0
39.00	2857.0
40.00	352.0
42.90	135.0
43.90	964.0
45.00	1164.0
45.90	228.0
47.00	1737.0
47.90	791.0
49.00	6234.0
50.00	26632.0
51.00	8587.0
52.00	370.0
52.90	240.0
54.90	343.0
56.00	2036.0
57.00	3747.0
58.00	121.0
59.90	1404.0
61.00	6751.0
62.00	7023.0
63.00	6049.0
63.90	952.0
65.00	1556.0
65.90	181.0
67.10	455.0
68.00	14729.0
69.00	14713.0
70.00	1043.0
70.90	100.0
72.00	899.0
73.00	6136.0
74.00	24896.0
75.00	70968.0
76.00	6037.0
77.00	853.0
78.00	615.0
78.90	4577.0
79.90	1564.0
80.90	4617.0
81.90	1086.0
83.00	102.0
85.90	251.0
87.00	6754.0
88.00	5658.0
90.80	649.0
92.00	3955.0
93.00	6368.0
94.00	15632.0
95.00	136064.0
96.00	8692.0
97.00	289.0
104.00	620.0
104.90	152.0
105.80	615.0
112.90	108.0
115.00	203.0
115.90	491.0
116.90	891.0
117.90	327.0
118.90	917.0
123.80	109.0
126.90	4394.0
127.80	1558.0
128.80	141.0
129.80	487.0
130.90	215.0
134.80	231.0
136.80	260.0
140.00	111.0
140.90	1360.0
142.00	267.0
142.90	1573.0
143.80	131.0
144.90	535.0
145.90	255.0
147.80	308.0
149.00	115.0
149.80	143.0
151.80	100.0
154.80	307.0
156.90	244.0
158.80	170.0
160.90	164.0
170.90	178.0
172.00	1358.0
174.00	97096.0
175.00	7378.0
176.00	92968.0
177.00	6090.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

253.80

3220.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185

m/z	Abundance
36.00	2763.0
37.00	6461.0
38.00	6413.0
39.00	2722.0
40.00	348.0
40.80	105.0
42.90	114.0
43.90	920.0
45.00	1125.0
46.00	173.0
47.00	1564.0
47.90	783.0
49.00	5882.0
50.00	25616.0
51.00	8101.0
52.00	333.0
53.00	194.0
55.00	334.0
56.00	1847.0
57.00	3510.0
60.00	1314.0
61.00	6408.0
62.00	6502.0
63.00	5687.0
63.80	936.0
65.00	1519.0
66.00	151.0
67.10	462.0
68.00	14568.0
69.00	13752.0
70.00	939.0
72.00	919.0
73.00	6052.0
74.00	23408.0
75.00	68864.0
76.00	5735.0
77.00	898.0
78.00	588.0
78.90	4510.0
79.90	1500.0
80.90	4514.0
81.90	1100.0
85.80	299.0
87.00	6297.0
88.00	5725.0
90.80	661.0
92.00	3701.0
93.00	6097.0
94.00	15142.0
95.00	131776.0
96.00	8242.0
97.00	276.0
104.00	619.0
104.90	138.0
105.90	611.0
112.90	151.0
114.90	240.0
115.90	459.0
116.90	886.0
118.00	310.0
118.90	839.0
126.90	4267.0
127.90	1506.0
128.80	171.0
129.90	459.0
130.90	207.0
134.90	242.0
136.80	228.0
140.90	1281.0
142.00	287.0
142.90	1693.0
143.80	141.0
144.90	526.0
145.90	248.0
147.80	316.0
149.00	147.0
149.80	143.0
154.80	288.0
157.00	253.0
158.80	154.0
160.80	131.0
171.00	153.0
172.00	1492.0
174.00	96216.0
175.00	7016.0
176.00	92408.0
177.00	5756.0
253.80	3231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB185