




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057302.D
 Acq On : 28 Dec 2023 01:06
 Operator : MD/SY
 Sample : 06021-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Z2

Manual IntegrationsAPPROVED

Quant Time: Dec 28 01:50:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 00:43:53 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

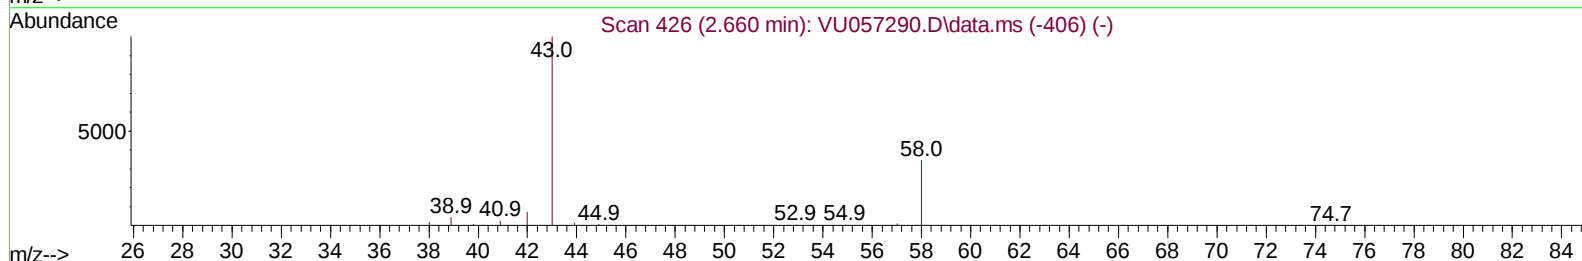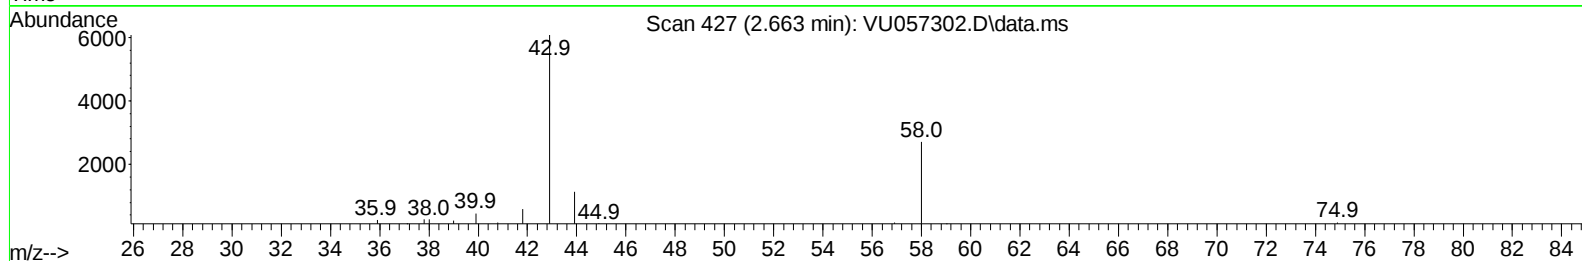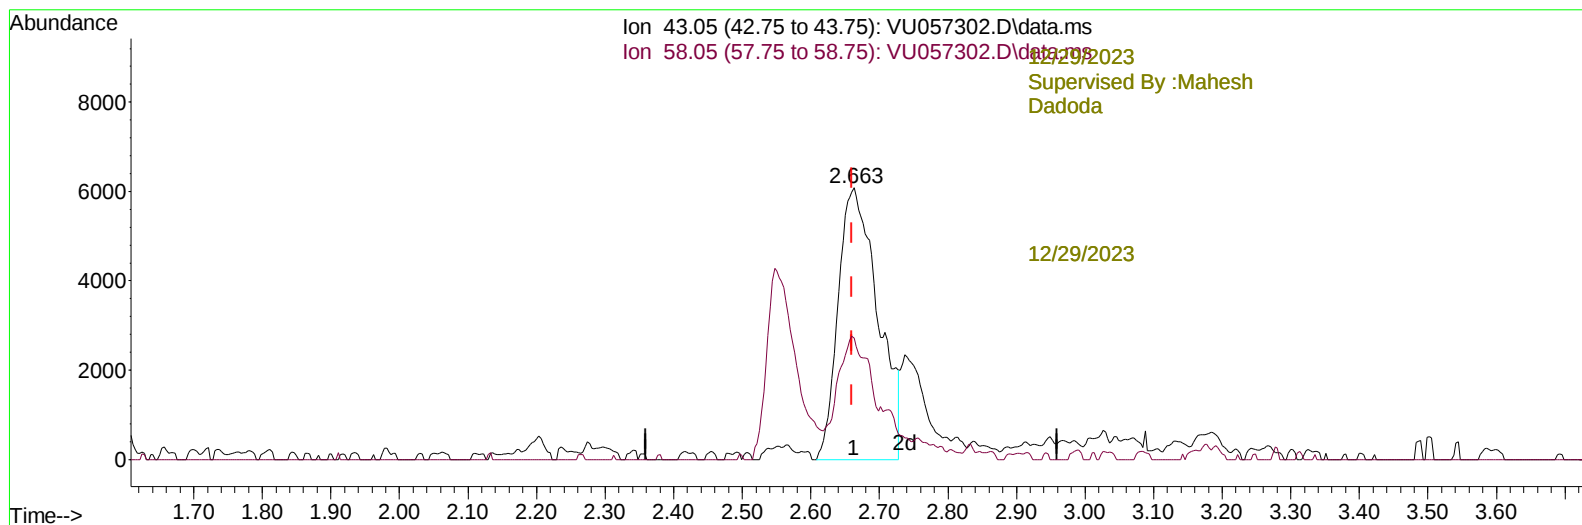

TIC: VU057302.D\data.ms

(13) Acetone (T)

2.663min (+ 0.003) 7.53 ug/L

response 24404

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	26.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057302.D
 Acq On : 28 Dec 2023 01:06
 Operator : MD/SY
 Sample : 06021-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Z2

Manual IntegrationsAPPROVED

Quant Time: Dec 28 01:50:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 00:43:53 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

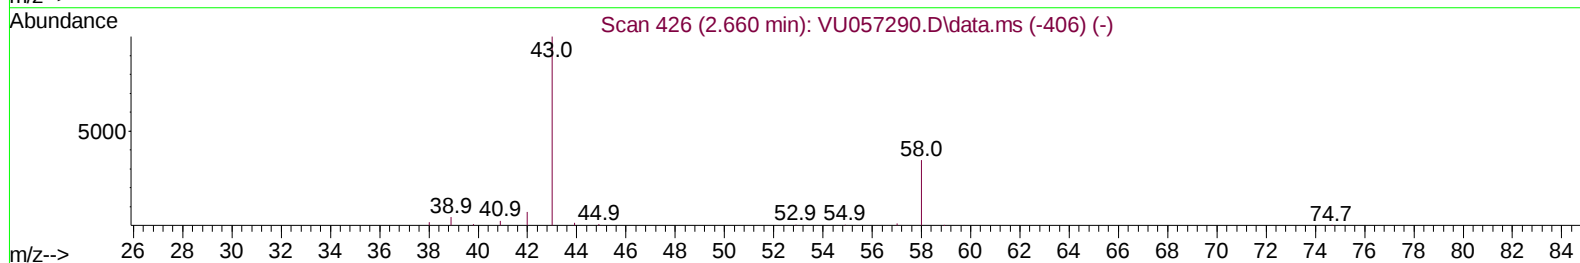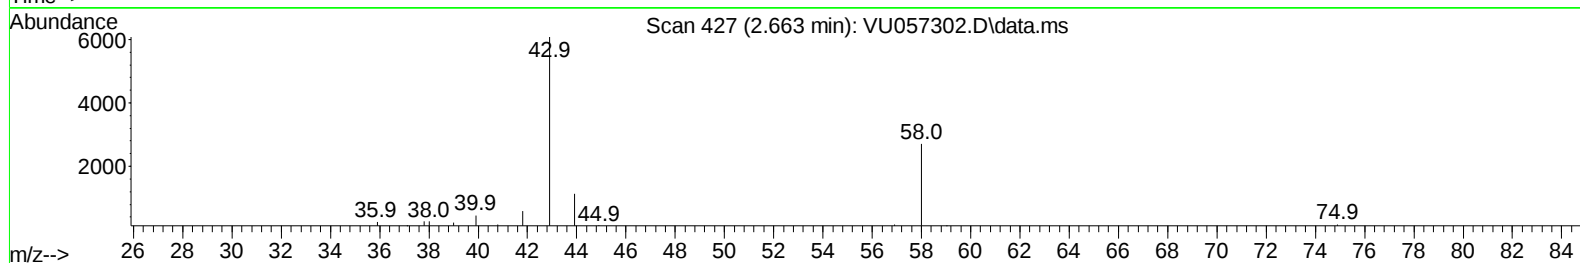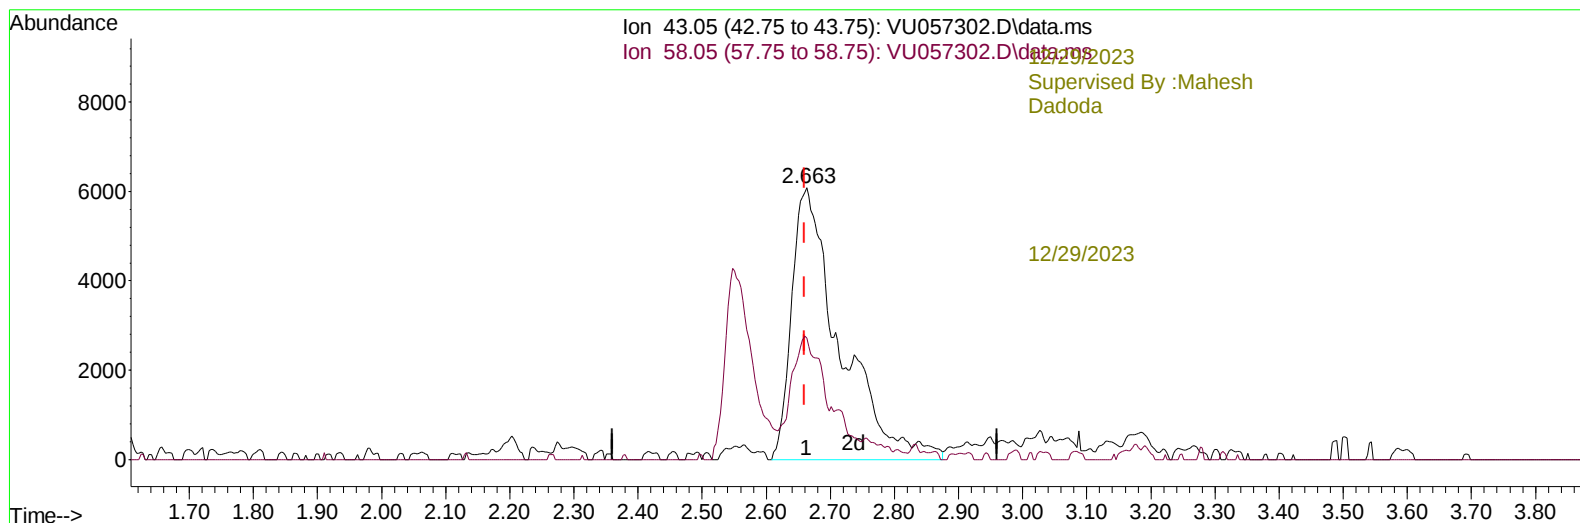

TIC: VU057302.D\data.ms

(13) Acetone (T)

2.663min (+ 0.003) 9.81 ug/L m

response 31780

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	20.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057302.D
 Acq On : 28 Dec 2023 01:06
 Operator : MD/SY
 Sample : 06021-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Z2

Manual IntegrationsAPPROVED

Quant Time: Dec 28 01:50:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 00:43:53 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----12/29/2023							
Supervised By :Mahesh							
Padoda							
Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		255294	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		256858	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		103237	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		115825	5.277	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.600%	
7) Chloroethane-d5	1.911	69		98754	5.602	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.000%	
11) 1,1-Dichloroethene-d2	2.560	65		47447	5.432	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	108.600%	
20) 2-Butanone-d5	4.637	46		287400	57.817	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.640%	
24) Chloroform-d	5.055	84		206763	5.298	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.000%	
26) 1,2-Dichloroethane-d4	5.695	65		109852	5.508	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.200%	
32) Benzene-d6	5.721	84		386730	5.282	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.600%	
36) 1,2-Dichloropropane-d6	6.682	67		129846	5.659	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.200%	
41) Toluene-d8	7.891	98		314720	4.982	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%	
43) trans-1,3-Dichloroprop...	8.174	79		48365	5.254	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.000%	
46) 2-Hexanone-d5	8.631	63		234101	56.145	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.280%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		103614	5.377	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152		111279	5.920	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.400%	
Target Compounds							
						Qvalue	
5) Vinyl chloride	1.602	62		126095	5.917	ug/L	97
12) 1,1-Dichloroethene	2.573	96		7072	0.424	ug/L #	1
13) Acetone	2.663	43		31780m	9.809	ug/L	
14) Carbon disulfide	2.789	76		6556	0.138	ug/L	97
18) trans-1,2-Dichloroethene	3.351	96		2246	0.136	ug/L	78
19) 1,1-Dichloroethane	3.862	63		64773	1.862	ug/L	96
22) cis-1,2-Dichloroethene	4.657	96		122556	6.404	ug/L	97
29) 1,1,1-Trichloroethane	5.309	97		259762	7.985	ug/L	100
34) Trichloroethene	6.534	95		1111009	56.344	ug/L	97
42) Toluene	7.968	91		21813	0.274	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057302.D
Acq On : 28 Dec 2023 01:06
Operator : MD/SY
Sample : 06021-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Z2

Manual IntegrationsAPPROVED

Quant Time: Dec 28 01:50:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 00:43:53 2023
Response via : Initial Calibration

Reviewed By :John
Carlone

