

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057291.D
 Acq On : 27 Dec 2023 20:15
 Operator : MD/SY
 Sample : VU1227WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK123

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	109	rVB	166414	194148	16.30%	2.188%
2	1.911	184	193	214	rVB	128361	181973	15.28%	2.051%
3	2.563	383	396	412	rBV	250224	410593	34.48%	4.627%
4	3.039	534	544	561	rVB3	9564	20066	1.68%	0.226%
5	3.174	574	586	603	rBV3	8306	18861	1.58%	0.213%
6	4.637	1029	1041	1088	rBV	120303	468191	39.31%	5.276%
7	5.055	1153	1171	1204	rVB	214814	488366	41.01%	5.503%
8	5.718	1353	1377	1405	rBV2	412145	1090809	91.59%	12.292%
9	6.242	1525	1540	1573	rBV	321458	636740	53.46%	7.175%
10	6.685	1663	1678	1702	rBV	252680	514582	43.21%	5.799%
11	7.560	1934	1950	1975	rBV	125303	232343	19.51%	2.618%
12	7.891	2040	2053	2077	rBV	460773	821925	69.01%	9.262%
13	8.174	2131	2141	2161	rBV	78468	143571	12.05%	1.618%
14	8.631	2271	2283	2316	rBV	590431	1190982	100.00%	13.420%
15	9.412	2513	2526	2559	rBV	457332	788947	66.24%	8.890%
16	10.749	2930	2942	2958	rBV	200691	325028	27.29%	3.663%
17	11.807	3259	3271	3289	rBV	389604	639269	53.68%	7.204%
18	12.187	3373	3389	3420	rBV	397179	678652	56.98%	7.647%
19	13.843	3896	3904	3922	rVB5	8991	15638	1.31%	0.176%
20	14.331	4047	4056	4065	rBV6	7792	13713	1.15%	0.155%




Sum of corrected areas: 8874397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057291.D
Acq On : 27 Dec 2023 20:15
Operator : MD/SY
Sample : VU1227WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

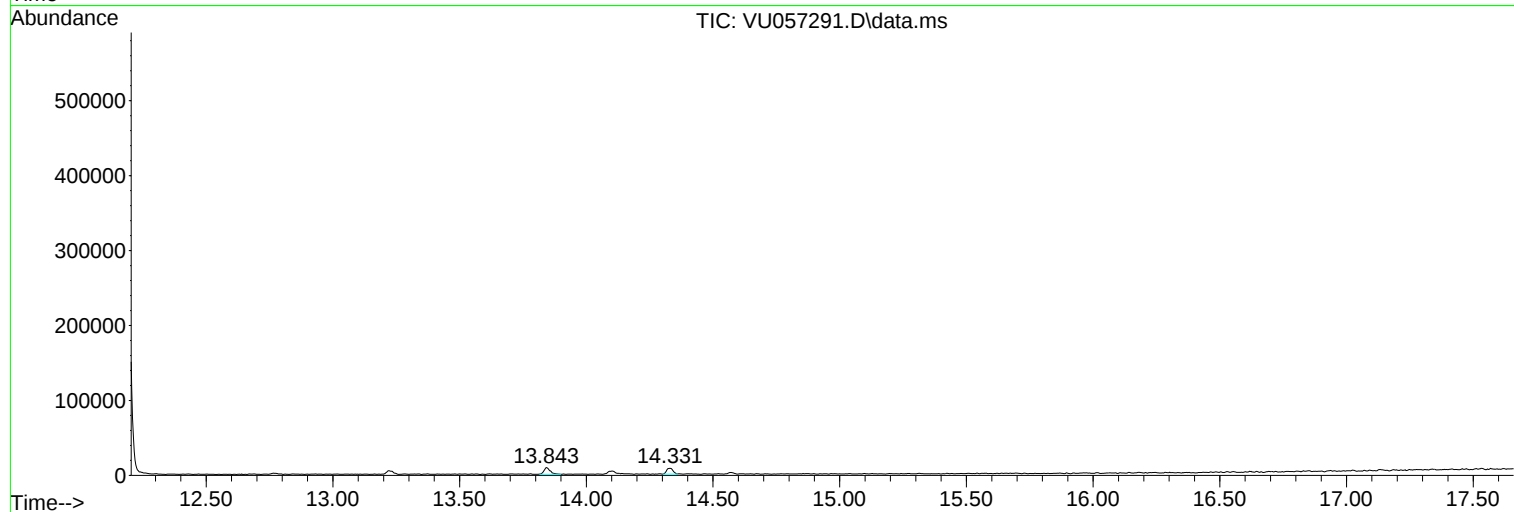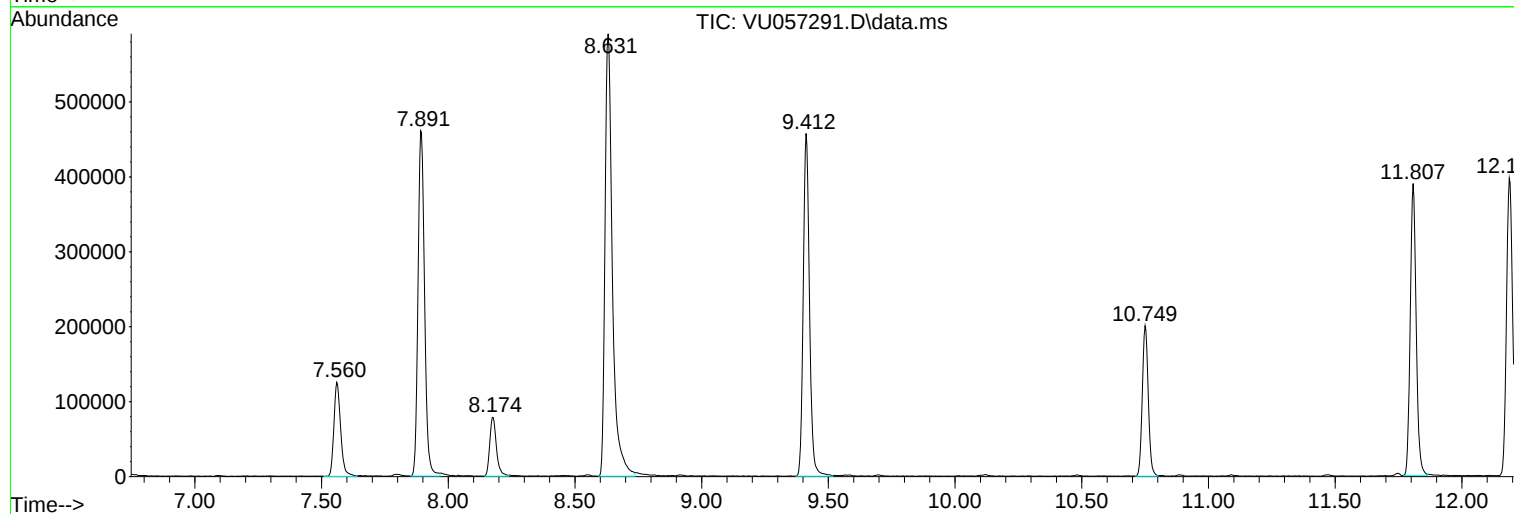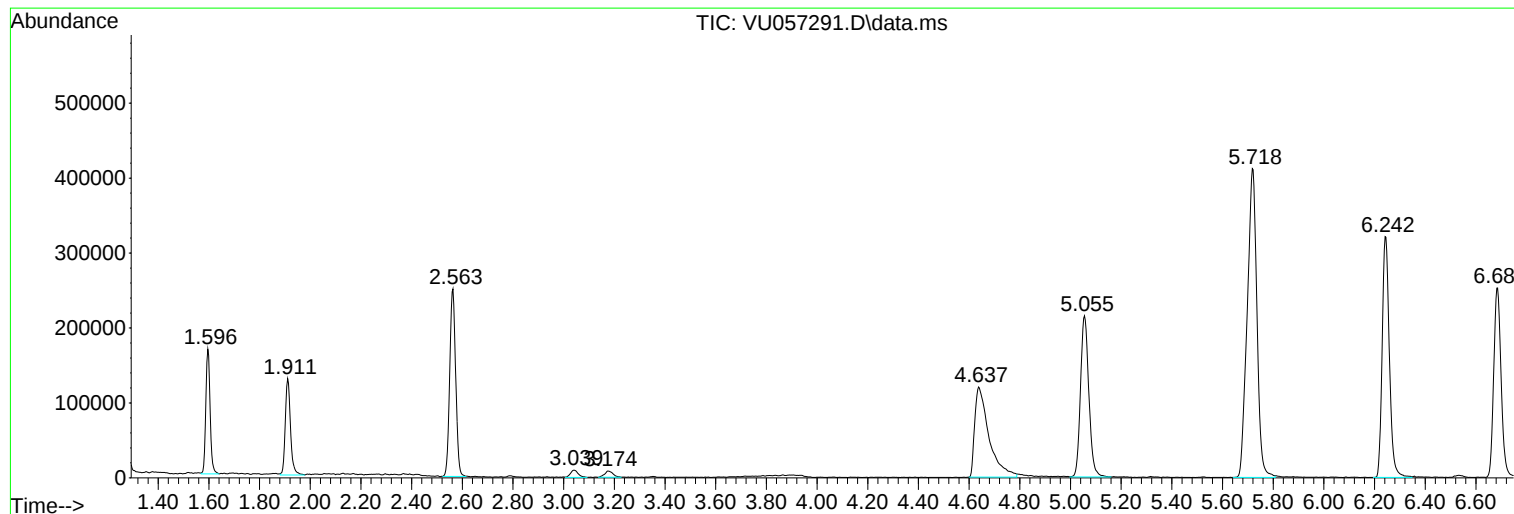

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057291.D
Acq On : 27 Dec 2023 20:15
Operator : MD/SY
Sample : VU1227WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057291.D
Acq On : 27 Dec 2023 20:15
Operator : MD/SY
Sample : VU1227WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc