

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057296.D
 Acq On : 27 Dec 2023 22:41
 Operator : MD/SY
 Sample : 05979-14DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGR44DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	107	rBV	154834	179598	15.36%	2.020%
2	1.911	184	193	215	rVB	120413	168556	14.42%	1.896%
3	2.560	382	395	411	rBV	227280	373211	31.92%	4.198%
4	3.039	533	544	566	rVB2	13560	26711	2.28%	0.300%
5	3.177	572	587	607	rBV	14726	34858	2.98%	0.392%
6	4.644	1027	1043	1087	rBV2	113708	464077	39.69%	5.220%
7	5.055	1154	1171	1196	rBV	195544	448911	38.40%	5.049%
8	5.718	1356	1377	1400	rBV2	379895	1006152	86.06%	11.317%
9	6.242	1527	1540	1568	rBV2	303946	609570	52.14%	6.856%
10	6.682	1663	1677	1701	rBV	240132	479058	40.97%	5.388%
11	7.560	1938	1950	1975	rBV	116661	212756	18.20%	2.393%
12	7.894	2041	2054	2074	rBV	419232	748045	63.98%	8.414%
13	8.174	2130	2141	2157	rBV	74338	130013	11.12%	1.462%
14	8.547	2244	2257	2272	rBV	321093	550372	47.07%	6.191%
15	8.631	2272	2283	2315	rBV	586879	1169188	100.00%	13.151%
16	9.412	2514	2526	2545	rBV	442106	745579	63.77%	8.386%
17	10.749	2925	2942	2966	rBV	186563	313438	26.81%	3.526%
18	11.807	3258	3271	3293	rBV	374844	605344	51.77%	6.809%
19	12.187	3376	3389	3414	rBV	373386	625094	53.46%	7.031%




Sum of corrected areas: 8890531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057296.D
Acq On : 27 Dec 2023 22:41
Operator : MD/SY
Sample : 05979-14DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

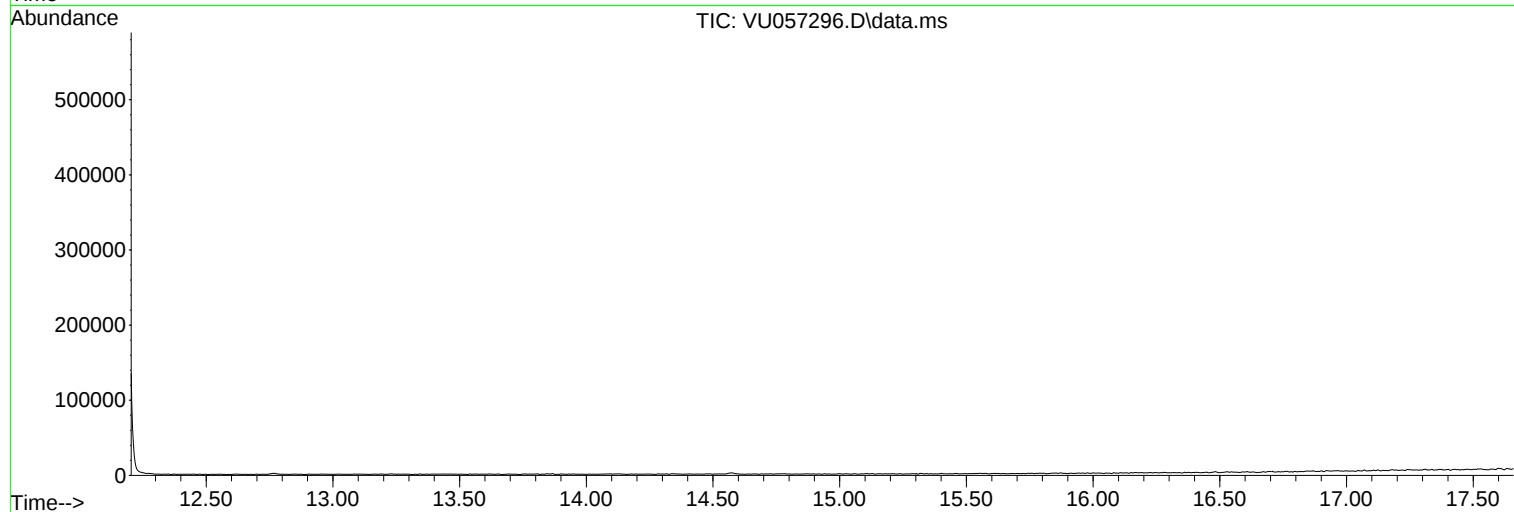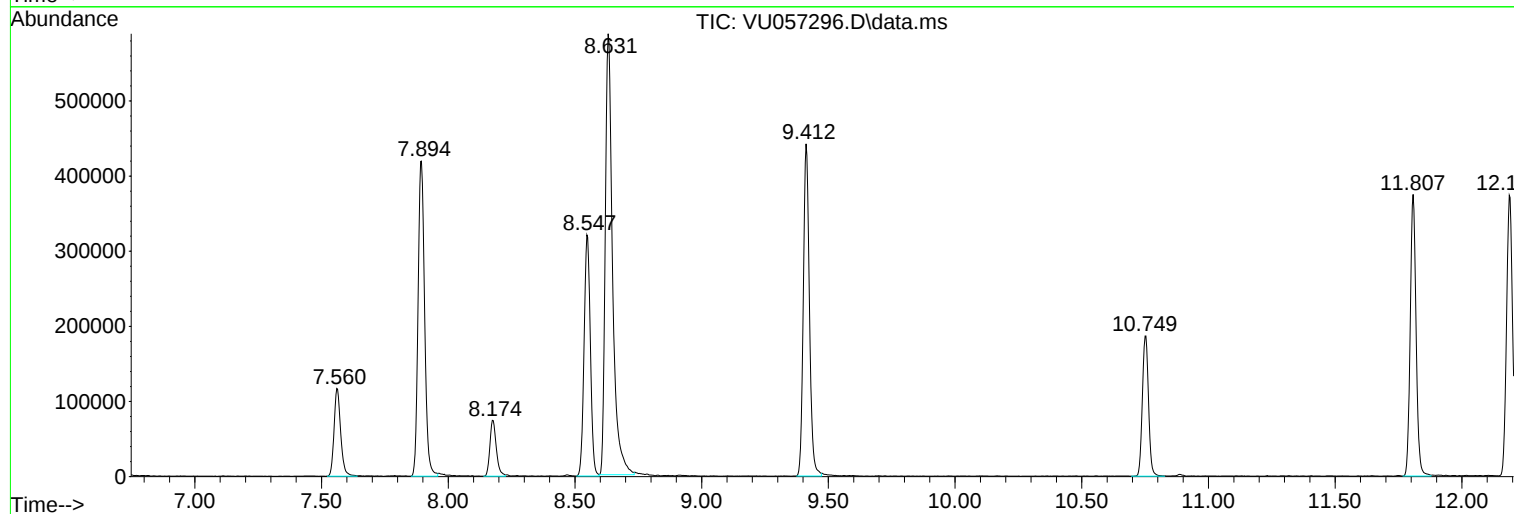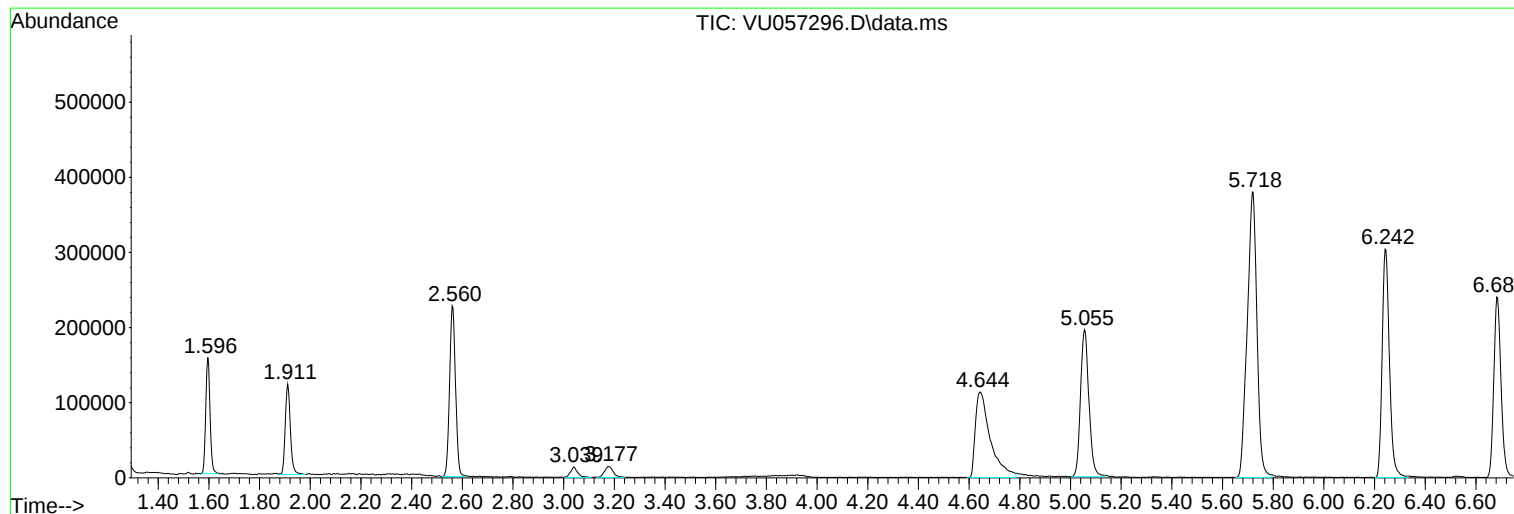

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057296.D
Acq On : 27 Dec 2023 22:41
Operator : MD/SY
Sample : 05979-14DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057296.D
Acq On : 27 Dec 2023 22:41
Operator : MD/SY
Sample : 05979-14DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------