

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057307.D
 Acq On : 28 Dec 2023 03:07
 Operator : MD/SY
 Sample : 06020-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH3P0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rVB	153633	175074	14.31%	2.013%
2	1.911	184	193	210	rVB	124903	170272	13.92%	1.958%
3	2.560	383	395	415	rVB	234620	382081	31.23%	4.393%
4	2.789	455	466	481	rVB	7703	14078	1.15%	0.162%
5	3.174	576	586	601	rVB2	7619	19030	1.56%	0.219%
6	4.644	1029	1043	1085	rBV	129603	478473	39.11%	5.501%
7	5.055	1155	1171	1195	rBV	211512	497033	40.63%	5.714%
8	5.718	1357	1377	1400	rBV3	388541	1035348	84.64%	11.903%
9	6.242	1528	1540	1562	rBV	318670	622187	50.86%	7.153%
10	6.685	1664	1678	1703	rBV	253078	496263	40.57%	5.705%
11	7.560	1938	1950	1969	rBV2	116924	212465	17.37%	2.443%
12	7.891	2041	2053	2071	rBV	429174	762774	62.35%	8.769%
13	8.174	2130	2141	2160	rBV	76157	134108	10.96%	1.542%
14	8.631	2272	2283	2320	rBV	608458	1223304	100.00%	14.064%
15	9.412	2513	2526	2545	rBV	453756	773024	63.19%	8.887%
16	10.750	2929	2942	2962	rBV	199762	331061	27.06%	3.806%
17	11.807	3259	3271	3295	rBV	388236	641899	52.47%	7.380%
18	12.061	3337	3350	3374	rBV4	22822	59512	4.86%	0.684%
19	12.187	3377	3389	3405	rVV	412364	670373	54.80%	7.707%




Sum of corrected areas: 8698359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057307.D
Acq On : 28 Dec 2023 03:07
Operator : MD/SY
Sample : 06020-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

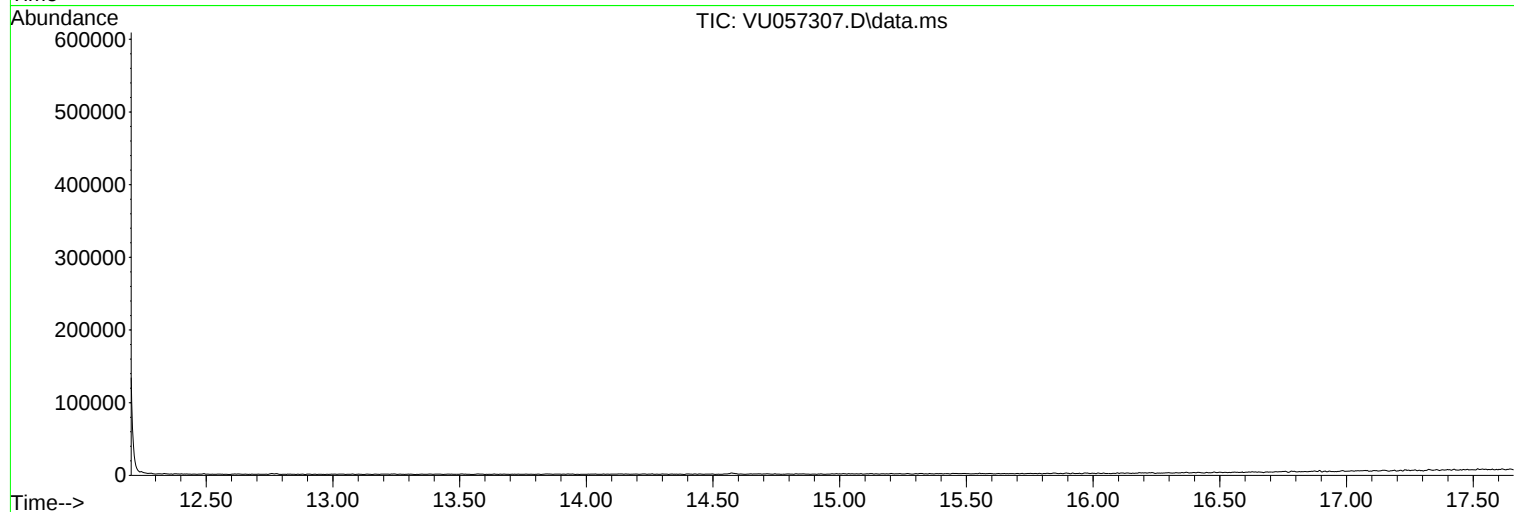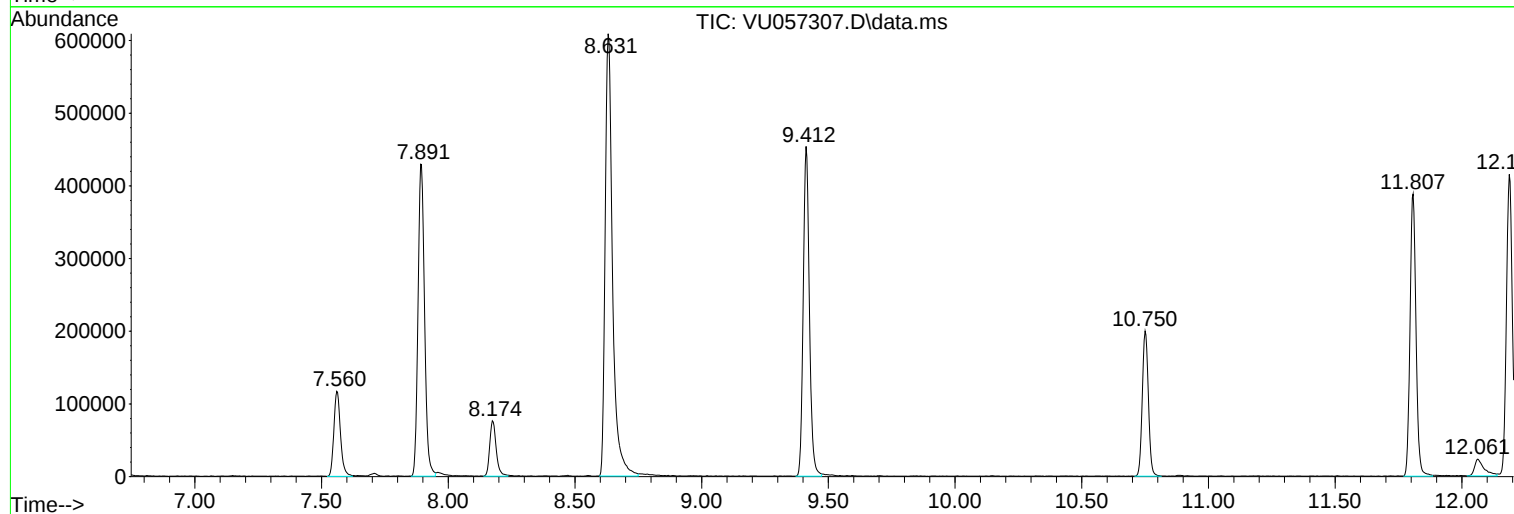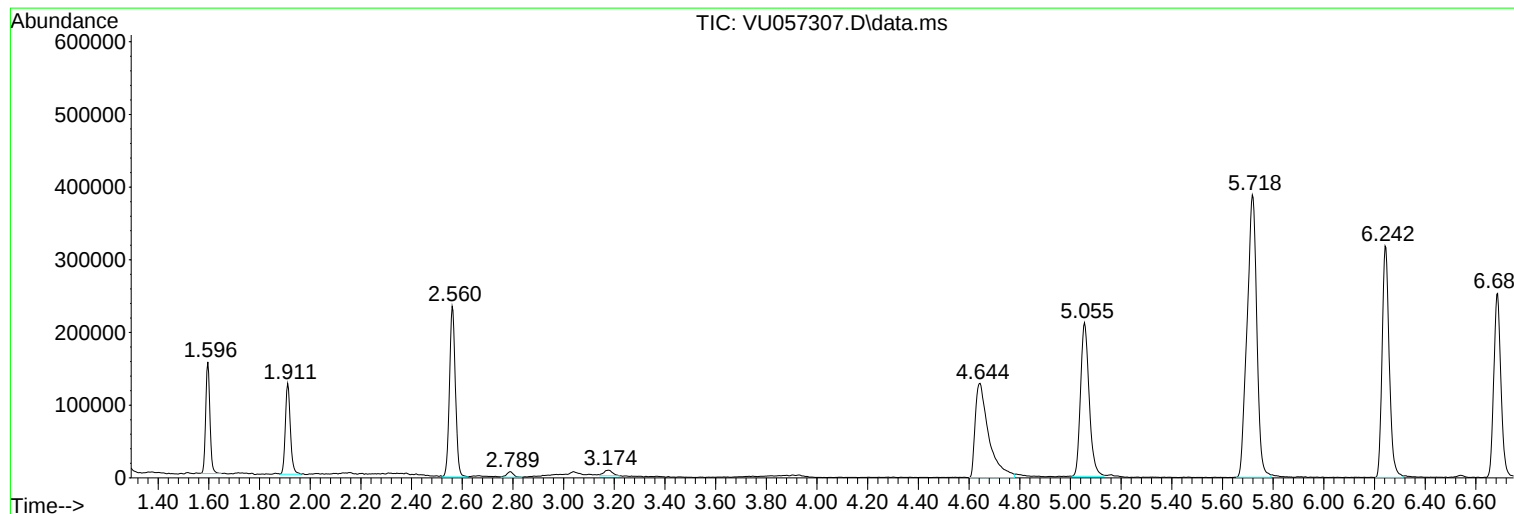

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057307.D
Acq On : 28 Dec 2023 03:07
Operator : MD/SY
Sample : 06020-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057307.D
Acq On : 28 Dec 2023 03:07
Operator : MD/SY
Sample : 06020-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------