

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057314.D
 Acq On : 28 Dec 2023 06:21
 Operator : MD/SY
 Sample : VU1227WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK124

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU057314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	110	rBV	163264	189629	15.63%	2.170%
2	1.769	143	149	160	rVB2	10396	13007	1.07%	0.149%
3	1.910	183	193	212	rBV	127999	178716	14.73%	2.045%
4	2.560	383	395	413	rBV	238608	388077	31.99%	4.441%
5	3.180	575	588	599	rVB2	8814	18105	1.49%	0.207%
6	4.640	1024	1042	1092	rBV2	131874	487956	40.22%	5.584%
7	5.055	1156	1171	1208	rBV	230690	566002	46.66%	6.477%
8	5.717	1356	1377	1396	rBV2	397655	1047868	86.38%	11.991%
9	6.241	1527	1540	1565	rBV	304374	596556	49.17%	6.827%
10	6.685	1662	1678	1705	rBV	249955	498577	41.10%	5.705%
11	7.563	1939	1951	1970	rBV	115664	213217	17.58%	2.440%
12	7.708	1980	1996	2009	rVB4	12526	23678	1.95%	0.271%
13	7.894	2040	2054	2069	rBV	429328	755871	62.31%	8.650%
14	7.968	2069	2077	2092	rVB2	25139	47168	3.89%	0.540%
15	8.174	2126	2141	2161	rBV2	73385	134251	11.07%	1.536%
16	8.630	2271	2283	2319	rBV	609644	1213141	100.00%	13.883%
17	9.412	2513	2526	2549	rBV	437289	757880	62.47%	8.673%
18	9.688	2605	2612	2627	rVB3	7495	12573	1.04%	0.144%
19	10.749	2928	2942	2961	rBV	204464	332541	27.41%	3.805%
20	11.807	3258	3271	3293	rBV	376769	613744	50.59%	7.023%
21	12.187	3374	3389	3406	rBV	385201	649976	53.58%	7.438%




Sum of corrected areas: 8738533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057314.D
Acq On : 28 Dec 2023 06:21
Operator : MD/SY
Sample : VU1227WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

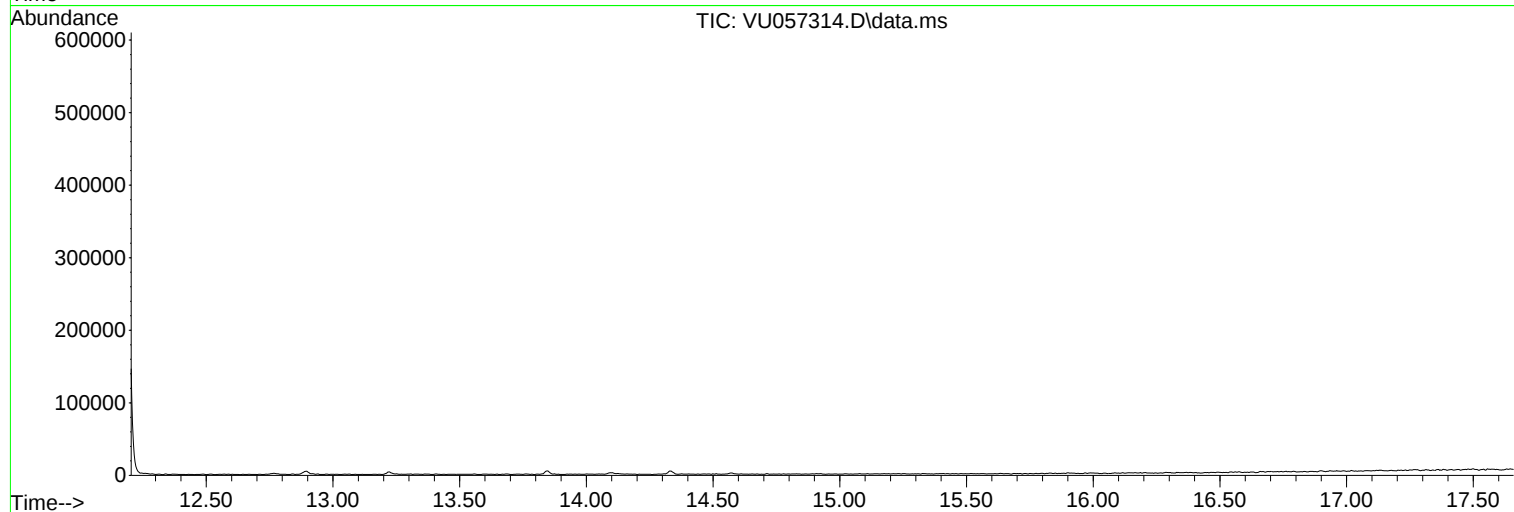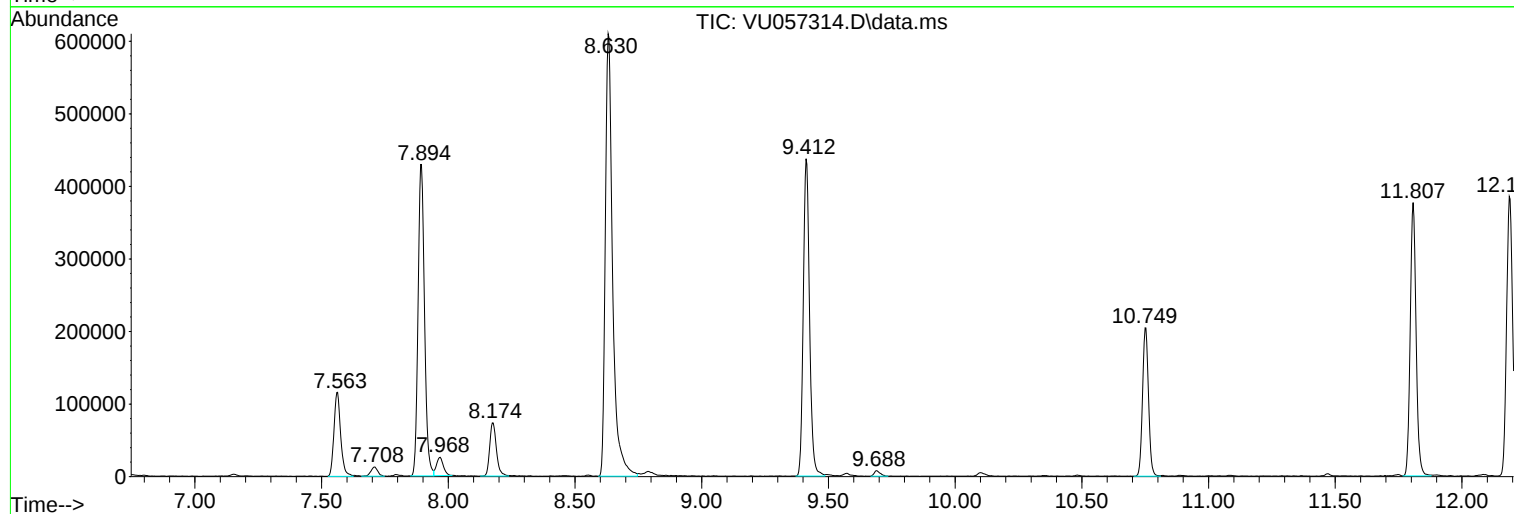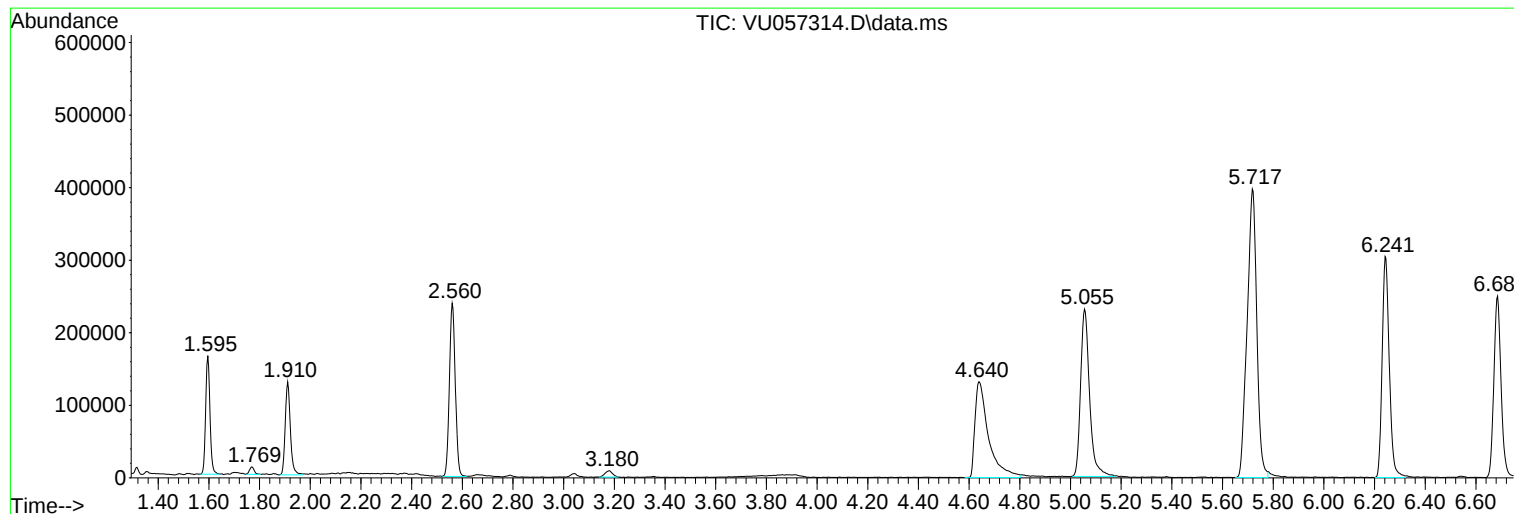

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057314.D
Acq On : 28 Dec 2023 06:21
Operator : MD/SY
Sample : VU1227WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057314.D
Acq On : 28 Dec 2023 06:21
Operator : MD/SY
Sample : VU1227WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------