

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
 Data File : VU057316.D
 Acq On : 28 Dec 2023 07:10
 Operator : MD/SY
 Sample : 06020-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7X7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	109	rVB	152755	175424	14.50%	2.004%
2	1.911	184	193	209	rBV	125466	169983	14.05%	1.942%
3	2.560	384	395	411	rVB	227317	371079	30.68%	4.240%
4	3.174	576	586	603	rVB4	6294	16888	1.40%	0.193%
5	4.641	1028	1042	1091	rBV	134530	492097	40.69%	5.622%
6	5.055	1153	1171	1199	rBV	209834	482748	39.91%	5.515%
7	5.718	1357	1377	1411	rBV2	391773	1039359	85.94%	11.875%
8	6.242	1527	1540	1565	rBV	312450	613017	50.68%	7.004%
9	6.538	1619	1632	1648	rBV3	57339	113170	9.36%	1.293%
10	6.685	1664	1678	1706	rBV	253381	505239	41.77%	5.772%
11	7.560	1935	1950	1972	rBV	118039	212017	17.53%	2.422%
12	7.894	2038	2054	2075	rBV	430522	763813	63.15%	8.726%
13	8.174	2130	2141	2155	rBV2	75740	129541	10.71%	1.480%
14	8.631	2270	2283	2326	rBV	603107	1209467	100.00%	13.818%
15	9.412	2512	2526	2552	rBV	454322	777786	64.31%	8.886%
16	10.750	2930	2942	2966	rBV	198236	324574	26.84%	3.708%
17	11.807	3259	3271	3288	rBV	392672	635923	52.58%	7.265%
18	12.061	3340	3350	3367	rBV2	23200	55650	4.60%	0.636%
19	12.187	3377	3389	3409	rBV	407444	665036	54.99%	7.598%




Sum of corrected areas: 8752811

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057316.D
Acq On : 28 Dec 2023 07:10
Operator : MD/SY
Sample : 06020-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

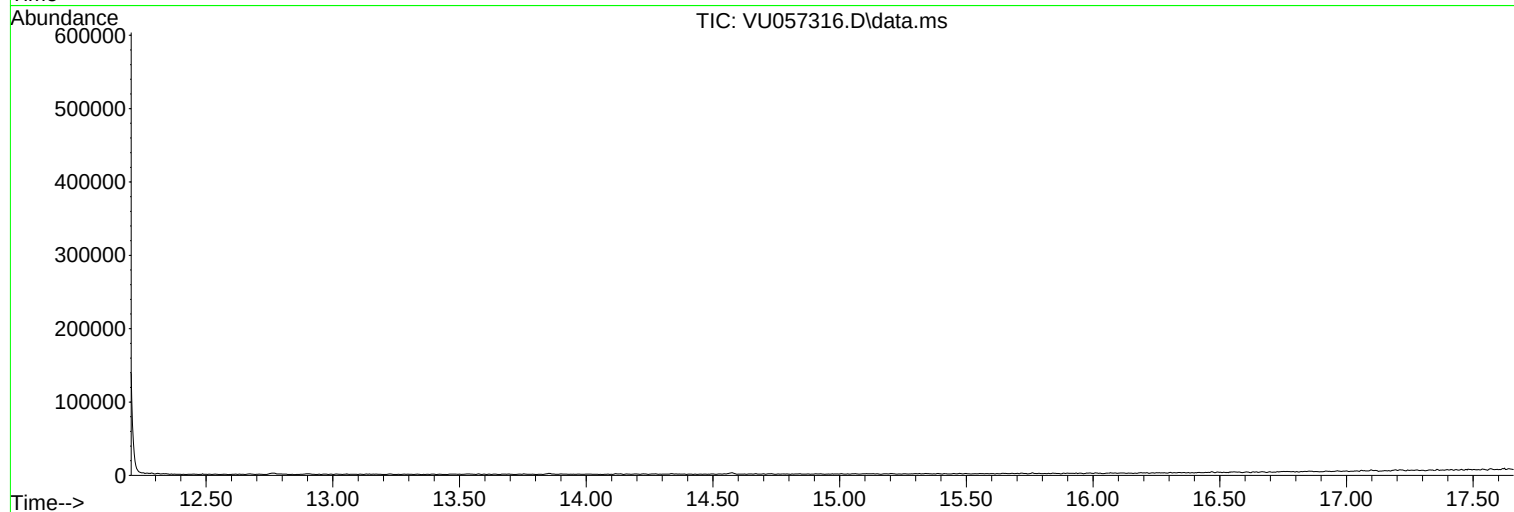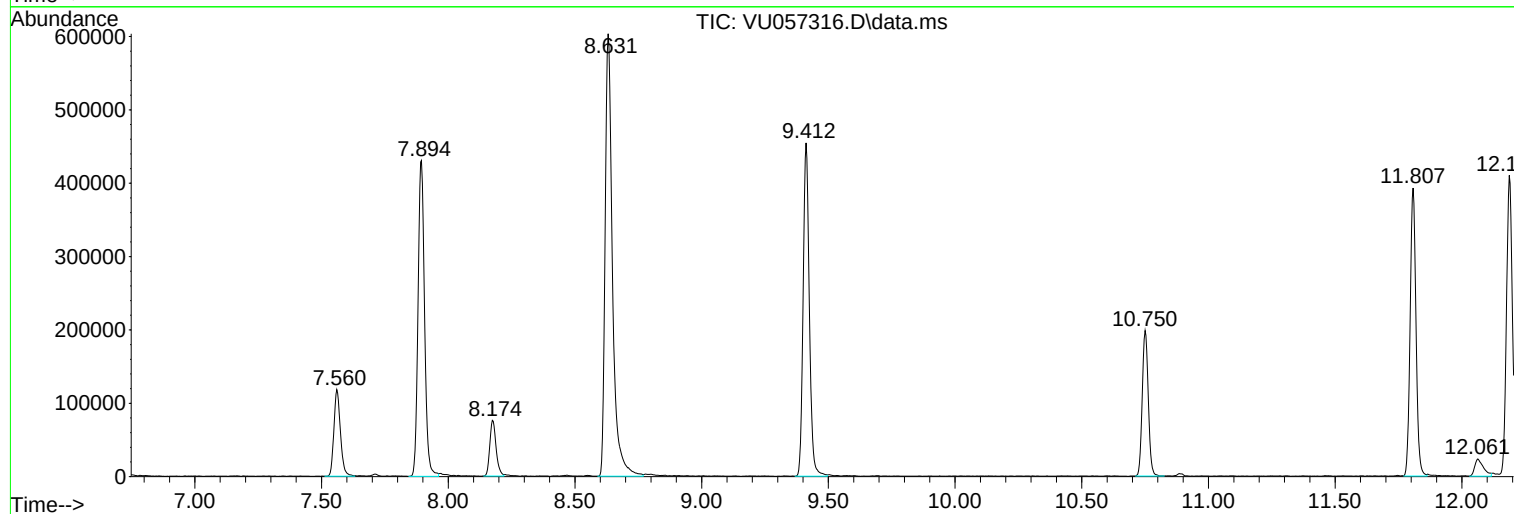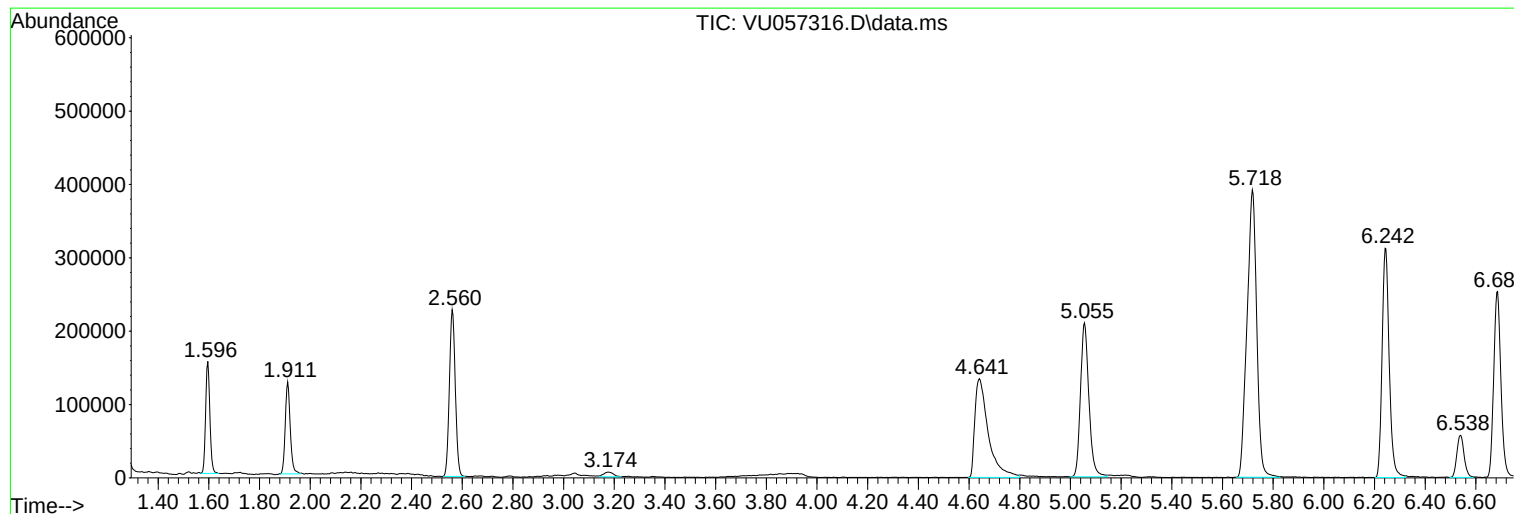

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057316.D
Acq On : 28 Dec 2023 07:10
Operator : MD/SY
Sample : 06020-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057316.D
Acq On : 28 Dec 2023 07:10
Operator : MD/SY
Sample : 06020-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------