


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122723\
Data File : VU057281.D
Acq On : 27 Dec 2023 12:25
Operator : MD/SY
Sample : BFB102
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB102

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 28 21:37:03 2023

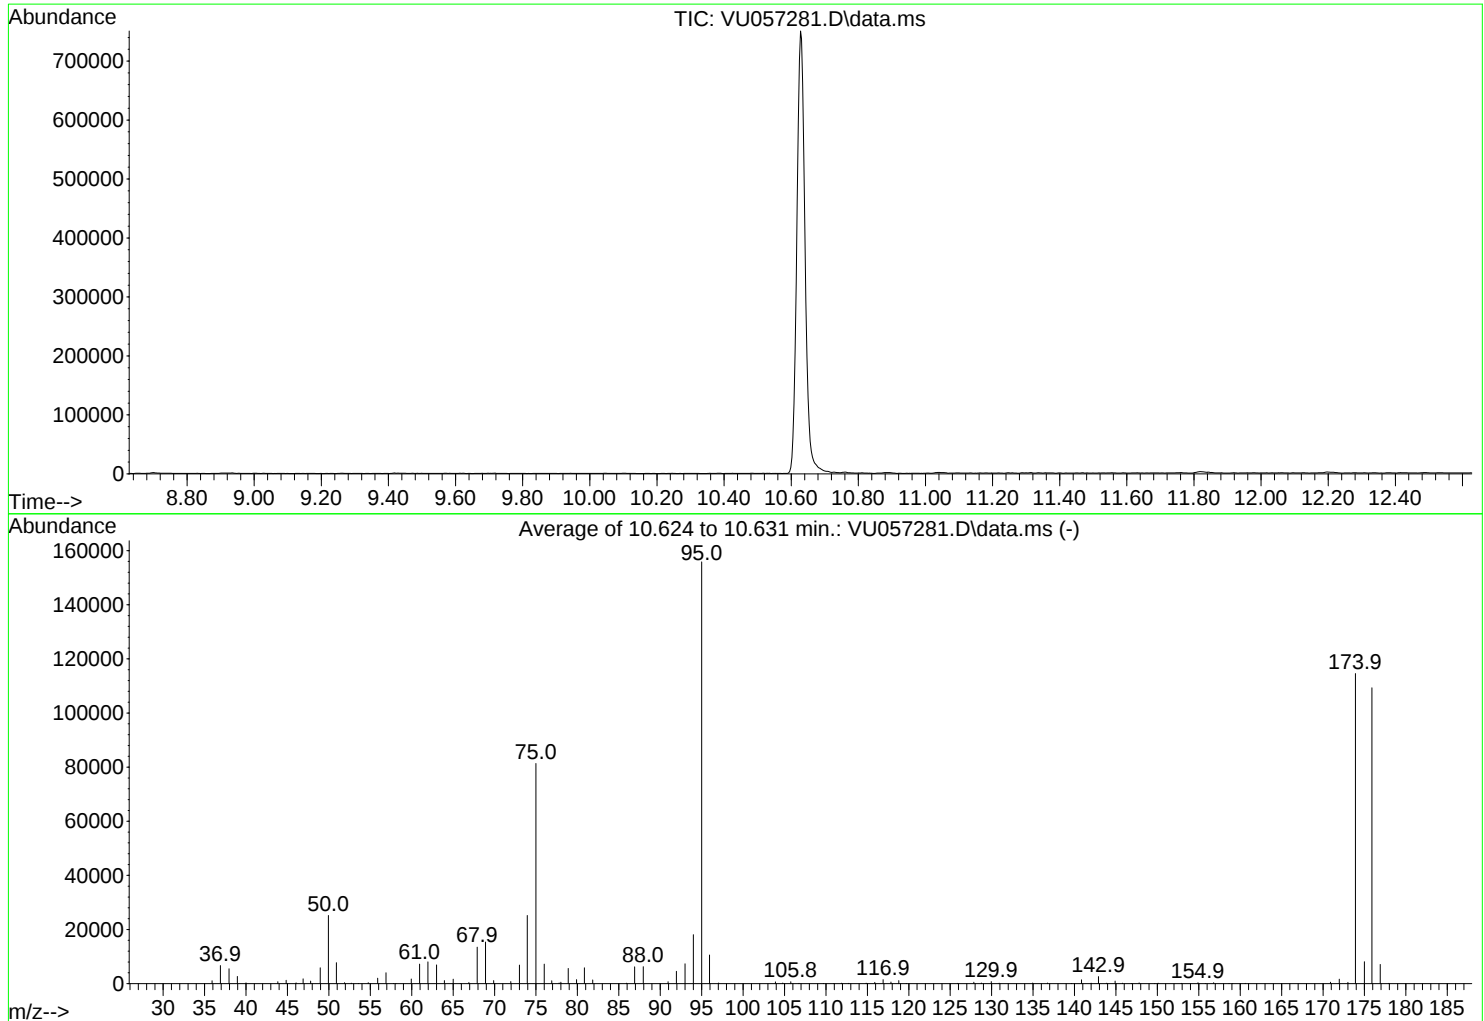

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	25173	PASS
75	95	30	80	52.2	81328	PASS
95	95	100	100	100.0	155861	PASS
96	95	5	9	6.8	10604	PASS
173	174	0.00	2	0.4	508	PASS
174	95	50	120	73.5	114611	PASS
175	174	5	9	7.1	8105	PASS
176	174	95	101	95.4	109309	PASS
177	176	5	9	6.5	7121	PASS

m/z	Abundance
39.80	388.0
43.90	406.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	974.0
36.90	6505.0
38.00	5419.0
39.00	2577.0
39.80	461.0
43.80	1100.0
44.90	1279.0
46.10	242.0
46.90	1770.0
47.80	870.0
49.00	5795.0
49.90	24560.0
50.90	7620.0
51.90	336.0
52.70	197.0
53.60	101.0
54.80	257.0
55.90	1814.0
56.90	4011.0
57.80	119.0
59.90	1640.0
61.00	7174.0
62.00	8014.0
63.00	6931.0
63.90	1051.0
65.00	1432.0
65.90	108.0
66.80	399.0
67.90	13095.0
68.90	15349.0
69.90	984.0
71.90	811.0
73.00	6557.0
74.00	24256.0
75.00	77528.0
76.00	7020.0
76.90	1036.0
77.80	783.0
78.90	5455.0
79.90	1506.0
80.90	5810.0
81.90	1298.0
86.90	6401.0
88.00	5904.0
90.90	717.0
92.00	4491.0
93.00	6763.0
94.00	17712.0
95.00	151616.0
95.90	10076.0
97.10	273.0
103.90	683.0
104.80	195.0
105.70	750.0
106.70	167.0
111.90	145.0
112.70	130.0
114.80	222.0
115.90	540.0
116.90	1369.0
117.80	656.0
118.80	1081.0
125.90	127.0
127.80	474.0
128.80	249.0
130.00	765.0
130.90	193.0
135.00	210.0
136.70	217.0
140.80	1540.0
142.00	147.0
142.90	2599.0
143.90	118.0
144.90	900.0
145.80	167.0
147.80	277.0
150.10	271.0
154.90	379.0
156.70	360.0
160.60	184.0
170.90	453.0
172.00	1534.0
173.00	1524.0
173.90	107984.0
175.00	7848.0
175.90	101816.0
176.90	6883.0
177.90	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	1108.0
36.90	6948.0
38.00	5657.0
39.00	2723.0
40.00	454.0
43.80	1121.0
44.90	1295.0
46.00	285.0
46.90	1784.0
47.80	962.0
48.90	6003.0
49.90	25904.0
50.90	7995.0
51.90	325.0
52.70	180.0
54.70	347.0
55.90	2048.0
56.90	4089.0
60.00	1795.0
61.00	7404.0
61.90	8270.0
63.00	7082.0
64.00	1121.0
65.00	1765.0
65.80	109.0
66.90	453.0
67.90	13812.0
68.90	15877.0
69.90	1178.0
71.90	797.0
73.00	6928.0
74.00	25728.0
75.00	84016.0
76.00	7445.0
76.90	1105.0
78.00	795.0
78.90	5777.0
79.90	1515.0
80.80	6069.0
81.80	1364.0
85.90	270.0
86.90	6456.0
87.90	6369.0
91.00	735.0
91.90	4649.0
93.00	7603.0
94.00	18472.0
95.00	160704.0
96.00	10907.0
97.10	268.0
103.90	633.0
104.80	258.0
105.70	729.0
106.70	146.0
110.90	118.0
111.90	188.0
112.80	135.0
114.80	209.0
115.90	517.0
116.90	1497.0
117.80	613.0
118.80	1140.0
119.70	130.0
125.90	165.0
127.90	546.0
128.70	272.0
130.00	811.0
131.00	197.0
135.00	255.0
136.70	260.0
139.70	121.0
140.80	1416.0
142.00	194.0
142.90	2688.0
143.90	175.0
144.90	970.0
145.80	220.0
146.90	112.0
147.80	304.0
150.10	232.0
152.90	162.0
154.90	357.0
155.80	109.0
156.80	346.0
158.70	108.0
160.60	159.0
170.90	572.0
172.00	1683.0
173.90	117856.0
175.00	8331.0
175.90	112584.0
176.90	7231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

177.90

102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

m/z	Abundance
35.90	1201.0
36.90	6622.0
37.90	5359.0
38.90	2674.0
40.00	477.0
43.90	1095.0
44.80	1151.0
46.00	340.0
46.90	1732.0
47.80	1009.0
48.90	5767.0
50.00	25056.0
50.90	7570.0
51.90	341.0
52.70	165.0
54.70	391.0
55.90	2108.0
56.90	3908.0
58.10	135.0
60.00	1723.0
60.90	6999.0
61.90	7870.0
63.00	6710.0
64.00	1117.0
65.00	1773.0
67.00	485.0
67.90	13570.0
68.90	14892.0
69.90	1196.0
72.00	772.0
73.00	7036.0
73.90	25672.0
75.00	82440.0
76.00	7251.0
76.90	978.0
78.00	833.0
78.90	5613.0
79.90	1478.0
80.80	5649.0
81.80	1385.0
86.00	234.0
86.90	5813.0
87.90	6452.0
91.00	684.0
91.90	4553.0
93.00	7603.0
94.00	18008.0
95.00	155264.0
96.00	10829.0
96.90	230.0
103.90	640.0
104.80	273.0
105.80	669.0
106.80	125.0
109.70	104.0
111.00	157.0
111.90	162.0
112.80	118.0
114.90	194.0
115.90	418.0
116.90	1526.0
117.90	592.0
118.80	1115.0
119.70	130.0
125.90	149.0
127.90	536.0
128.70	263.0
129.90	696.0
130.80	212.0
134.90	268.0
136.80	292.0
139.60	134.0
140.90	1392.0
142.00	241.0
142.90	2527.0
143.90	226.0
144.90	948.0
145.80	252.0
146.90	119.0
147.80	252.0
149.70	163.0
150.10	124.0
152.90	163.0
154.90	316.0
155.80	114.0
156.90	325.0
158.60	120.0
159.10	128.0
161.00	157.0
170.90	512.0
171.90	1685.0
173.90	117992.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102

175.00	8136.0
175.90	113528.0
176.90	7250.0
178.00	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB102