

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
 Data File : VU062622.D
 Acq On : 27 Dec 2024 16:57
 Operator : MD/SY
 Sample : P5309-20
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	111	rVB	34785	41334	13.37%	1.507%
2	1.904	182	191	203	rVB	28206	36697	11.87%	1.338%
3	2.557	383	394	409	rBV	60805	100358	32.45%	3.659%
4	3.695	738	748	757	rBB4	2126	4296	1.39%	0.157%
5	4.615	1026	1034	1072	rBV	36774	100723	32.57%	3.672%
6	5.052	1154	1170	1197	rBV2	62511	141670	45.81%	5.165%
7	5.714	1358	1376	1406	rBV3	118722	309236	100.00%	11.273%
8	6.238	1527	1539	1569	rBV	130599	252676	81.71%	9.211%
9	6.534	1624	1631	1645	rBB7	4647	8485	2.74%	0.309%
10	6.679	1664	1676	1699	rBV2	69653	138063	44.65%	5.033%
11	7.557	1939	1949	1973	rBV	39964	71825	23.23%	2.618%
12	7.888	2040	2052	2073	rBV	151496	266764	86.27%	9.725%
13	8.174	2131	2141	2160	rBV2	23321	41228	13.33%	1.503%
14	8.463	2222	2231	2243	rBB3	3423	5479	1.77%	0.200%
15	8.624	2271	2281	2321	rBV	146018	279686	90.44%	10.196%
16	9.409	2514	2525	2547	rBV	179999	301981	97.65%	11.009%
17	10.746	2930	2941	2955	rBV	56317	91968	29.74%	3.353%
18	10.888	2973	2985	2997	rBB2	7054	11463	3.71%	0.418%
19	11.804	3258	3270	3287	rBV	176016	291623	94.30%	10.631%
20	12.184	3376	3388	3408	rBV	143250	243754	78.82%	8.886%
21	12.766	3561	3569	3577	rBV2	2416	3754	1.21%	0.137%




Sum of corrected areas: 2743063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
Data File : VU062622.D
Acq On : 27 Dec 2024 16:57
Operator : MD/SY
Sample : P5309-20
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

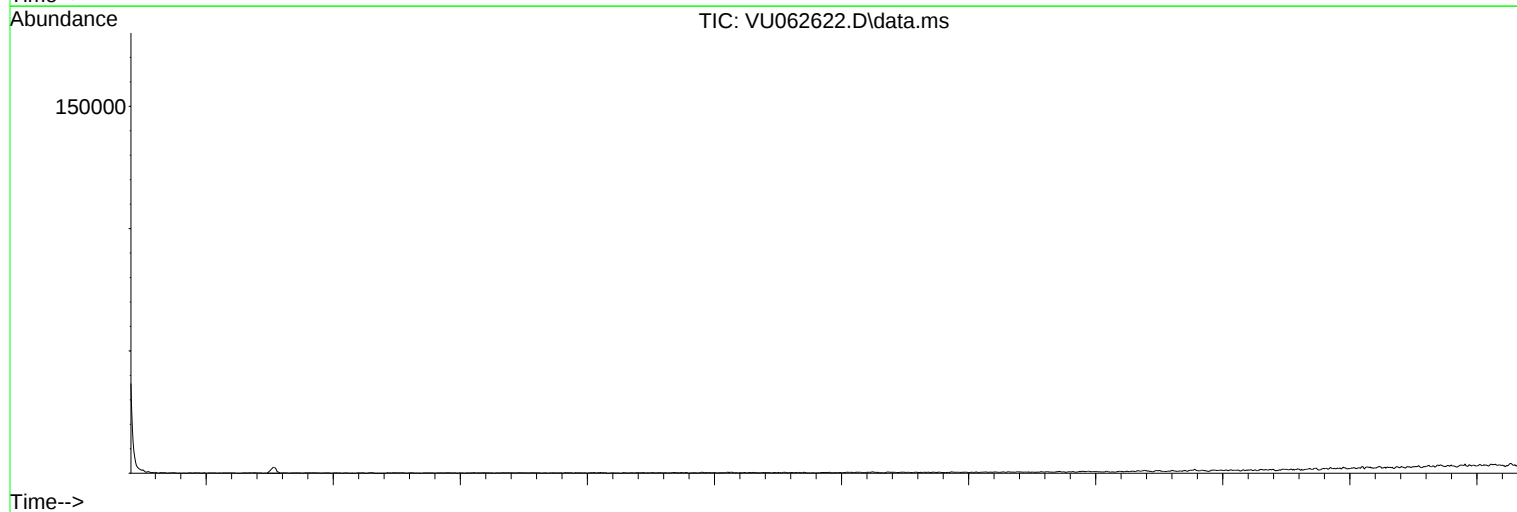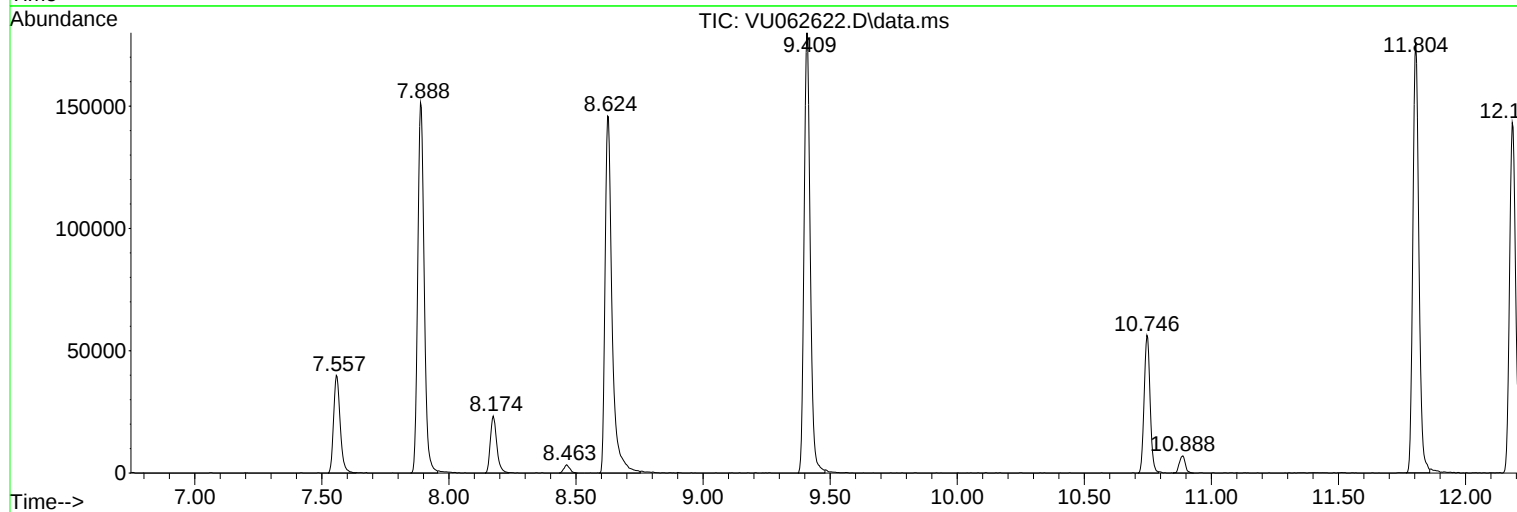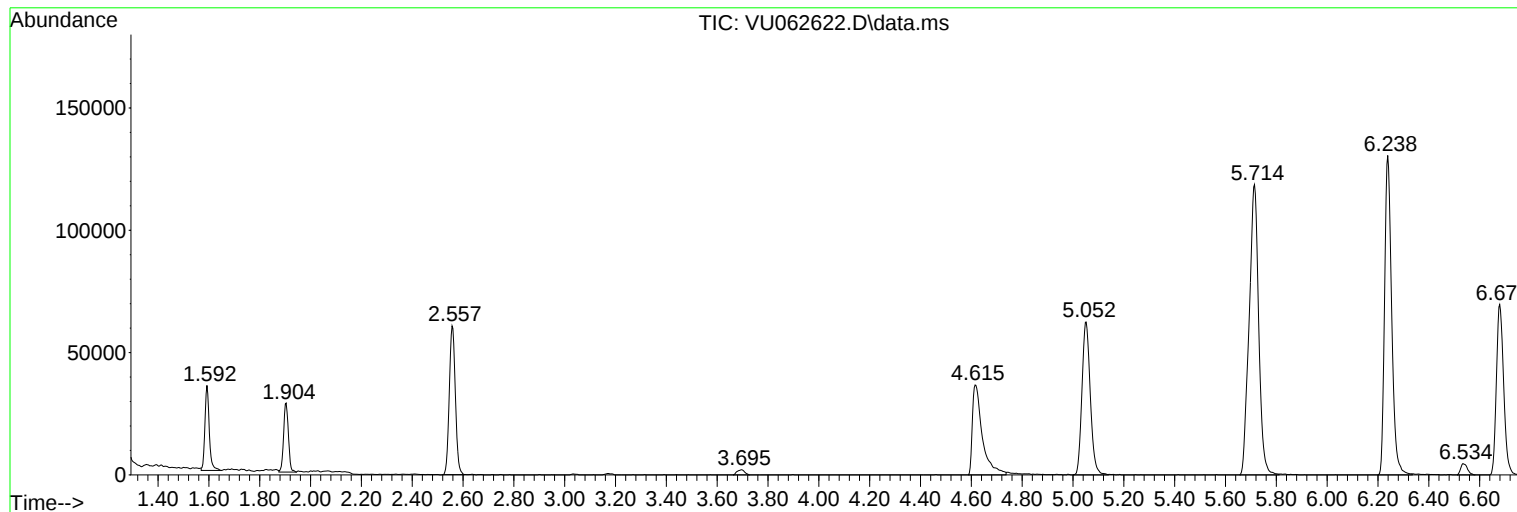

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
Data File : VU062622.D
Acq On : 27 Dec 2024 16:57
Operator : MD/SY
Sample : P5309-20
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
Data File : VU062622.D
Acq On : 27 Dec 2024 16:57
Operator : MD/SY
Sample : P5309-20
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------