

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
 Data File : VU062623.D
 Acq On : 27 Dec 2024 17:21
 Operator : MD/SY
 Sample : P5344-14
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CJ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.355	14	20	27	rBV2	11035	11977	3.70%	0.403%
2	1.593	86	94	109	rVB	35468	42447	13.12%	1.430%
3	1.905	183	191	206	rVB	29753	38300	11.84%	1.290%
4	2.072	234	243	252	rVV	19091	25660	7.93%	0.864%
5	2.130	252	261	281	rVB	31030	47445	14.67%	1.598%
6	2.557	382	394	408	rBV	65144	104736	32.38%	3.528%
7	2.628	408	416	431	rVV2	3883	6976	2.16%	0.235%
8	2.785	449	465	494	rBV2	11965	38979	12.05%	1.313%
9	3.689	738	746	758	rBB4	2539	4857	1.50%	0.164%
10	4.618	1025	1035	1039	rBV2	41456	73918	22.85%	2.490%
11	4.818	1087	1097	1109	rBV3	2916	6573	2.03%	0.221%
12	5.049	1155	1169	1191	rBV2	66134	148856	46.02%	5.015%
13	5.715	1358	1376	1397	rBV2	121940	323462	100.00%	10.897%
14	6.239	1528	1539	1561	rBV2	122930	236526	73.12%	7.968%
15	6.535	1621	1631	1649	rBV	29836	57323	17.72%	1.931%
16	6.679	1664	1676	1694	rBV2	74620	144022	44.53%	4.852%
17	7.557	1939	1949	1963	rBV	41904	74031	22.89%	2.494%
18	7.888	2040	2052	2068	rBV	158552	278387	86.06%	9.378%
19	7.965	2068	2076	2089	rVB2	8215	15595	4.82%	0.525%
20	8.174	2131	2141	2158	rBV2	24181	44262	13.68%	1.491%
21	8.547	2248	2257	2267	rBB5	10739	18358	5.68%	0.618%
22	8.624	2271	2281	2317	rBV	155600	292011	90.28%	9.837%
23	9.409	2512	2525	2544	rBV	169347	287102	88.76%	9.672%
24	9.692	2605	2613	2625	rBB2	3653	5097	1.58%	0.172%
25	10.747	2930	2941	2958	rBB	60387	95781	29.61%	3.227%
26	11.804	3259	3270	3291	rBV	163971	273406	84.52%	9.211%
27	12.065	3342	3351	3366	rBV4	6279	13888	4.29%	0.468%
28	12.184	3377	3388	3413	rBV	155196	258435	79.90%	8.706%




Sum of corrected areas: 2968410

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
Data File : VU062623.D
Acq On : 27 Dec 2024 17:21
Operator : MD/SY
Sample : P5344-14
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

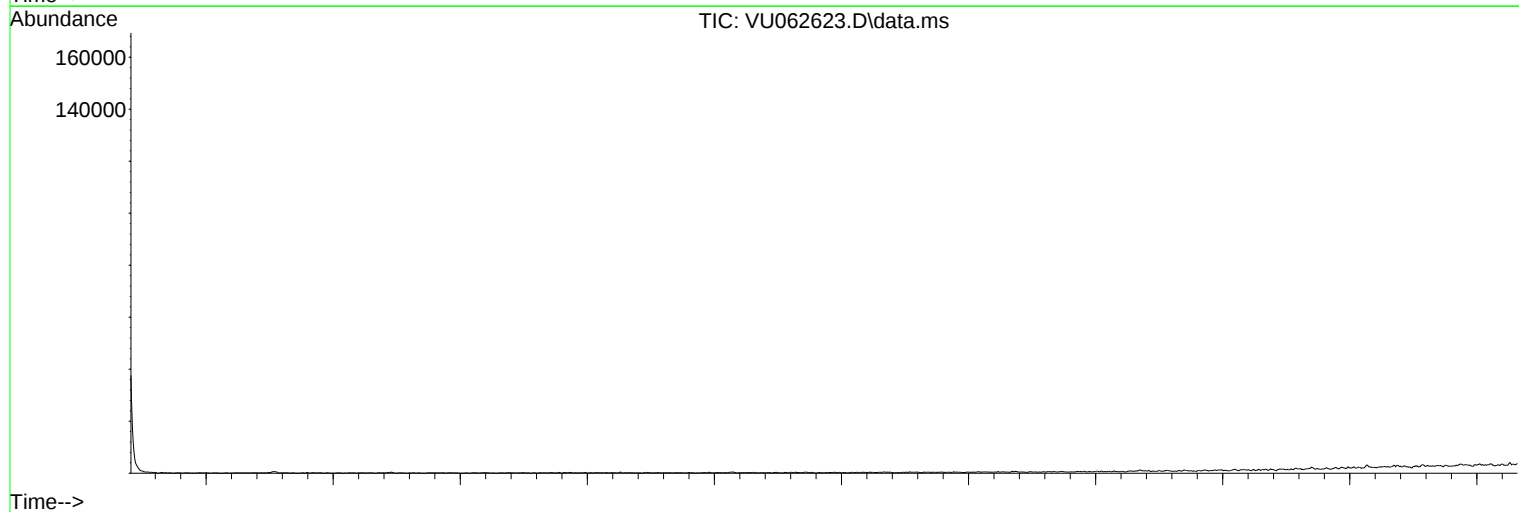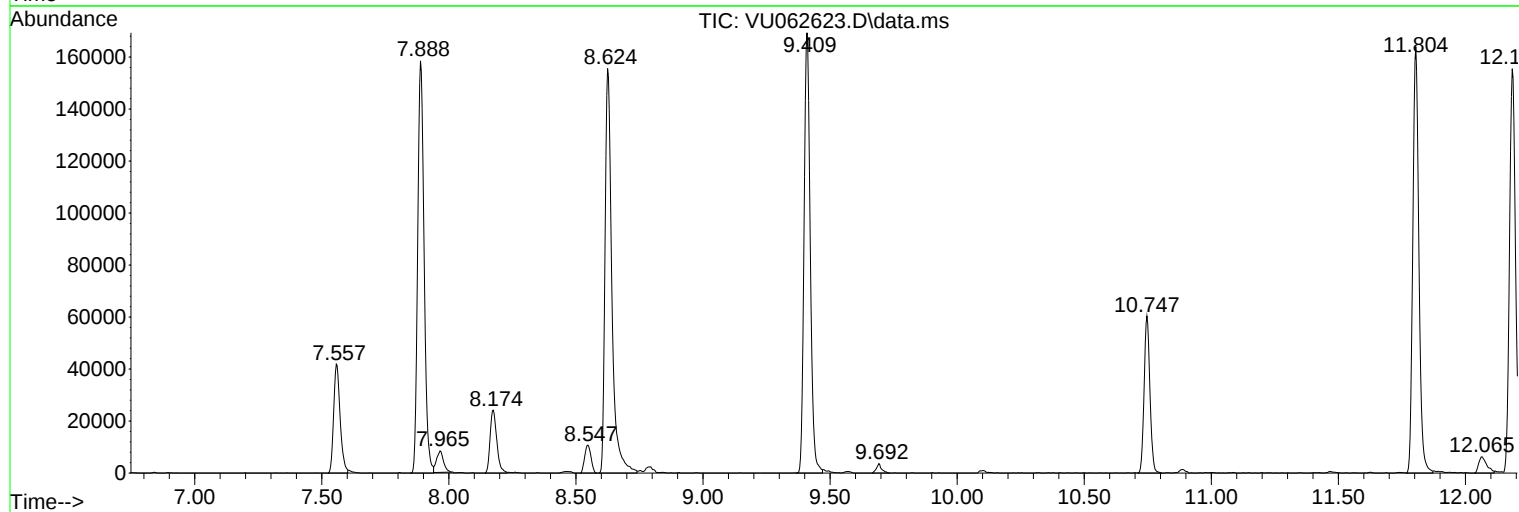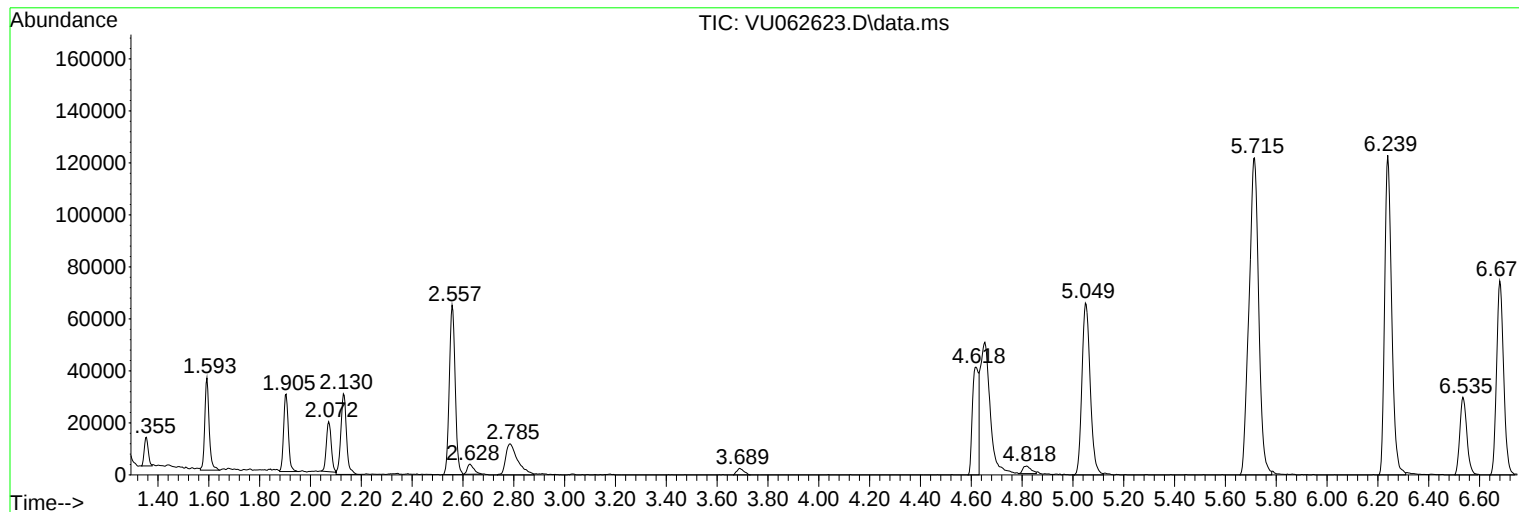

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
Data File : VU062623.D
Acq On : 27 Dec 2024 17:21
Operator : MD/SY
Sample : P5344-14
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CJ3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.072	0.54 ug/L	25660	1,4-Difluorobenzene	6.239

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2	Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3	Fluorodichloromethane	102	CHCl2F	000075-43-4	90
4	1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7
5	Cyclopentene, 1-chloro-	102	C5H7Cl	000930-29-0	5

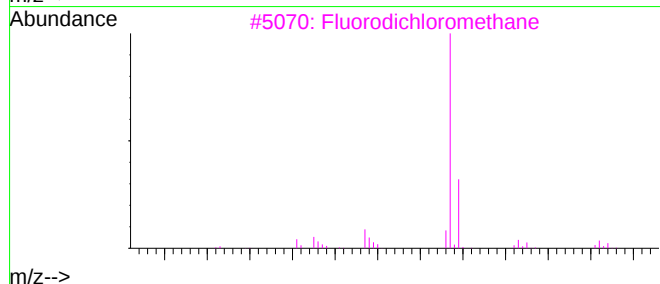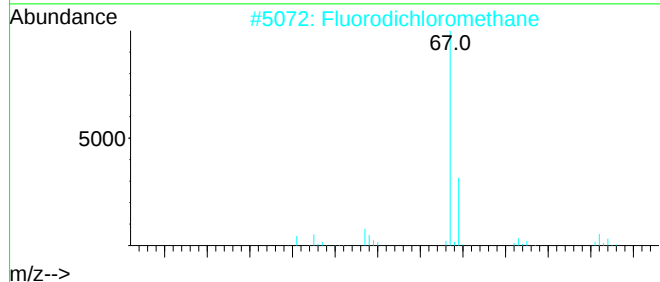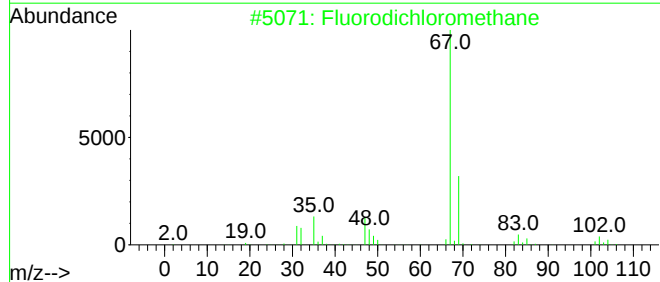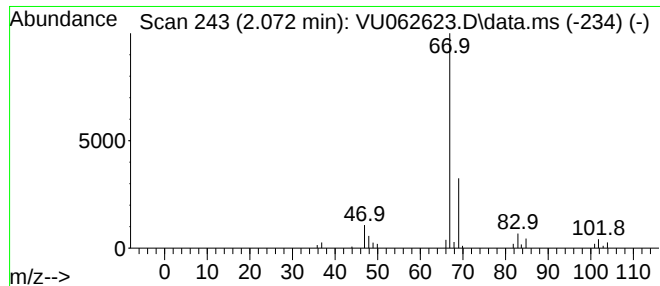

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
Data File : VU062623.D
Acq On : 27 Dec 2024 17:21
Operator : MD/SY
Sample : P5344-14
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.072	0.5	ug/L	25660	1	6.239	236526	5.0