
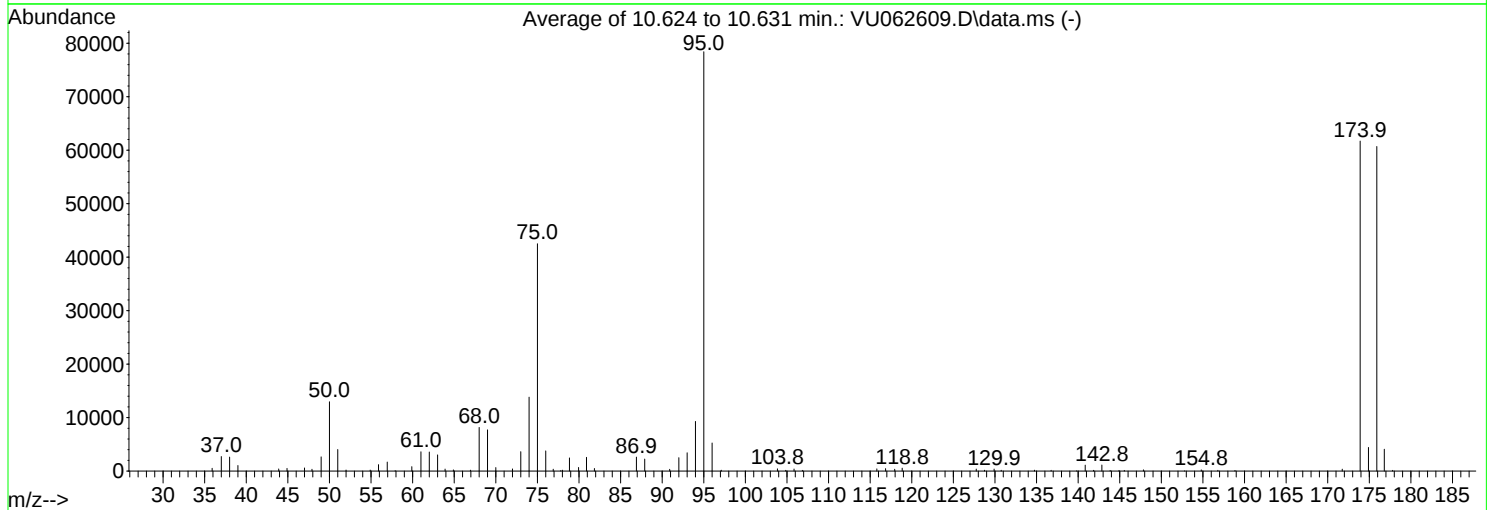


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122724\
Data File : VU062609.D
Acq On : 27 Dec 2024 11:22
Operator : MD/SY
Sample : BFB054
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB054

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 27 21:56:24 2024

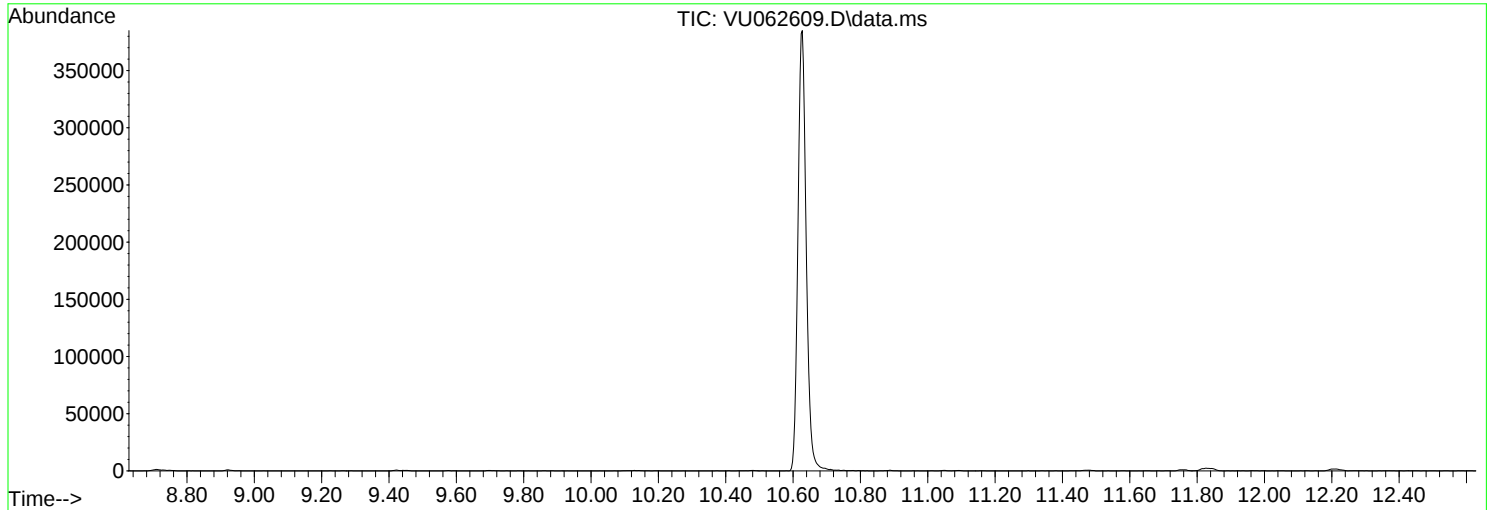

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	12967	PASS
75	95	30	80	54.2	42509	PASS
95	95	100	100	100.0	78413	PASS
96	95	5	9	6.7	5253	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.7	61707	PASS
175	174	5	9	7.2	4415	PASS
176	174	95	101	98.4	60693	PASS
177	176	5	9	6.7	4083	PASS

m/z	Abundance
43.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	543.0
37.00	2857.0
38.00	2713.0
39.00	1037.0
43.90	553.0
44.90	518.0
46.90	602.0
47.90	361.0
49.00	2829.0
50.00	13446.0
51.00	4253.0
52.00	230.0
55.00	194.0
55.90	1235.0
57.00	1806.0
57.90	122.0
59.90	907.0
61.00	3772.0
62.00	3669.0
63.00	3210.0
63.90	373.0
64.90	213.0
67.00	192.0
68.00	8397.0
69.00	7847.0
70.00	647.0
72.00	381.0
73.00	3670.0
74.00	14412.0
75.00	43992.0
76.00	3886.0
76.90	399.0
77.80	244.0
78.80	2564.0
80.00	747.0
80.90	2564.0
81.90	566.0
86.90	2761.0
87.90	2183.0
90.90	328.0
92.00	2407.0
93.00	3474.0
94.00	9510.0
95.00	80168.0
96.00	5451.0
97.10	160.0
103.90	479.0
104.80	142.0
105.80	367.0
106.90	122.0
115.80	387.0
116.80	475.0
117.90	334.0
118.80	597.0
127.80	364.0
128.70	122.0
129.90	369.0
130.80	171.0
134.80	190.0
136.80	170.0
140.80	1050.0
141.80	153.0
142.80	1179.0
143.80	110.0
144.90	134.0
145.50	106.0
147.90	236.0
154.80	226.0
156.80	161.0
158.90	107.0
171.80	391.0
173.90	61536.0
174.90	4554.0
175.90	61160.0
176.80	4275.0
177.80	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	533.0
37.00	2782.0
38.00	2677.0
39.00	1095.0
43.90	533.0
44.90	529.0
47.00	592.0
47.90	343.0
49.00	2761.0
50.00	13257.0
51.00	4122.0
52.00	206.0
54.90	191.0
55.90	1245.0
56.90	1703.0
57.90	103.0
59.90	892.0
61.00	3696.0
62.00	3614.0
63.00	3114.0
63.90	408.0
64.90	229.0
66.90	159.0
68.00	8304.0
69.00	7865.0
70.00	695.0
72.00	403.0
73.00	3734.0
74.00	14173.0
75.00	43880.0
76.00	3868.0
76.90	344.0
78.00	243.0
78.80	2547.0
80.00	679.0
80.90	2639.0
81.90	501.0
86.90	2671.0
87.90	2247.0
90.90	359.0
92.00	2600.0
93.00	3532.0
94.00	9540.0
95.00	80576.0
96.00	5540.0
97.10	161.0
103.90	437.0
104.90	159.0
105.90	404.0
106.80	151.0
115.80	450.0
116.80	460.0
117.90	348.0
118.80	555.0
127.70	397.0
128.70	176.0
129.90	406.0
130.80	161.0
134.70	193.0
136.70	138.0
140.80	1133.0
141.90	151.0
142.80	1172.0
143.90	131.0
144.90	109.0
145.50	123.0
147.80	250.0
152.80	105.0
154.80	244.0
156.80	172.0
158.80	124.0
171.70	362.0
173.90	63448.0
174.90	4510.0
175.90	62224.0
176.80	4200.0
177.80	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054

m/z	Abundance
35.90	484.0
37.00	2529.0
38.00	2450.0
39.00	1005.0
43.90	405.0
44.90	457.0
47.10	578.0
47.90	338.0
49.00	2391.0
50.00	12197.0
51.00	3728.0
52.00	168.0
54.80	194.0
55.90	1130.0
56.90	1551.0
59.90	687.0
61.00	3365.0
62.00	3399.0
63.00	2750.0
63.90	364.0
64.90	252.0
66.90	158.0
68.00	7772.0
69.00	7421.0
70.00	615.0
72.00	428.0
73.00	3474.0
74.00	12880.0
75.00	39656.0
76.00	3566.0
76.90	322.0
78.00	273.0
78.90	2291.0
79.90	601.0
80.90	2504.0
81.80	394.0
86.90	2398.0
87.90	2294.0
90.90	320.0
92.00	2493.0
93.00	3244.0
94.00	8795.0
95.00	74496.0
96.00	4767.0
97.10	170.0
103.80	350.0
104.90	125.0
105.90	393.0
106.90	141.0
115.80	417.0
116.90	447.0
118.00	339.0
118.90	507.0
127.70	369.0
128.80	188.0
129.90	362.0
130.70	130.0
134.80	139.0
136.70	114.0
139.80	117.0
140.90	1152.0
141.90	141.0
142.90	1042.0
143.90	115.0
145.60	145.0
147.80	228.0
154.80	209.0
156.80	121.0
158.80	116.0
171.70	327.0
173.90	60136.0
174.90	4182.0
175.90	58696.0
176.80	3773.0
177.80	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB054