

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122818\
 Data File : VU028973.D
 Acq On : 27 Dec 2018 19:05
 Operator : MD/SY
 Sample : J6506-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF029

Quant Time: Dec 28 09:08:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 28 03:05:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	123752	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	115430	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	54510	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	31012	4.68	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.60%
7) Chloroethane-d5	1.68	69	28148	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.27	63	45428	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	4.20	46	88816	51.31	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.62%
24) Chloroform-d	4.65	84	62296	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.31	65	31363	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
32) Benzene-d6	5.34	84	132835	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	6.33	67	43891	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.56	98	118813	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
43) trans-1,3-Dichloropropene-	7.85	79	15805	4.87	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.40%
46) 2-Hexanone-d5	8.31	63	75401	50.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.98%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	34060	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	45640	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
13) Acetone	2.33	43	13624	9.751 ug/L	95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122818\
Data File : VU028973.D
Acq On : 27 Dec 2018 19:05
Operator : MD/SY
Sample : J6506-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF029

Quant Time: Dec 28 09:08:41 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 28 03:05:23 2018
Response via : Initial Calibration

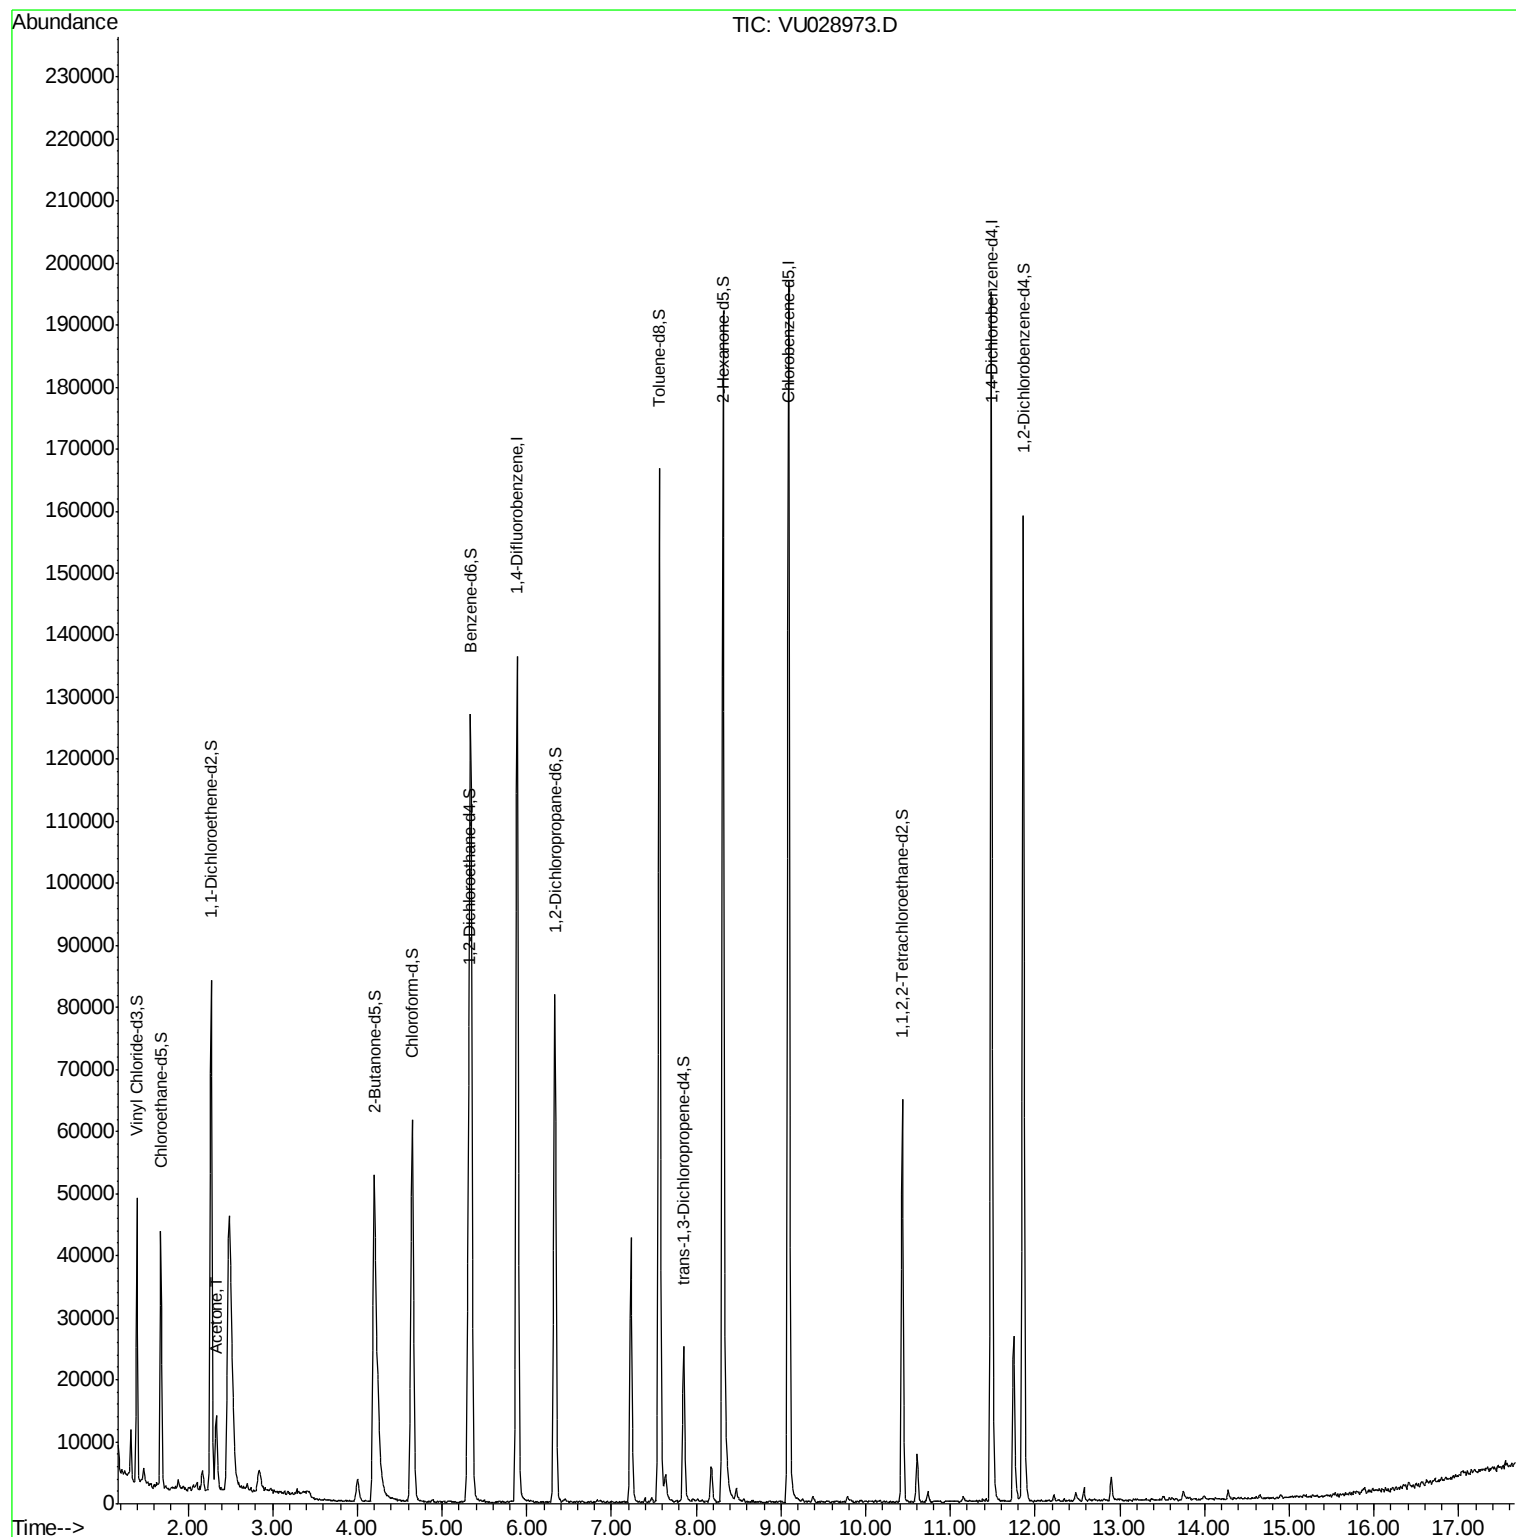

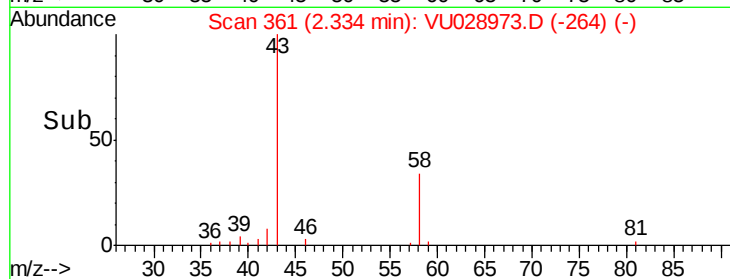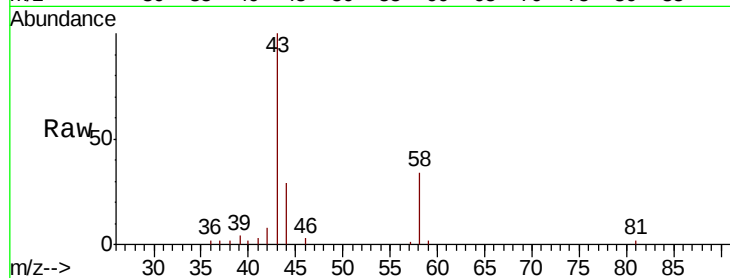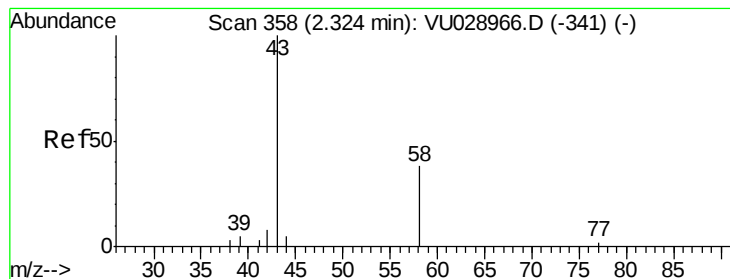

#13

Acetone

Concen: 9.751 ug/L

RT: 2.33 min Scan# 361

Delta R.T. 0.01 min

Lab File: VU028973.D

Acq: 27 Dec 2018 19:05

Instrument :
MSVOA_U
ClientSampleId :
BF029

Tot Ion: 43 Resp: 13624

Ion Ratio Lower Upper

43 100

58 33.1 0.0 71.8

