

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122818\
 Data File : VU028974.D
 Acq On : 27 Dec 2018 19:28
 Operator : MD/SY
 Sample : J6506-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF031

Quant Time: Dec 28 03:29:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 28 03:05:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	124223	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	115728	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	55585	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	30460	4.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.60%
7) Chloroethane-d5	1.68	69	28528	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.40%
11) 1,1-Dichloroethene-d2	2.27	63	44943	3.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.80%
20) 2-Butanone-d5	4.19	46	88478	50.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.84%
24) Chloroform-d	4.65	84	61084	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.31	65	32099	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.34	84	130562	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.33	67	43961	5.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.60%
41) Toluene-d8	7.57	98	118557	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.85	79	15318	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	8.31	63	73557	49.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.22%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33433	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	44471	4.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.60%


Target Compounds					Ovalue
13) Acetone	2.32	43	12888	9.189 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122818\
Data File : VU028974.D
Acq On : 27 Dec 2018 19:28
Operator : MD/SY
Sample : J6506-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF031

Quant Time: Dec 28 03:29:40 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 28 03:05:23 2018
Response via : Initial Calibration

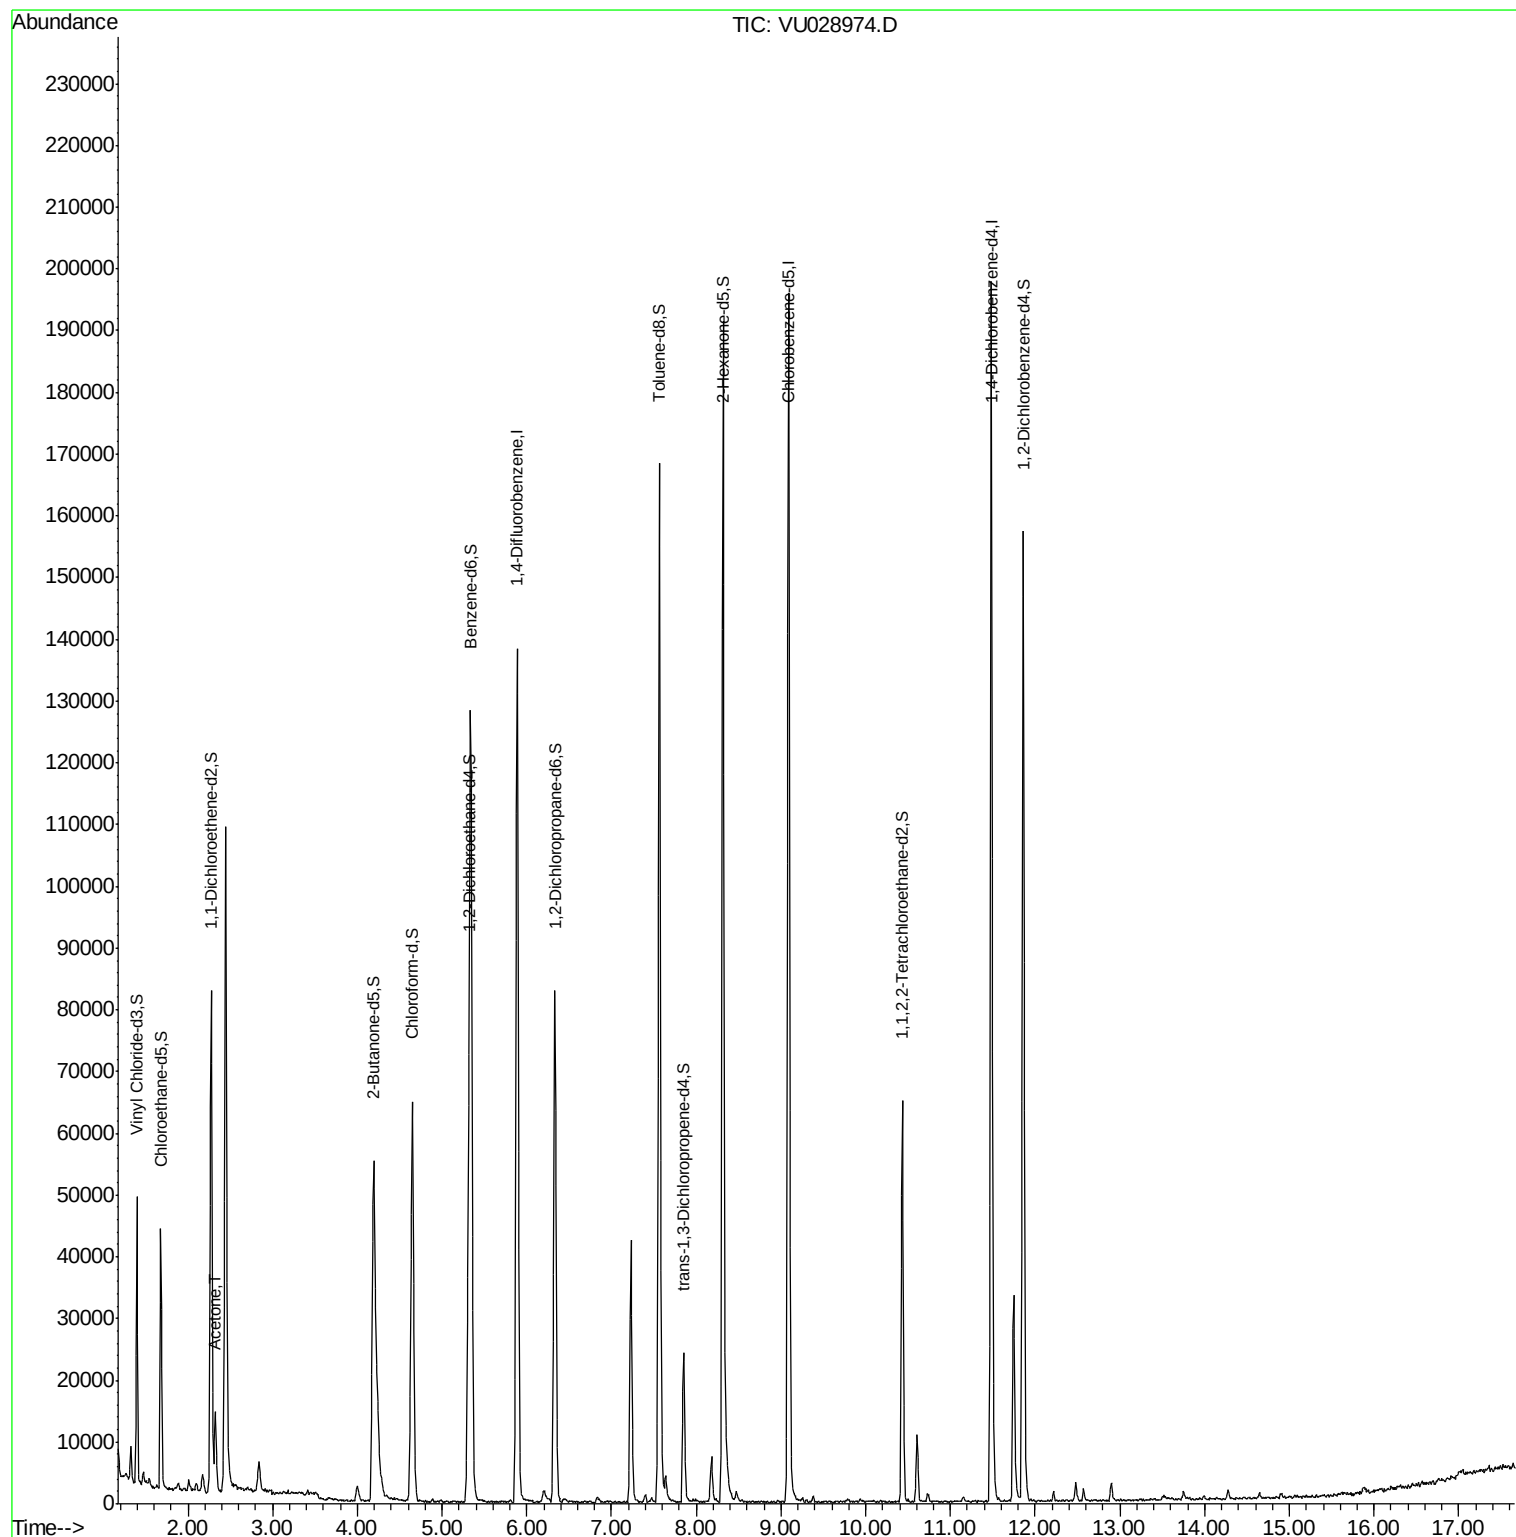

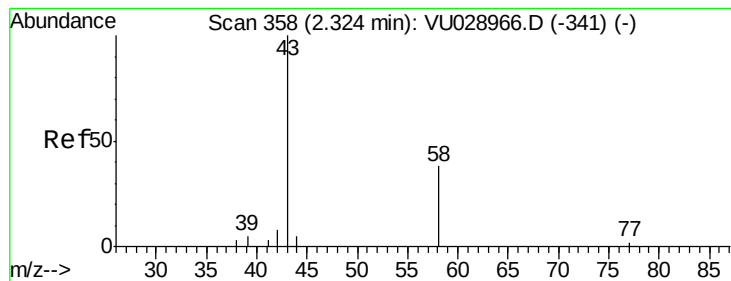

#13

Acetone

Concen: 9.189 ug/L

RT: 2.32 min Scan# 357

Delta R.T. 0.00 min

Lab File: VU028974.D

Acq: 27 Dec 2018 19:28

Instrument :
MSVOA_U
ClientSampleId :
BF031

Tot Ion: 43 Resp: 12888

Ion Ratio Lower Upper

43 100

58 33.8 0.0 71.8

