

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122818\
 Data File : VU028975.D
 Acq On : 27 Dec 2018 19:52
 Operator : MD/SY
 Sample : J6506-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF039

Quant Time: Dec 28 03:28:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 28 03:05:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	124208	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	118048	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	56095	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	30669	4.61	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.20%
7) Chloroethane-d5	1.68	69	28322	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.27	63	45419	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	4.19	46	91057	52.41	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.82%
24) Chloroform-d	4.65	84	60996	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.31	65	31883	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.34	84	131110	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.33	67	43685	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	7.57	98	115894	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
43) trans-1,3-Dichloropropene-	7.85	79	15441	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.31	63	74594	49.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.64%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33212	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	45553	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	12596	8.982 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122818\
Data File : VU028975.D
Acq On : 27 Dec 2018 19:52
Operator : MD/SY
Sample : J6506-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF039

Quant Time: Dec 28 03:28:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 28 03:05:23 2018
Response via : Initial Calibration

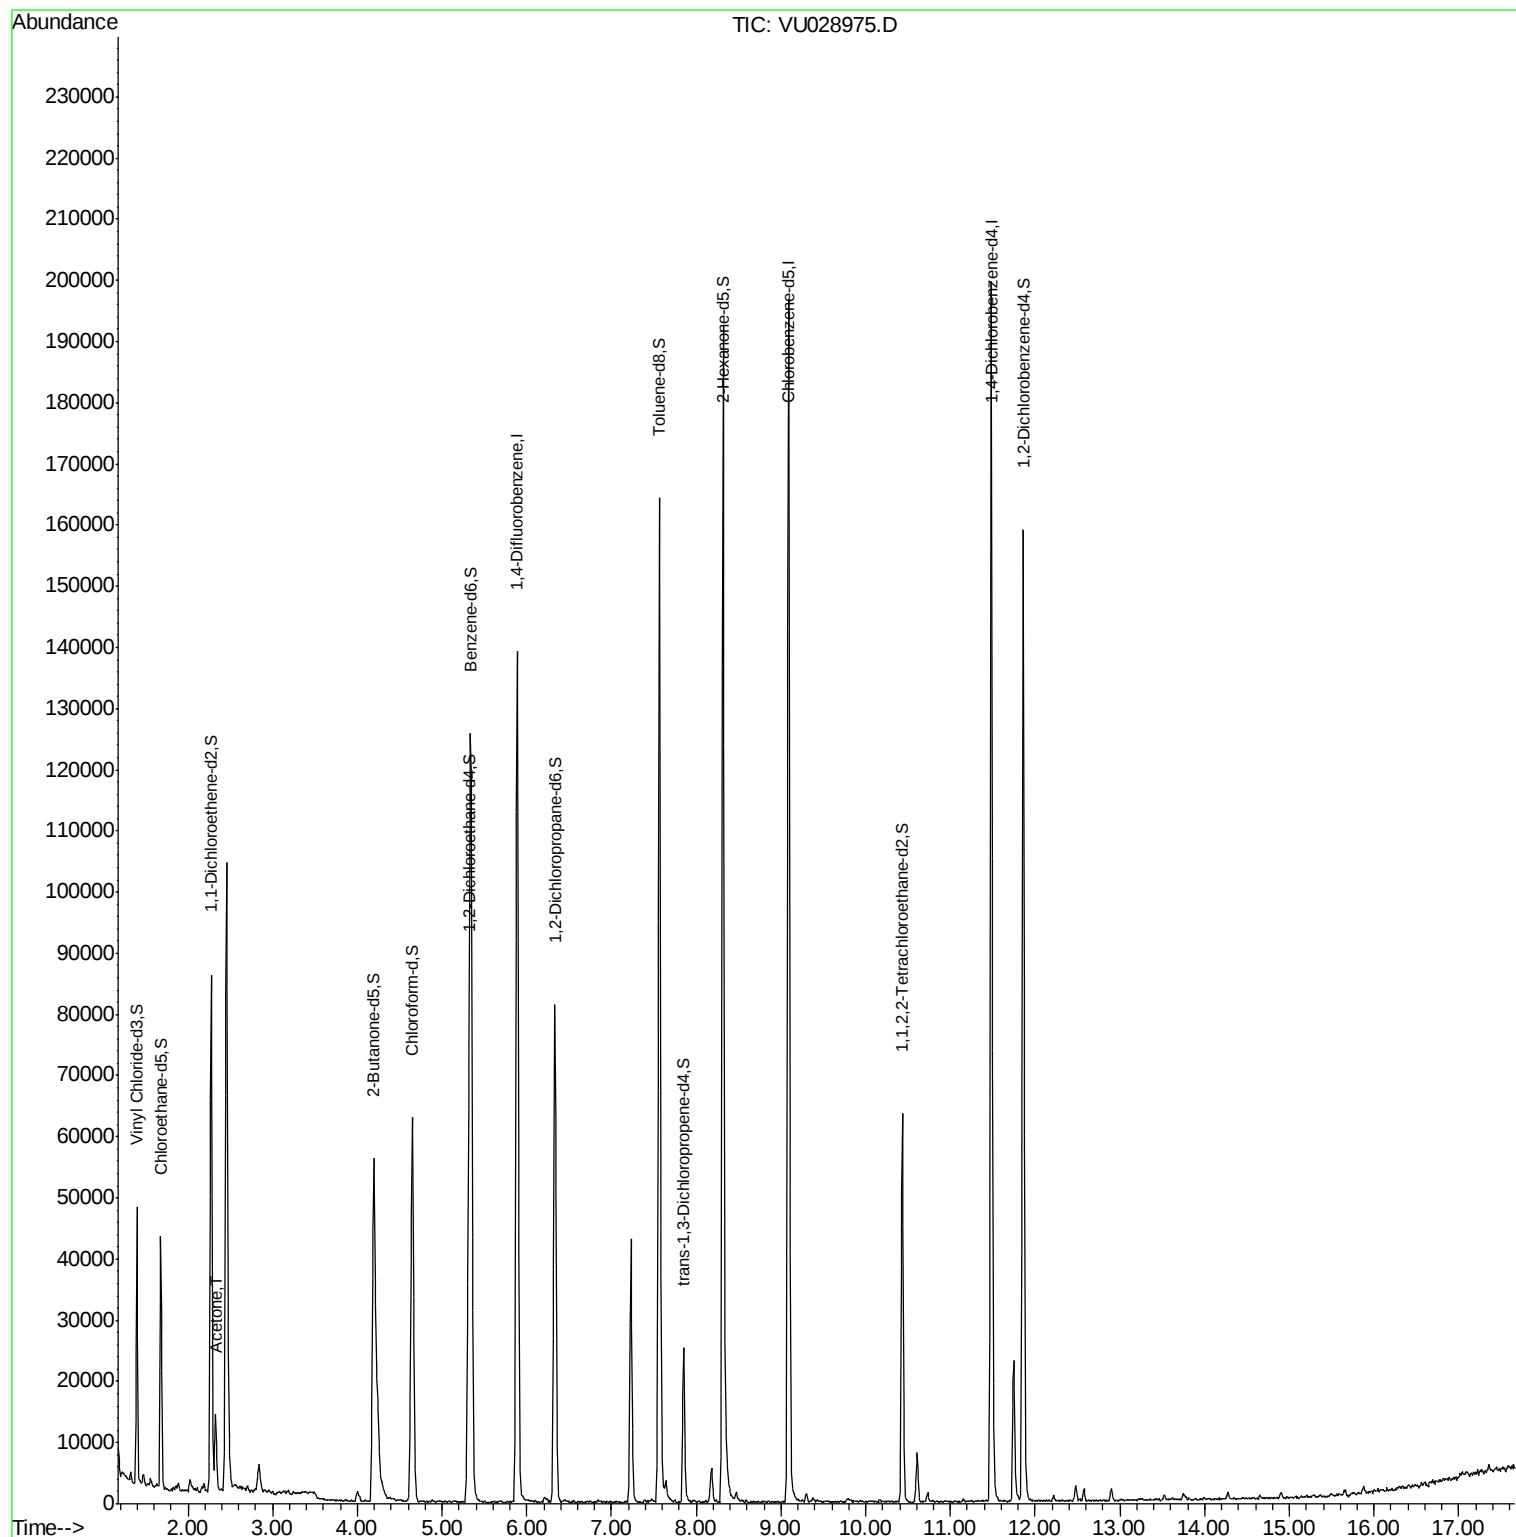

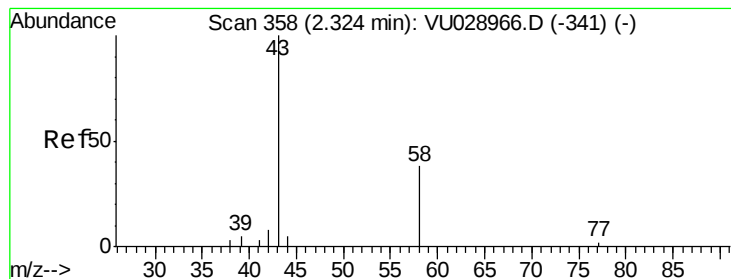

#13
 Acetone
 Concen: 8.982 ug/L
 RT: 2.32 min Scan# 358
 Delta R.T. 0.00 min
 Lab File: VU028975.D
 Acq: 27 Dec 2018 19:52

Instrument :
 MSVOA_U
 ClientSampleId :
 BF039

Tot Ion: 43 Resp: 12596
 Ion Ratio Lower Upper
 43 100
 58 34.6 0.0 71.8

