

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122818\
 Data File : VU028977.D
 Acq On : 27 Dec 2018 20:40
 Operator : MD/SY
 Sample : J6507-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF048

Quant Time: Dec 28 09:10:08 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 28 03:05:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	117657	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	113121	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	54120	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	29869	4.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.80%
7) Chloroethane-d5	1.68	69	26573	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.27	63	42503	3.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.80%
20) 2-Butanone-d5	4.19	46	84427	51.30	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.60%
24) Chloroform-d	4.65	84	58136	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.31	65	29416	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
32) Benzene-d6	5.34	84	123095	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.33	67	40569	4.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.00%
41) Toluene-d8	7.57	98	109869	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.85	79	14387	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.31	63	70479	48.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.26%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	31595	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	42863	4.73	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.60%


Target Compounds					Ovalue
13) Acetone	2.32	43	11364	8.555 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122818\
Data File : VU028977.D
Acq On : 27 Dec 2018 20:40
Operator : MD/SY
Sample : J6507-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF048

Quant Time: Dec 28 09:10:08 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 28 03:05:23 2018
Response via : Initial Calibration

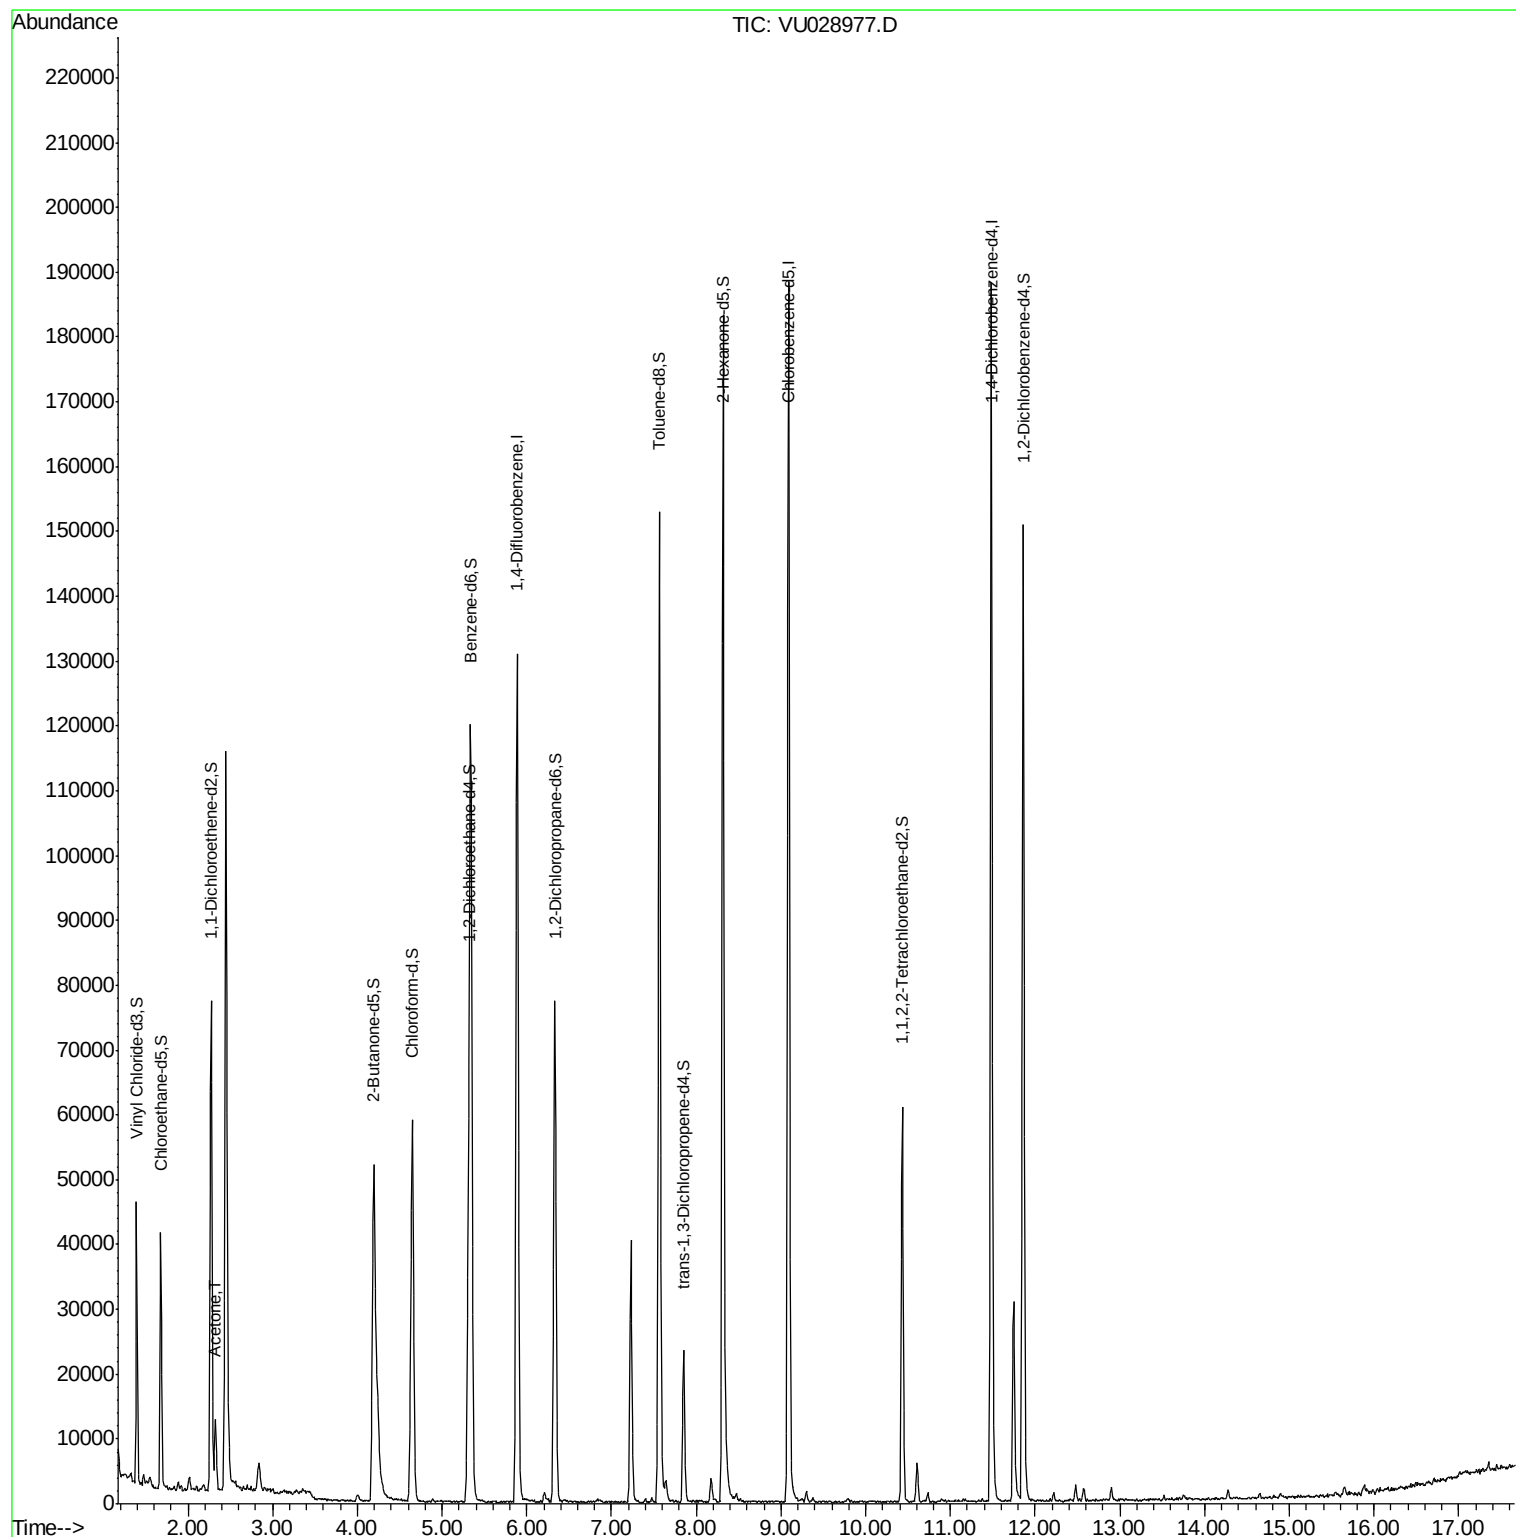

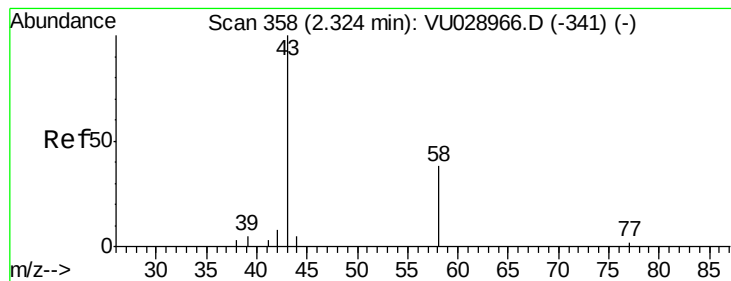

#13

Acetone

Concen: 8.555 ug/L

RT: 2.32 min Scan# 358

Delta R.T. 0.00 min

Lab File: VU028977.D

Acq: 27 Dec 2018 20:40

Instrument :
MSVOA_U
ClientSampleId :
BF048

Tot Ion: 43 Resp: 11364

Ion Ratio Lower Upper

43 100

58 32.6 0.0 71.8

