


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122819\
Data File : VU036362.D
Acq On : 28 Dec 2019 11:04
Operator : JC/MD
Sample : BFB26
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Dec 30 06:07:33 2019

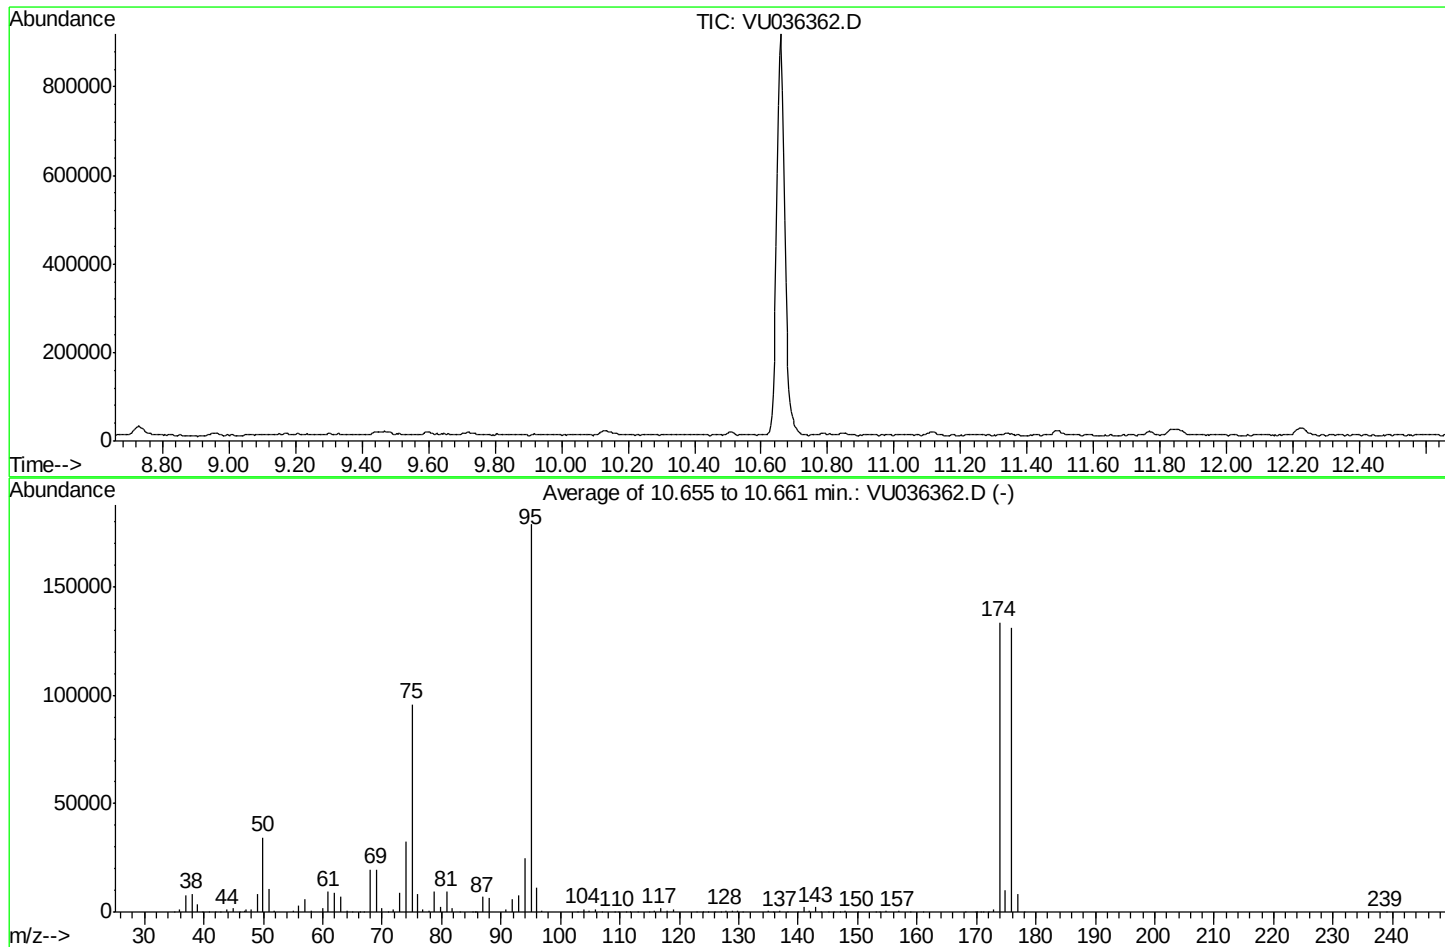

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	34524	PASS
75	95	30	80	53.6	95962	PASS
95	95	100	100	100.0	178889	PASS
96	95	5	9	6.4	11456	PASS
173	174	0.00	2	0.7	962	PASS
174	95	50	120	74.6	133530	PASS
175	174	5	9	7.6	10190	PASS
176	174	95	101	98.0	130898	PASS
177	176	5	9	6.3	8215	PASS

m/z	Abundance
35.90	2088.0
36.90	8441.0
38.00	8955.0
39.00	3922.0
39.80	307.0
40.80	980.0
42.00	284.0
42.90	997.0
43.90	2771.0
44.90	1803.0
46.10	204.0
47.00	1655.0
47.80	1026.0
48.90	8111.0
49.90	34736.0
50.90	11452.0
51.90	535.0
54.00	182.0
55.00	1528.0
56.00	3454.0
57.00	6455.0
58.00	265.0
59.90	1819.0
60.90	9224.0
61.90	8742.0
63.00	6613.0
64.00	672.0
64.90	174.0
66.90	481.0
68.00	19928.0
69.00	20128.0
70.00	1898.0
71.00	545.0
71.90	956.0
73.00	8273.0
73.90	32816.0
75.00	94528.0
76.00	8070.0
76.80	1192.0
77.90	744.0
78.80	8997.0
79.90	2581.0
80.90	9539.0
81.90	1861.0
83.00	521.0
84.10	137.0
84.80	374.0
85.30	288.0
85.90	299.0
86.90	6727.0
87.90	6248.0
90.80	1117.0
91.90	6356.0
93.00	7989.0
94.00	23832.0
95.00	173248.0
96.00	11253.0
97.00	750.0
98.00	239.0
102.90	263.0
103.90	1306.0
104.80	498.0
105.80	1163.0
106.90	201.0
109.00	195.0
109.70	180.0
111.00	358.0
111.80	238.0
112.90	238.0
115.00	208.0
115.90	631.0
116.80	1655.0
117.80	769.0
118.90	1256.0
122.90	122.0
123.90	234.0
125.90	165.0
126.90	158.0
127.80	864.0
128.90	467.0
129.80	558.0
130.70	176.0
134.90	410.0
136.90	533.0
138.10	147.0
139.90	137.0
140.90	2205.0
141.80	388.0
142.90	2214.0
143.70	132.0
145.10	188.0
145.90	328.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

147.00	298.0
147.80	401.0
149.90	186.0
153.00	185.0
153.70	222.0
154.70	300.0
156.90	341.0
159.00	135.0
161.00	189.0
169.80	230.0
171.10	295.0
172.00	337.0
172.90	975.0
173.90	127696.0
174.90	9771.0
175.90	123960.0
176.90	8269.0
178.00	295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
35.10	224.0
35.90	2143.0
36.90	7893.0
38.00	9010.0
38.90	3996.0
39.80	323.0
40.80	1130.0
42.00	252.0
42.90	990.0
43.90	2733.0
44.90	2024.0
46.00	216.0
47.10	1847.0
47.90	1031.0
48.90	8751.0
49.90	35440.0
50.90	11165.0
51.90	590.0
55.00	1434.0
56.00	3679.0
57.00	6830.0
58.10	333.0
59.90	1747.0
60.90	9437.0
62.00	9342.0
63.00	7021.0
64.00	653.0
64.90	190.0
66.30	140.0
66.90	515.0
67.90	20456.0
69.00	20704.0
70.00	2199.0
71.00	660.0
71.90	892.0
73.00	8927.0
74.00	33032.0
75.00	98344.0
76.00	8538.0
76.80	1178.0
77.90	666.0
78.80	9928.0
79.90	2584.0
80.90	10076.0
81.80	2049.0
83.00	486.0
83.90	165.0
84.80	287.0
85.20	257.0
85.60	321.0
86.90	7387.0
87.90	6704.0
90.80	1177.0
91.90	6061.0
93.00	8317.0
94.00	25360.0
95.00	184384.0
96.00	11936.0
96.90	665.0
98.10	265.0
102.90	261.0
103.90	1350.0
104.80	514.0
105.90	1043.0
106.90	234.0
109.00	102.0
109.80	179.0
110.90	318.0
111.70	196.0
112.90	273.0
114.90	171.0
115.70	587.0
116.80	1596.0
117.80	753.0
118.90	1168.0
122.90	121.0
123.90	167.0
124.80	141.0
125.80	116.0
126.90	196.0
127.80	917.0
128.90	434.0
129.80	659.0
130.70	262.0
134.90	501.0
135.70	120.0
136.90	591.0
138.10	120.0
140.00	135.0
140.90	2119.0
141.90	391.0
142.90	2344.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

145.10	258.0
145.90	309.0
147.10	246.0
147.90	439.0
150.00	191.0
153.00	166.0
153.60	190.0
154.80	356.0
156.90	360.0
158.80	203.0
161.00	249.0
169.80	225.0
170.80	291.0
172.00	362.0
172.90	911.0
173.90	137344.0
174.90	10533.0
175.90	135104.0
176.90	8413.0
178.00	233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
35.90	2047.0
36.90	7402.0
38.00	8172.0
38.90	3730.0
39.80	347.0
40.80	1020.0
42.00	245.0
42.90	1041.0
43.90	2610.0
44.90	2010.0
46.10	189.0
46.80	1761.0
47.90	958.0
48.90	8397.0
49.90	33752.0
51.00	9689.0
51.90	636.0
55.00	1348.0
56.00	3708.0
57.00	6364.0
58.20	374.0
60.00	1760.0
60.90	8870.0
62.00	8954.0
63.00	7077.0
64.10	662.0
64.90	174.0
66.30	132.0
66.90	573.0
67.90	18680.0
69.00	19544.0
70.00	2115.0
71.00	663.0
71.90	926.0
73.00	8873.0
74.00	31344.0
75.00	95016.0
76.00	8140.0
76.80	953.0
77.80	679.0
78.80	9902.0
79.90	2342.0
80.90	9325.0
81.80	2093.0
83.10	405.0
83.90	163.0
84.80	154.0
85.10	158.0
85.60	319.0
86.90	6968.0
87.90	6354.0
90.90	1026.0
91.90	5533.0
93.00	7890.0
94.00	24672.0
95.00	179520.0
96.00	11580.0
96.90	644.0
98.00	273.0
102.90	189.0
103.90	1112.0
104.80	567.0
105.90	1016.0
106.90	251.0
109.80	194.0
110.90	243.0
111.60	202.0
112.90	297.0
114.90	167.0
115.80	651.0
116.70	1275.0
117.90	817.0
118.90	1082.0
122.90	104.0
123.80	102.0
124.90	160.0
126.90	153.0
127.80	890.0
129.00	407.0
129.80	715.0
130.70	395.0
134.90	577.0
135.80	166.0
136.90	514.0
140.90	1968.0
141.90	356.0
143.00	2400.0
145.10	358.0
145.90	216.0
147.20	169.0
147.90	460.0
150.00	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

153.50	110.0
154.80	329.0
156.90	322.0
158.80	209.0
161.00	256.0
168.20	126.0
170.00	182.0
170.70	304.0
172.90	1002.0
173.90	135552.0
174.90	10268.0
175.90	133632.0
176.90	7965.0
178.00	156.0
238.90	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
35.80	805.0
38.00	342.0
38.90	376.0
39.80	264.0
40.90	974.0
41.90	184.0
42.80	866.0
43.90	1669.0
45.10	282.0
49.90	118.0
53.00	262.0
53.90	168.0
54.90	806.0
56.10	405.0
57.10	666.0
59.70	101.0
66.00	174.0
66.80	389.0
68.00	231.0
68.80	365.0
70.00	189.0
71.10	536.0
72.70	148.0
77.00	155.0
78.90	268.0
79.80	103.0
80.80	298.0
81.90	258.0
82.90	468.0
84.00	156.0
84.80	298.0
90.90	154.0
92.90	111.0
95.00	161.0
95.90	133.0
96.90	259.0
97.90	305.0
105.10	187.0
111.00	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26