


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122820\
 Data File : VU041818.D
 Acq On : 28 Dec 2020 09:30
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB351

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR122820WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Dec 29 00:47:36 2020

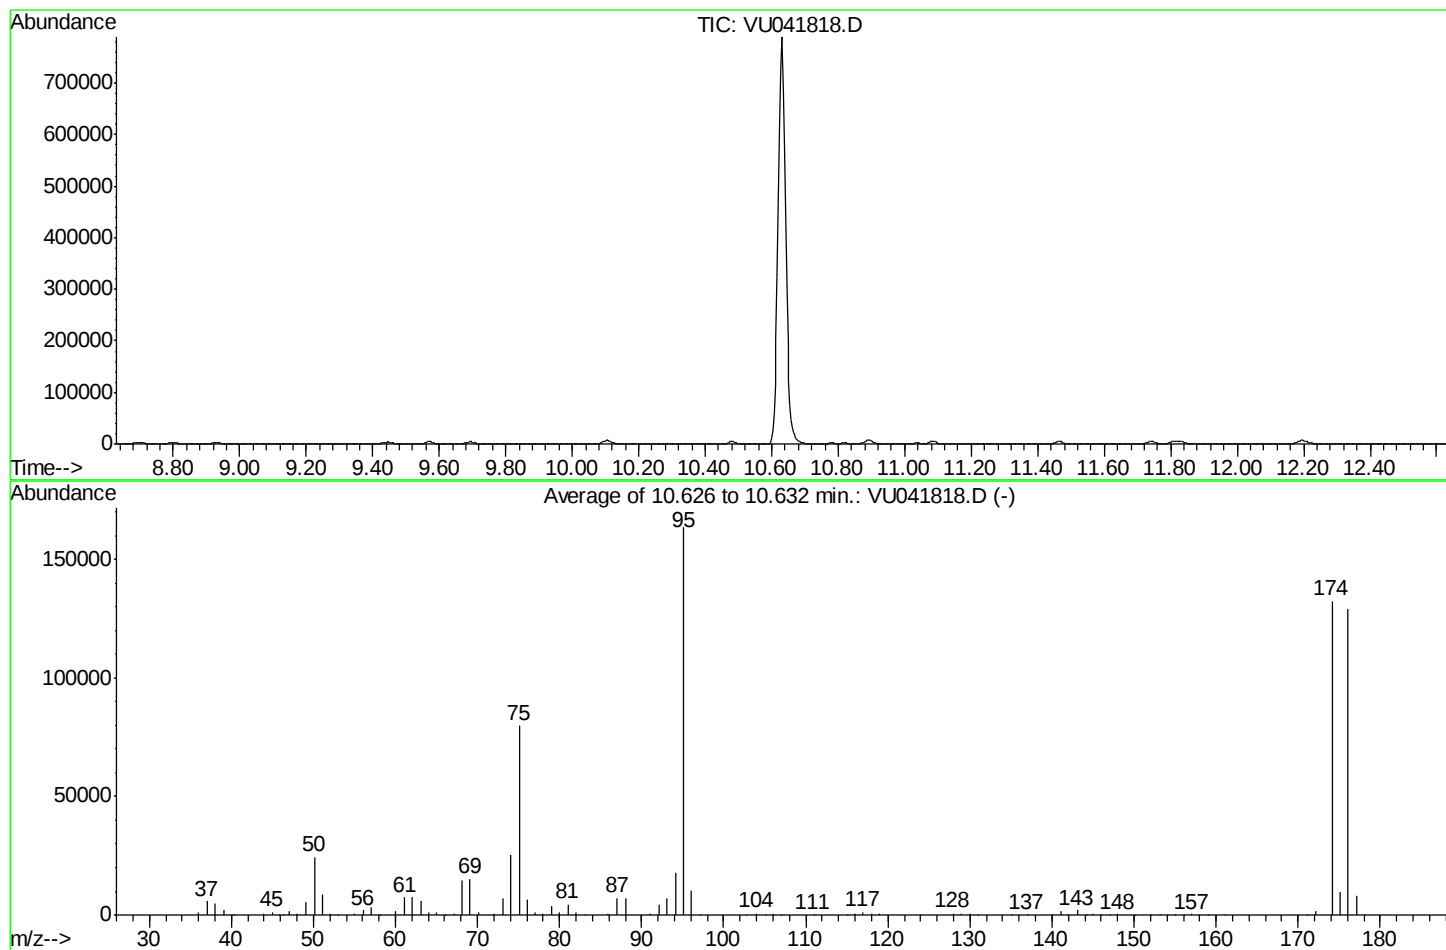

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	24565	PASS
75	95	30	80	48.7	79626	PASS
95	95	100	100	100.0	163456	PASS
96	95	5	9	6.4	10525	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.9	132269	PASS
175	174	5	9	7.5	9969	PASS
176	174	95	101	97.4	128810	PASS
177	176	5	9	6.4	8185	PASS

m/z	Abundance
36.00	1152.0
37.00	5499.0
38.00	5147.0
39.10	2316.0
40.30	122.0
44.00	704.0
45.00	1032.0
45.90	196.0
47.00	1442.0
48.00	672.0
49.00	5607.0
50.10	23808.0
51.10	8319.0
52.00	288.0
52.90	176.0
54.90	404.0
56.00	1810.0
57.10	3256.0
58.10	147.0
60.00	1436.0
61.10	7358.0
62.10	7158.0
63.10	5881.0
64.10	823.0
65.00	1147.0
67.00	349.0
68.10	13856.0
69.10	15101.0
70.10	960.0
72.00	773.0
73.10	6512.0
74.10	24512.0
75.10	77328.0
76.10	6350.0
77.00	762.0
78.00	607.0
79.00	4099.0
80.00	1251.0
81.00	4200.0
82.00	905.0
83.10	122.0
86.00	363.0
87.00	7119.0
88.10	6731.0
91.00	562.0
92.10	4028.0
93.10	6305.0
94.10	17184.0
95.10	155584.0
96.10	10144.0
97.00	135.0
102.80	104.0
104.00	657.0
105.00	218.0
106.00	614.0
107.00	125.0
115.10	112.0
116.00	547.0
117.00	1180.0
118.00	606.0
119.00	791.0
123.90	111.0
128.00	542.0
128.90	306.0
130.00	527.0
131.00	232.0
134.90	164.0
137.00	239.0
140.00	111.0
141.00	1381.0
141.90	184.0
143.10	1761.0
144.10	120.0
145.00	582.0
146.00	200.0
147.00	139.0
148.00	322.0
154.00	109.0
155.10	201.0
156.00	107.0
157.00	235.0
157.90	157.0
159.00	135.0
171.00	322.0
172.10	1507.0
174.10	123784.0
175.10	9300.0
176.10	120640.0
177.10	7782.0
178.00	168.0

Instrument :
MSVOA_U
ClientSampleId :
BFB351

m/z	Abundance
36.00	1268.0
37.00	5857.0
38.00	5285.0
39.10	2380.0
40.00	160.0
44.00	698.0
45.00	1168.0
45.80	226.0
47.10	1520.0
48.00	751.0
49.00	5553.0
50.10	25272.0
51.10	8977.0
52.00	341.0
52.90	206.0
55.00	443.0
56.10	1929.0
57.10	3454.0
58.00	165.0
60.00	1453.0
61.10	7841.0
62.10	7630.0
63.10	6083.0
64.10	945.0
65.00	1080.0
66.00	108.0
67.10	398.0
68.10	15019.0
69.10	15810.0
70.10	1020.0
72.00	772.0
73.10	7116.0
74.10	26208.0
75.10	82504.0
76.10	6920.0
77.00	862.0
77.90	620.0
79.00	4056.0
80.00	1297.0
81.00	4796.0
82.00	1005.0
83.10	119.0
86.00	311.0
87.00	7540.0
88.10	7326.0
91.00	676.0
92.10	4193.0
93.10	7123.0
94.10	18272.0
95.10	168832.0
96.10	10739.0
97.10	224.0
102.80	110.0
104.00	724.0
105.00	236.0
106.00	664.0
107.00	146.0
115.10	114.0
116.00	539.0
117.00	1266.0
118.00	567.0
119.00	860.0
123.90	114.0
128.00	667.0
128.90	346.0
130.00	575.0
131.00	252.0
135.00	225.0
137.00	220.0
140.00	134.0
141.00	1480.0
141.90	178.0
143.10	1959.0
144.10	114.0
145.10	557.0
146.00	229.0
146.90	125.0
148.00	398.0
150.10	128.0
152.00	115.0
153.00	133.0
155.10	259.0
156.10	145.0
157.00	309.0
158.00	136.0
159.00	148.0
171.10	306.0
172.10	1571.0
174.10	136576.0
175.10	10262.0
176.10	133056.0
177.10	8404.0

Instrument :
MSVOA_U
ClientSampleId :
BFB351

178.10

196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB351

m/z	Abundance
36.00	1175.0
37.10	5750.0
38.00	4968.0
39.10	2287.0
40.00	259.0
44.00	706.0
45.00	1068.0
45.90	150.0
46.20	175.0
47.10	1511.0
48.00	910.0
49.10	5247.0
50.10	24616.0
51.10	8472.0
52.00	383.0
52.90	198.0
55.00	435.0
56.10	2087.0
57.10	3455.0
58.00	176.0
60.10	1332.0
61.10	7257.0
62.10	7276.0
63.10	5722.0
64.10	837.0
65.10	991.0
66.10	106.0
67.20	433.0
68.10	14624.0
69.10	15201.0
70.10	1002.0
72.00	722.0
73.10	7021.0
74.10	25448.0
75.10	79048.0
76.10	6826.0
77.00	893.0
77.90	587.0
79.00	3714.0
80.00	1273.0
81.00	4695.0
82.00	1034.0
85.90	283.0
87.00	7073.0
88.10	7139.0
91.00	682.0
92.10	4182.0
93.10	7317.0
94.10	17784.0
95.10	165952.0
96.10	10693.0
97.10	270.0
104.00	670.0
105.00	220.0
106.00	613.0
107.00	141.0
111.00	140.0
115.00	128.0
116.10	529.0
117.00	1139.0
118.00	440.0
119.00	830.0
128.00	642.0
128.90	326.0
130.00	556.0
131.00	263.0
135.10	245.0
137.00	220.0
140.00	117.0
141.10	1525.0
141.90	199.0
143.10	2020.0
144.20	103.0
145.10	561.0
146.00	277.0
146.90	101.0
148.00	457.0
150.10	192.0
152.00	102.0
153.10	154.0
155.00	289.0
156.10	122.0
157.10	368.0
159.00	172.0
161.10	140.0
171.10	232.0
172.10	1478.0
174.10	136448.0
175.10	10346.0
176.10	132736.0
177.10	8371.0
178.10	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB351

m/z	Abundance
44.00	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB351