


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122821\
 Data File : VU046613.D
 Acq On : 28 Dec 2021 09:09
 Operator : SY/MD
 Sample : BFB037
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB037

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 30 04:21:35 2021

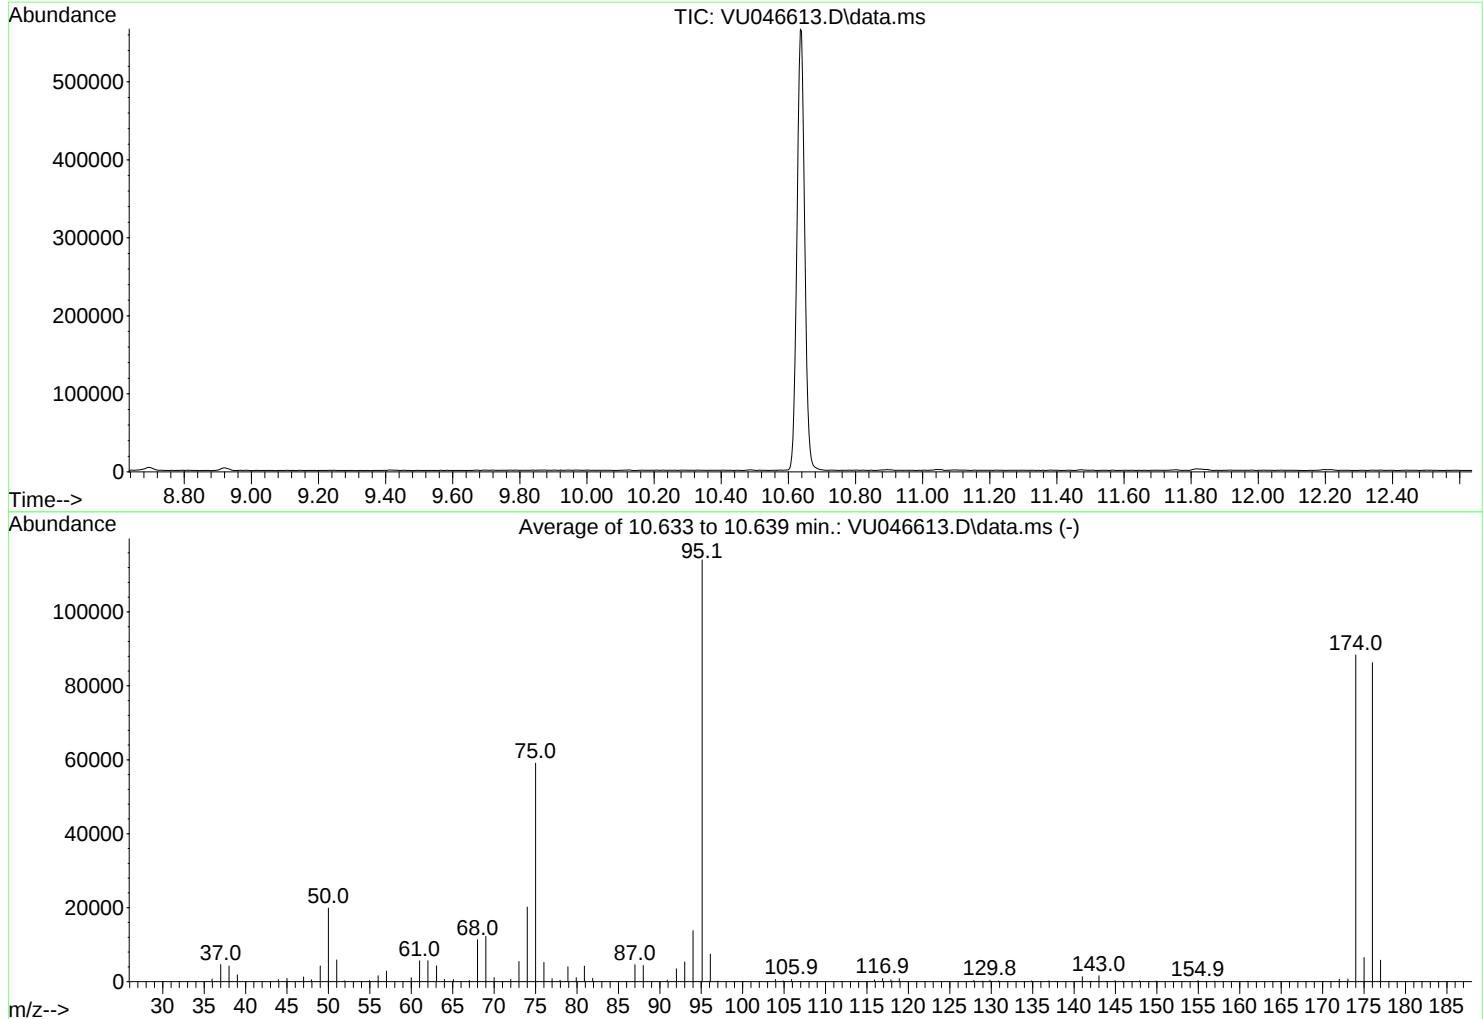

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	19923	PASS
75	95	30	80	51.8	59080	PASS
95	95	100	100	100.0	114088	PASS
96	95	5	9	6.5	7431	PASS
173	174	0.00	2	0.9	754	PASS
174	95	50	120	77.5	88368	PASS
175	174	5	9	7.4	6530	PASS
176	174	95	101	97.6	86291	PASS
177	176	5	9	6.7	5792	PASS

m/z	Abundance
35.90	218.0
39.90	1957.0
43.90	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
36.00	968.0
37.00	4512.0
38.00	3918.0
39.00	1823.0
39.90	1781.0
44.00	727.0
45.00	844.0
45.90	116.0
47.00	1193.0
47.90	618.0
49.00	4019.0
50.00	19248.0
51.00	5511.0
51.90	249.0
55.00	292.0
56.00	1536.0
57.00	2709.0
58.00	122.0
60.00	1025.0
61.00	5338.0
62.00	5417.0
63.10	4076.0
64.00	623.0
65.10	635.0
67.00	286.0
68.00	10898.0
69.00	11712.0
70.00	951.0
72.00	580.0
73.00	5031.0
74.00	19496.0
75.00	56208.0
76.00	4975.0
77.00	770.0
78.00	341.0
78.90	3771.0
79.90	1075.0
80.90	3967.0
81.90	902.0
87.00	4404.0
88.00	3994.0
90.90	423.0
92.00	3460.0
93.00	5078.0
94.00	12912.0
95.10	107040.0
96.10	7194.0
97.00	183.0
103.90	531.0
104.90	212.0
105.90	546.0
106.90	103.0
115.90	430.0
116.90	872.0
117.90	491.0
118.90	832.0
127.90	386.0
128.90	190.0
129.80	372.0
130.90	183.0
134.90	216.0
137.00	236.0
141.00	1315.0
141.90	179.0
143.00	1585.0
143.90	107.0
144.90	344.0
145.90	189.0
147.90	230.0
149.90	150.0
155.00	254.0
156.90	166.0
158.90	145.0
160.90	123.0
170.90	115.0
172.00	677.0
173.00	689.0
174.00	81784.0
175.00	6106.0
176.00	79808.0
177.00	5431.0
178.00	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
36.00	984.0
37.00	4800.0
38.00	4333.0
39.00	1884.0
39.90	1729.0
44.00	777.0
45.00	877.0
45.90	112.0
47.00	1292.0
47.90	553.0
49.00	4371.0
50.00	20584.0
51.00	6058.0
51.90	288.0
54.90	297.0
56.00	1677.0
57.00	2940.0
58.00	157.0
60.00	1081.0
61.00	5762.0
62.00	5872.0
63.00	4425.0
64.00	608.0
65.10	584.0
67.00	325.0
68.00	11636.0
69.00	12645.0
70.00	1132.0
72.00	636.0
73.00	5661.0
74.00	20848.0
75.00	61016.0
76.00	5408.0
77.00	871.0
77.90	379.0
78.90	4157.0
79.90	1121.0
80.90	4308.0
81.90	913.0
82.90	112.0
87.00	4798.0
88.00	4513.0
90.90	432.0
92.00	3568.0
93.00	5518.0
94.00	14225.0
95.10	117864.0
96.10	7697.0
97.00	202.0
104.00	570.0
104.90	228.0
105.90	642.0
110.90	121.0
113.00	119.0
115.90	479.0
116.90	930.0
117.90	527.0
118.90	881.0
127.90	399.0
128.90	177.0
129.90	426.0
130.90	213.0
134.90	231.0
137.00	209.0
141.00	1328.0
141.90	150.0
143.00	1620.0
143.90	103.0
144.90	319.0
145.90	170.0
147.90	263.0
149.90	165.0
154.90	329.0
157.00	212.0
159.00	155.0
161.00	106.0
172.00	697.0
173.10	783.0
174.00	91056.0
175.00	6798.0
176.00	89032.0
177.00	6011.0
178.00	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037

m/z	Abundance
36.00	956.0
37.00	4564.0
38.00	4492.0
39.00	1723.0
40.00	1681.0
44.00	728.0
45.00	832.0
46.00	109.0
47.00	1250.0
48.00	454.0
49.00	4337.0
50.00	19936.0
51.00	6059.0
51.90	285.0
54.90	301.0
56.00	1647.0
57.00	2964.0
58.00	171.0
60.00	1000.0
61.00	5779.0
62.00	5706.0
63.00	4339.0
64.00	535.0
65.10	531.0
67.00	316.0
68.00	11480.0
69.00	12414.0
70.00	1127.0
72.00	639.0
73.00	5662.0
74.00	20144.0
75.00	60016.0
76.00	5229.0
77.00	862.0
77.90	409.0
78.90	4128.0
79.90	1025.0
80.90	4265.0
81.90	889.0
82.90	133.0
86.00	147.0
87.00	4582.0
88.00	4662.0
90.90	398.0
92.00	3424.0
93.00	5407.0
94.00	14321.0
95.10	117360.0
96.10	7403.0
97.00	206.0
104.00	573.0
104.90	218.0
105.90	690.0
110.90	139.0
111.90	103.0
113.00	124.0
114.90	101.0
115.90	474.0
116.90	855.0
117.90	513.0
118.90	829.0
127.90	429.0
128.90	170.0
129.90	428.0
130.90	218.0
134.90	240.0
136.90	163.0
141.00	1337.0
142.10	128.0
143.00	1551.0
145.00	272.0
145.90	160.0
147.90	292.0
149.90	172.0
152.90	118.0
154.90	359.0
157.00	217.0
159.00	160.0
161.00	115.0
172.00	691.0
173.10	791.0
174.00	92264.0
175.00	6687.0
176.00	90032.0
177.00	5933.0
178.00	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB037