




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
 Data File : VU052596.D
 Acq On : 28 Dec 2022 18:39
 Operator : JC/MD
 Sample : N6216-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:28:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 29 00:24:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/30/2022
 Supervised By :Mahesh Dadoda 12/30/2022

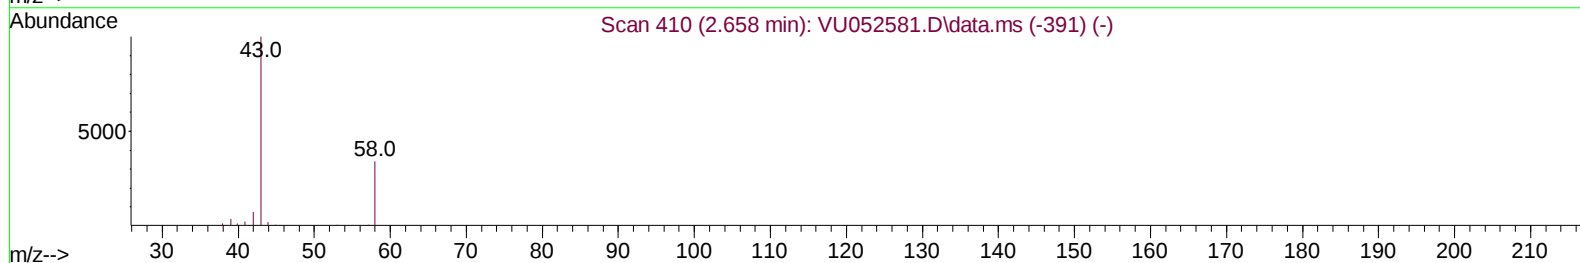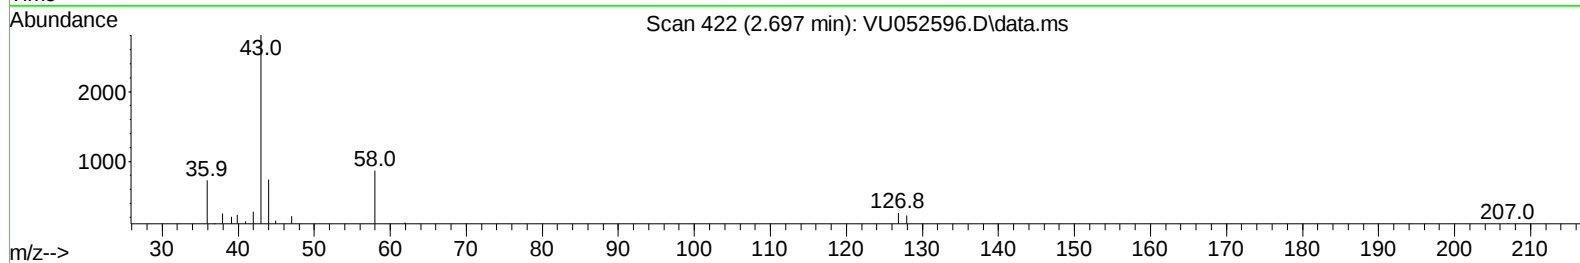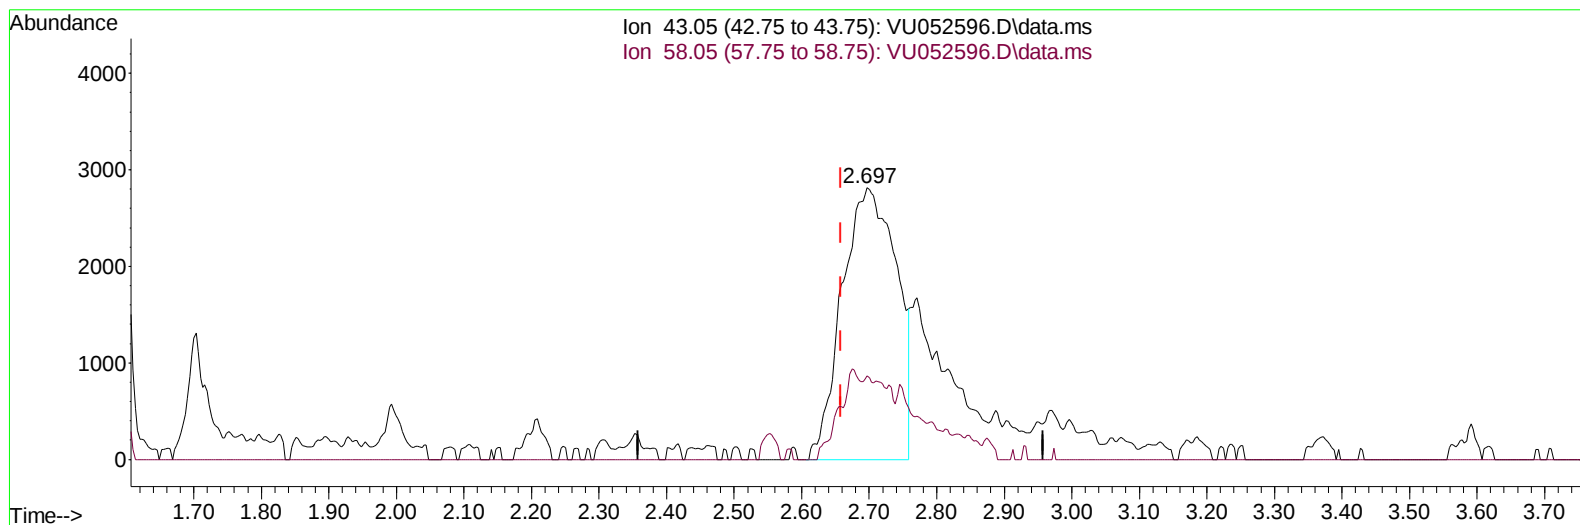

TIC: VU052596.D\data.ms

(13) Acetone (T)

2.697min (+ 0.039) 3.61 ug/L

response 15718

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.70	12.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
 Data File : VU052596.D
 Acq On : 28 Dec 2022 18:39
 Operator : JC/MD
 Sample : N6216-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:28:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 29 00:24:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/30/2022
 Supervised By :Mahesh Dadoda 12/30/2022

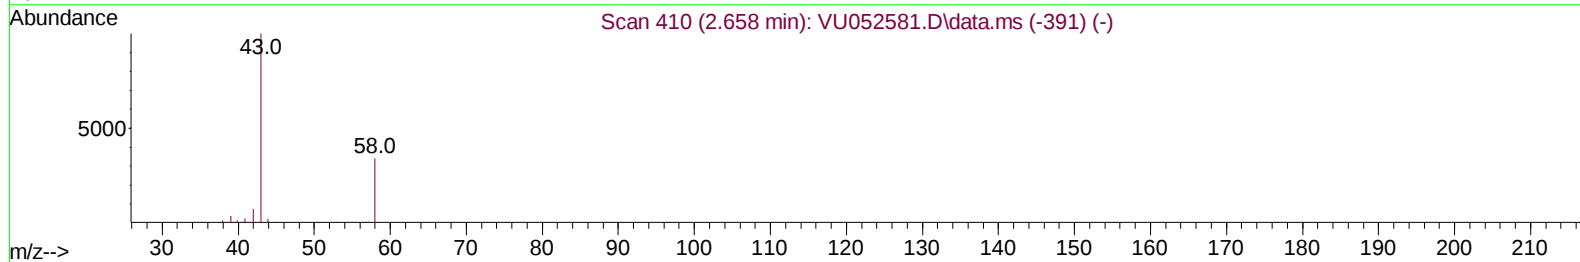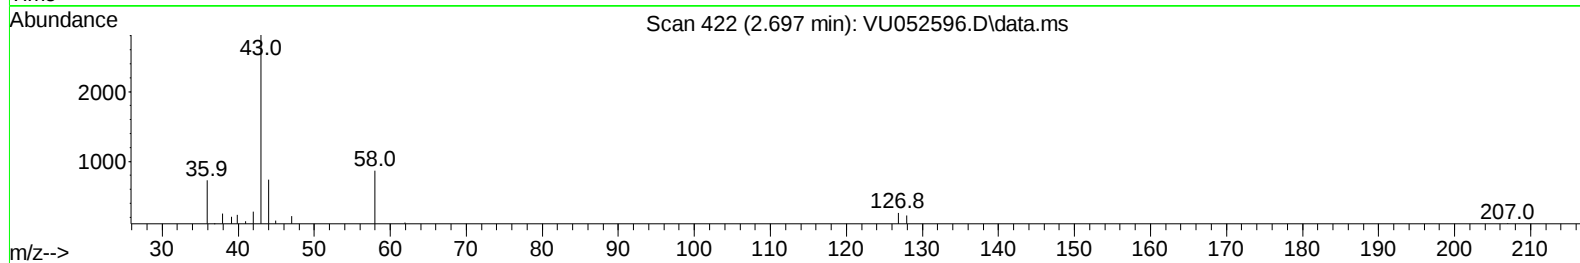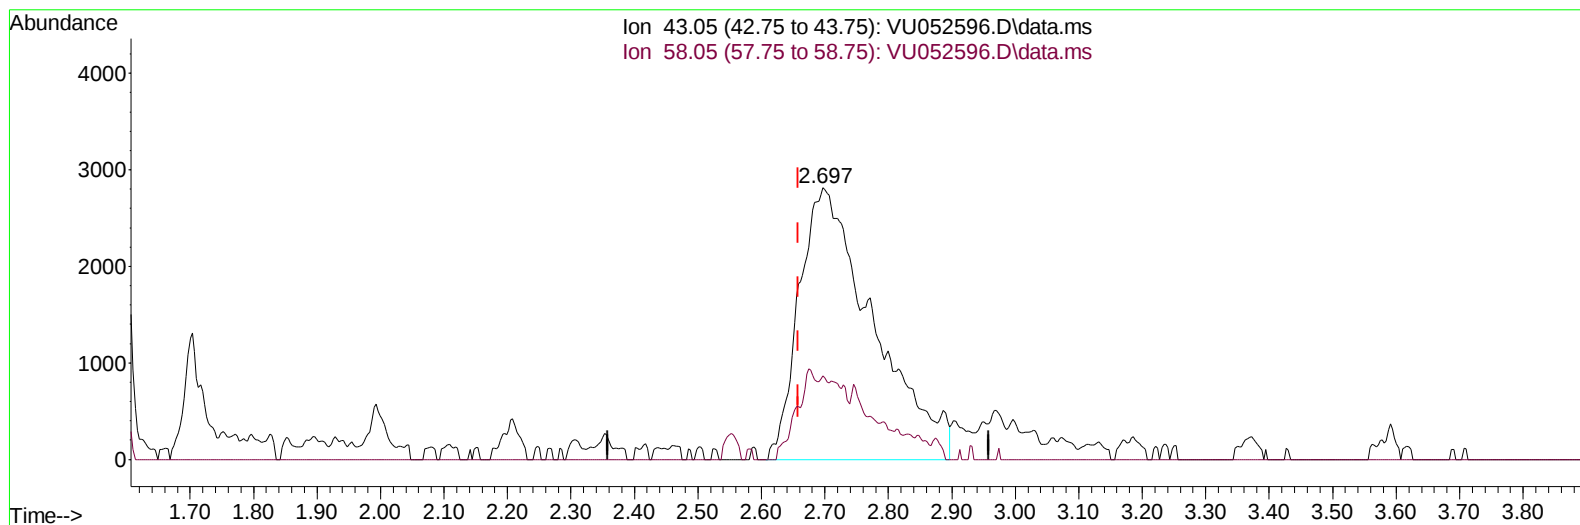

TIC: VU052596.D\data.ms

(13) Acetone (T)

2.697min (+ 0.039) 5.21 ug/L m

response 22697

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.70	8.91
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
 Data File : VU052596.D
 Acq On : 28 Dec 2022 18:39
 Operator : JC/MD
 Sample : N6216-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:28:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 29 00:24:48 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/30/2022
 Supervised By :Mahesh Dadoda 12/30/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.247	114		188059	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117		185055	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152		82201	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.601	65		49625	2.605	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	52.000%	
7) Chloroethane-d5	1.916	69		53495	3.256	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	65.200%	
11) 1,1-Dichloroethene-d2	2.568	65		24119	2.942	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.800%#	
20) 2-Butanone-d5	4.662	46		290286	49.133	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.260%	
24) Chloroform-d	5.060	84		128189	3.988	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.800%	
26) 1,2-Dichloroethane-d4	5.697	65		78702	4.221	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.400%	
32) Benzene-d6	5.726	84		237716	3.747	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.000%	
36) 1,2-Dichloropropane-d6	6.687	67		90083	4.125	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.400%	
41) Toluene-d8	7.893	98		175753	3.300	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.000%#	
43) trans-1,3-Dichloroprop...	8.176	79		31393	4.198	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%	
46) 2-Hexanone-d5	8.632	63		226153	55.272	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.540%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84		89463	4.825	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%	
66) 1,2-Dichlorobenzene-d4	12.189	152		74451	4.449	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.000%	
Target Compounds							
13) Acetone	2.697	43		22697m	5.211	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
Data File : VU052596.D
Acq On : 28 Dec 2022 18:39
Operator : JC/MD
Sample : N6216-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:28:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 29 00:24:48 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 12/30/2022
Supervised By :Mahesh Dadoda 12/30/2022

