

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
 Data File : VU052590.D
 Acq On : 28 Dec 2022 15:51
 Operator : JC/MD
 Sample : N6171-12DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBQD0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	13	rVB2	21156	17894	1.56%	0.234%
2	1.600	71	81	90	rVB	81768	97908	8.51%	1.282%
3	1.915	170	179	197	rVB	77033	104500	9.08%	1.368%
4	2.568	370	382	400	rVB	132237	218645	19.00%	2.863%
5	3.044	515	530	546	rBV2	31394	63060	5.48%	0.826%
6	4.642	1010	1027	1063	rBV	134977	489353	42.53%	6.408%
7	5.060	1141	1157	1186	rVB	143886	323388	28.11%	4.235%
8	5.722	1342	1363	1390	rBV2	287161	765726	66.56%	10.027%
9	6.246	1512	1526	1548	rBV	228443	431579	37.51%	5.651%
10	6.687	1647	1663	1690	rBV	200024	387896	33.72%	5.079%
11	7.562	1919	1935	1949	rBV	87842	157769	13.71%	2.066%
12	7.896	2026	2039	2069	rBV	318973	548992	47.72%	7.189%
13	8.176	2114	2126	2144	rBV	56506	95975	8.34%	1.257%
14	8.549	2228	2242	2256	rBV	584164	983622	85.50%	12.880%
15	8.632	2256	2268	2303	rVB	615356	1150498	100.00%	15.065%
16	9.414	2498	2511	2536	rBV	324506	534097	46.42%	6.994%
17	10.751	2914	2927	2946	rBV	168700	269528	23.43%	3.529%
18	11.806	3243	3255	3274	rBV	300202	477198	41.48%	6.249%
19	12.188	3361	3374	3390	rBV	322972	519104	45.12%	6.797%




Sum of corrected areas: 7636732

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
Data File : VU052590.D
Acq On : 28 Dec 2022 15:51
Operator : JC/MD
Sample : N6171-12DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

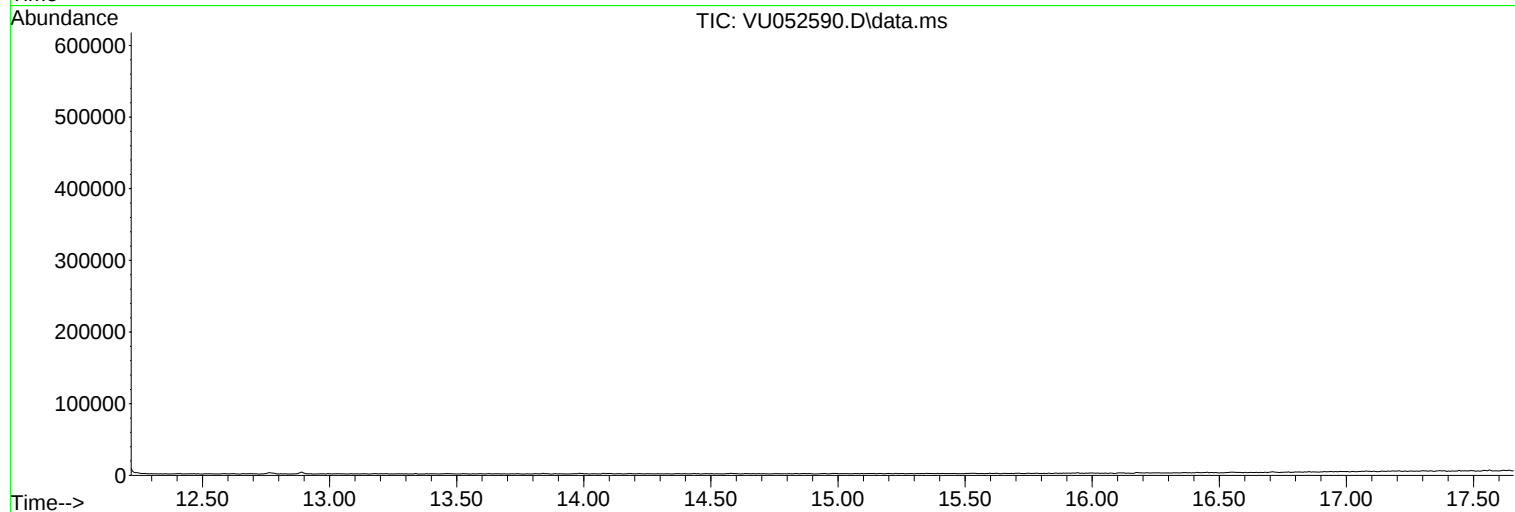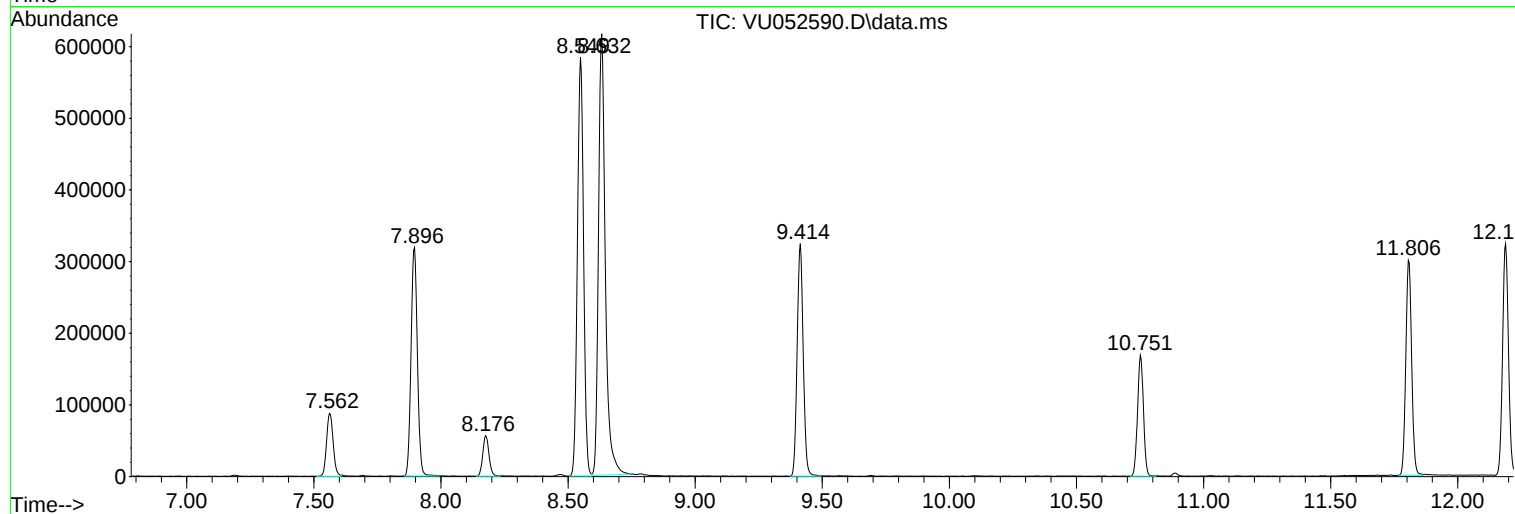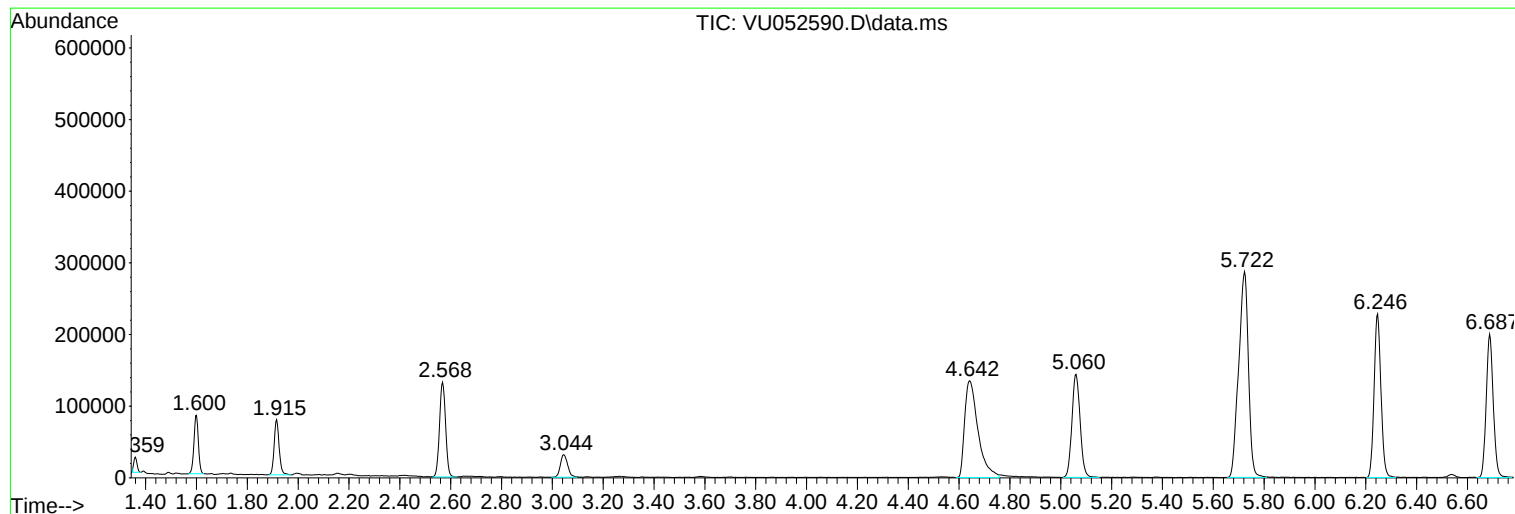

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
Data File : VU052590.D
Acq On : 28 Dec 2022 15:51
Operator : JC/MD
Sample : N6171-12DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122822\
Data File : VU052590.D
Acq On : 28 Dec 2022 15:51
Operator : JC/MD
Sample : N6171-12DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc