




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

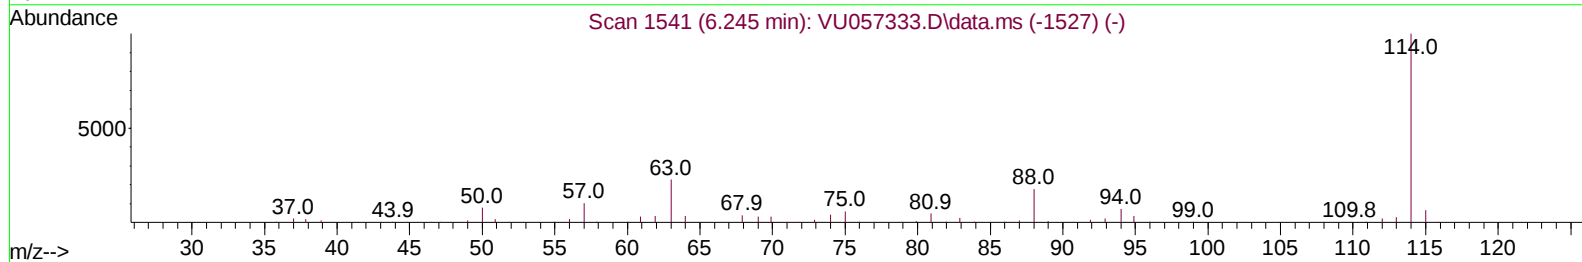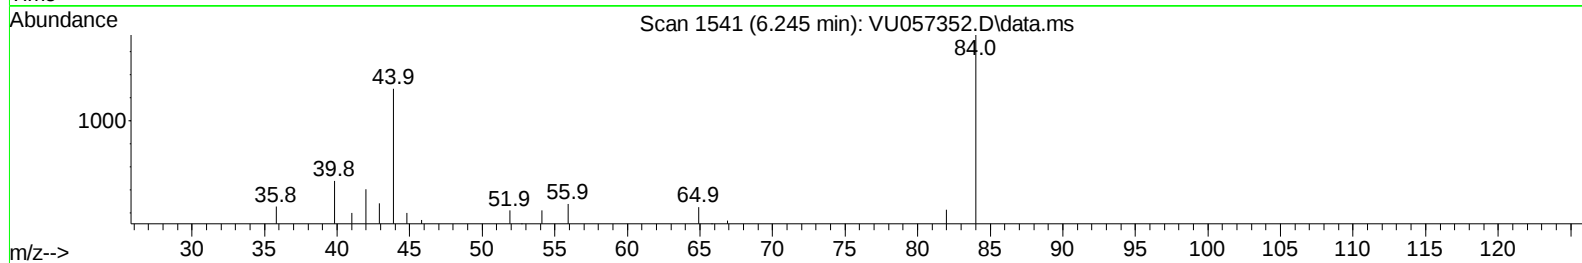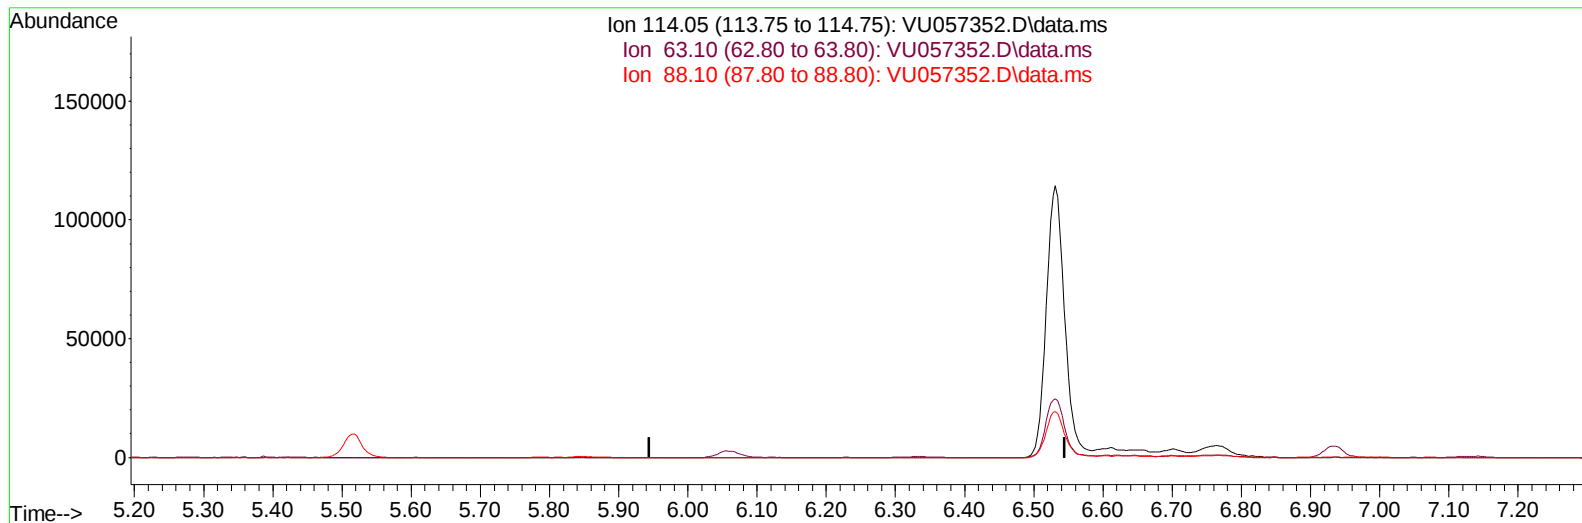

TIC: VU057352.D\data.ms

(1) 1,4-Difluorobenzene (I)

6.245min (-6.245) 0.00 ug/L

response 0

Ion	Exp%	Act%
114.05	100.00	0.00
63.10	22.00	0.00#
88.10	17.80	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057352.D
Acq On : 28 Dec 2023 22:48
Operator : MD/SY
Sample : 06020-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Y1

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

Quant Time: Dec 29 00:06:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

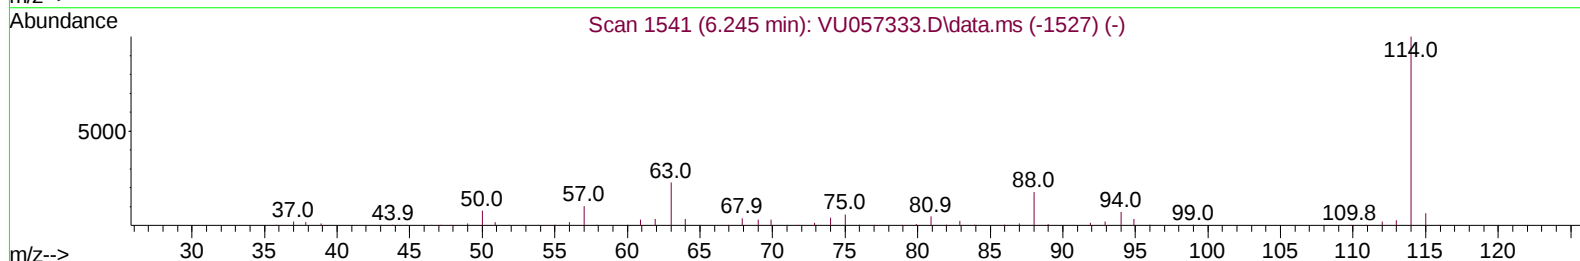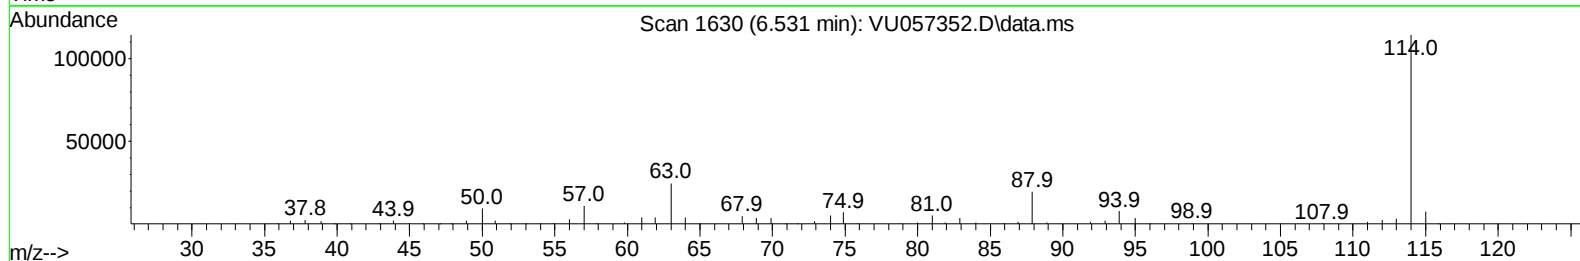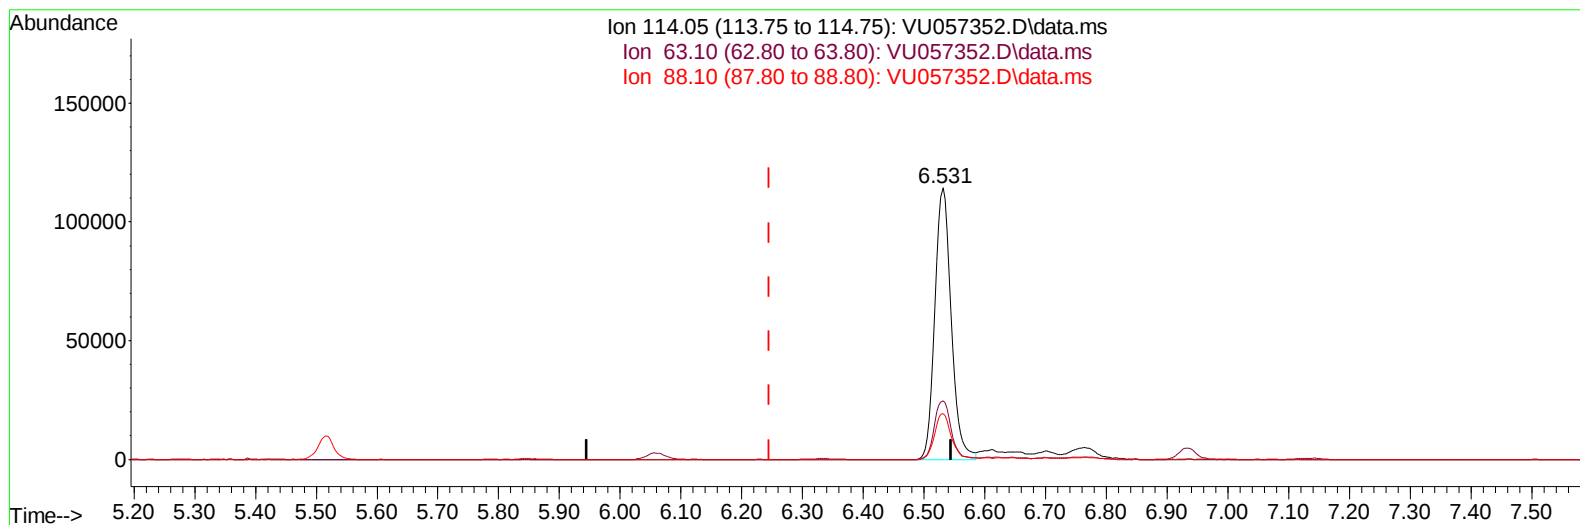

TIC: VU057352.D\data.ms

(1) 1,4-Difluorobenzene (I)

6.531min (+ 0.286) 5.00 ug/L m

response 210727

Ion	Exp%	Act%
114.05	100.00	100.00
63.10	22.00	0.00#
88.10	17.80	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057352.D
Acq On : 28 Dec 2023 22:48
Operator : MD/SY
Sample : 06020-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

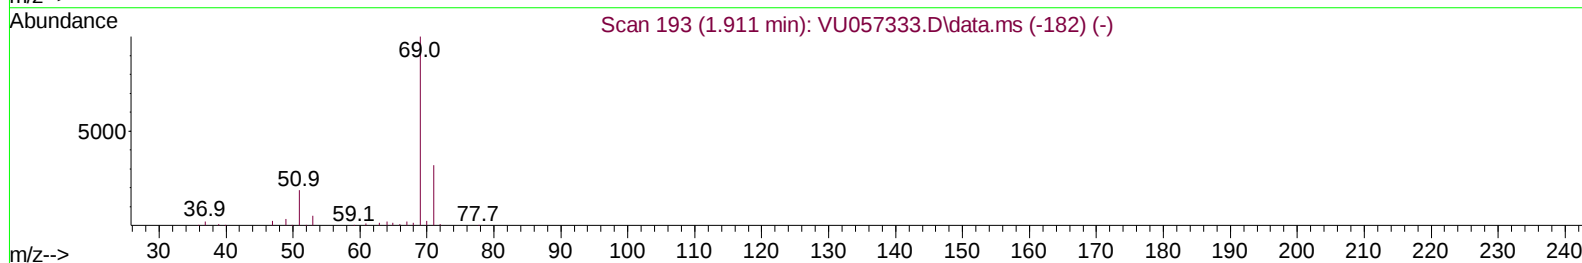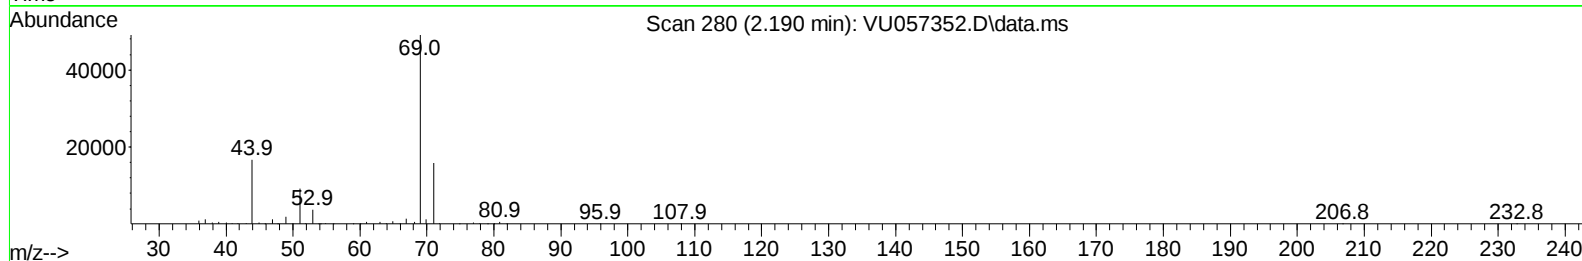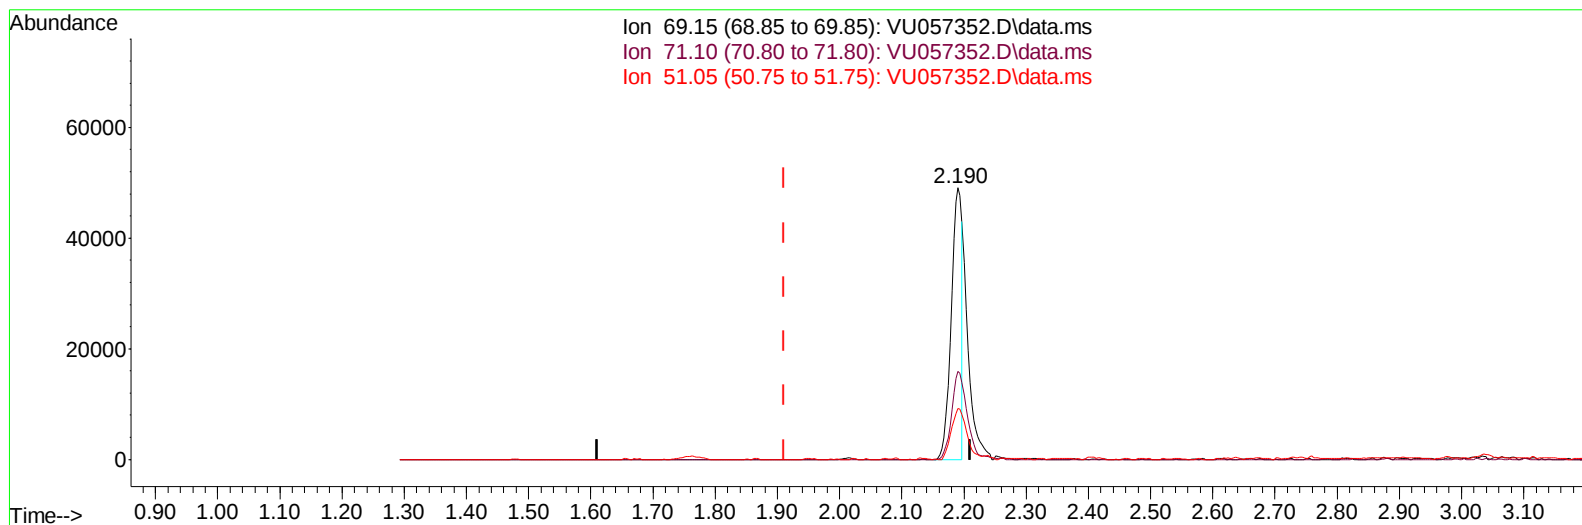

TIC: VU057352.D\data.ms

(7) Chloroethane-d5 (S)

2.190min (+ 0.280) 4.06 ug/L

response 59025

Ion	Exp%	Act%
69.15	100.00	100.00
71.10	31.90	31.33
51.05	25.10	18.73
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057352.D
Acq On : 28 Dec 2023 22:48
Operator : MD/SY
Sample : 06020-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

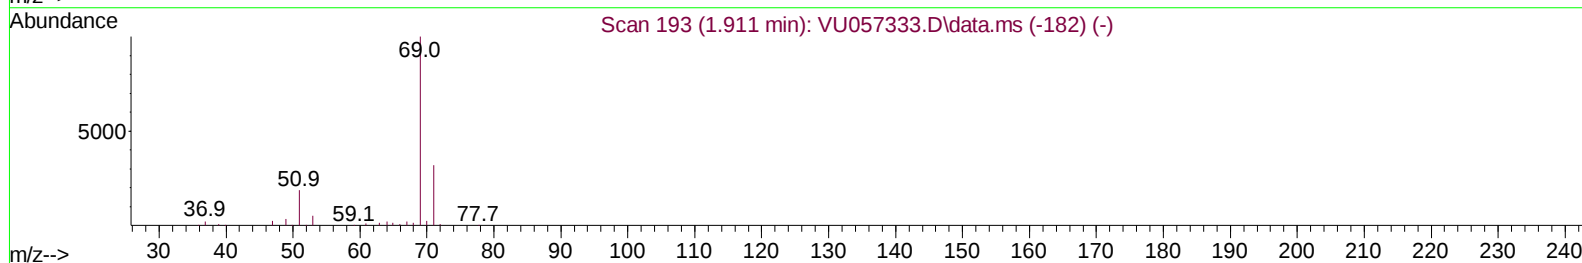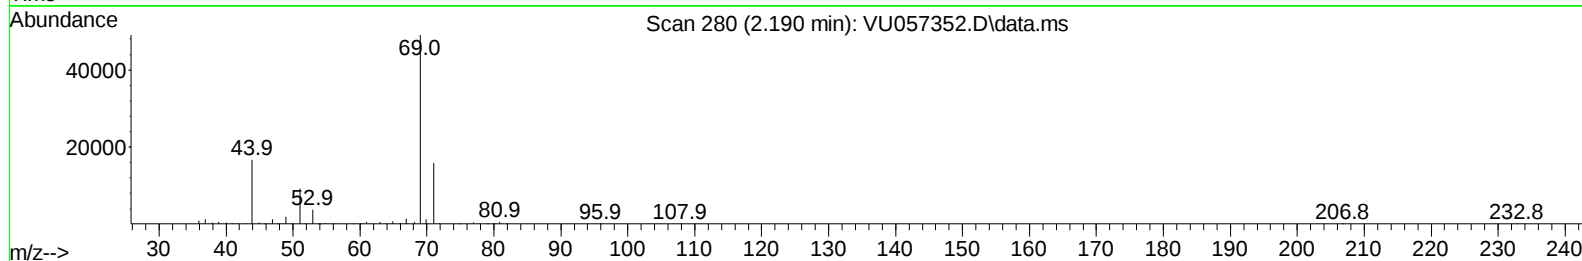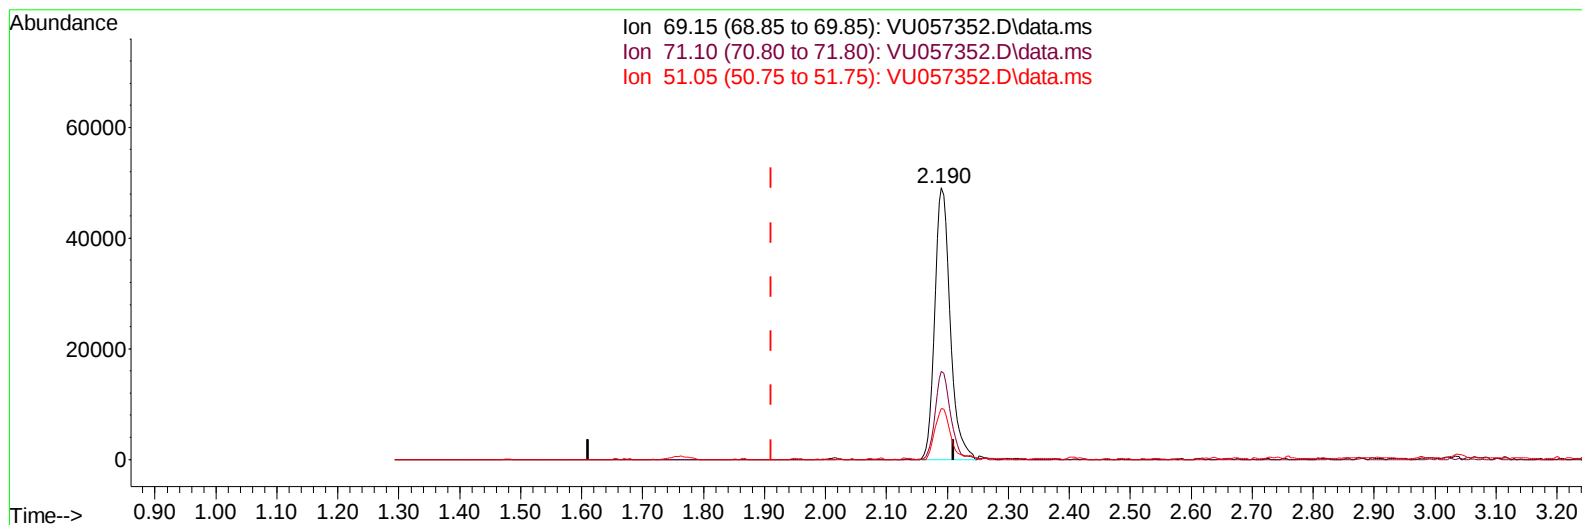

TIC: VU057352.D\data.ms

(7) Chloroethane-d5 (S)

2.190min (+ 0.280) 5.84 ug/L m

response 84959

Ion	Exp%	Act%
69.15	100.00	100.00
71.10	31.90	21.77#
51.05	25.10	13.01#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057352.D
Acq On : 28 Dec 2023 22:48
Operator : MD/SY
Sample : 06020-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

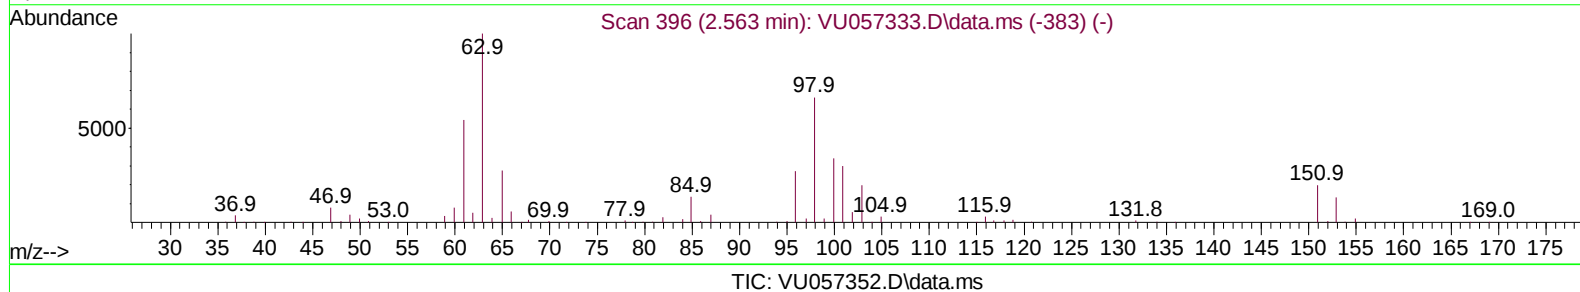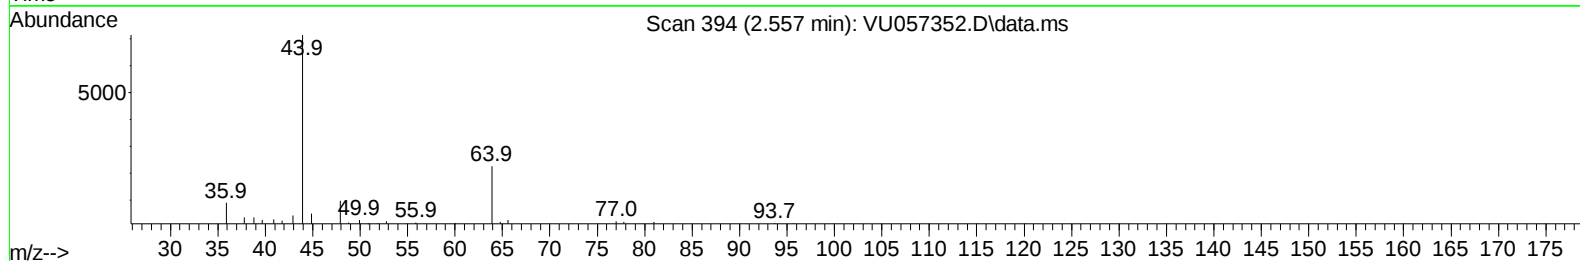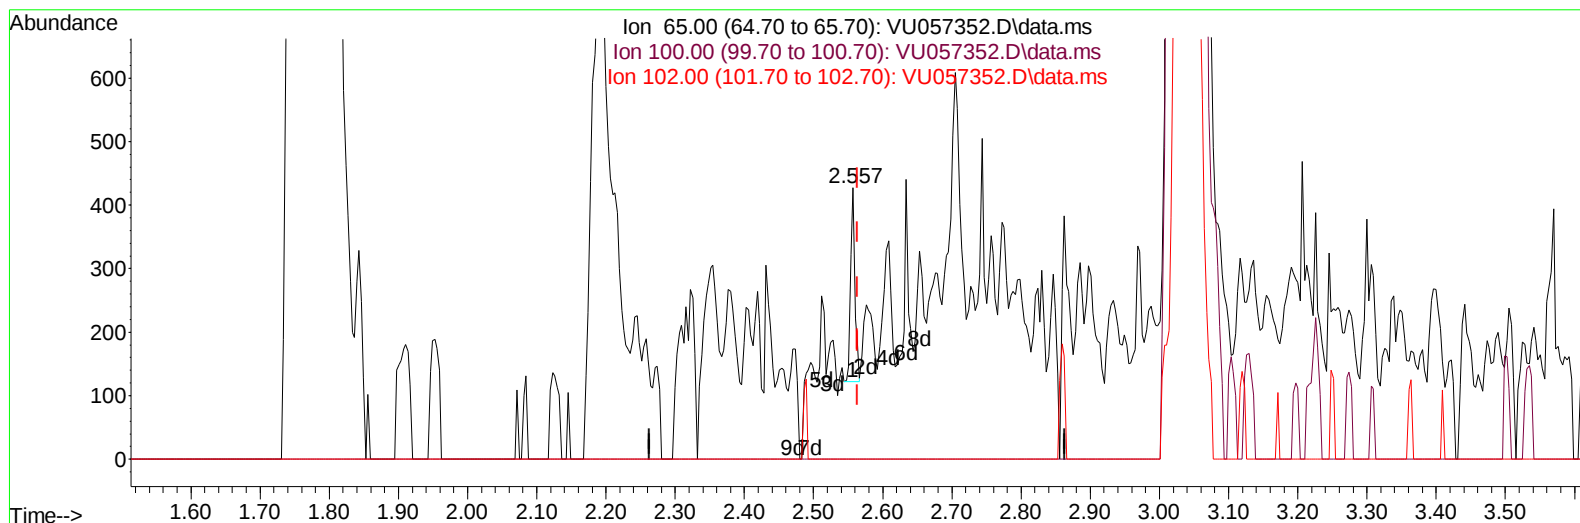

(11) 1,1-Dichloroethene-d2 (S)

2.557min (-0.006) 0.02 ug/L

response 134

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	138.90	0.00#
102.00	21.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057352.D
Acq On : 28 Dec 2023 22:48
Operator : MD/SY
Sample : 06020-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

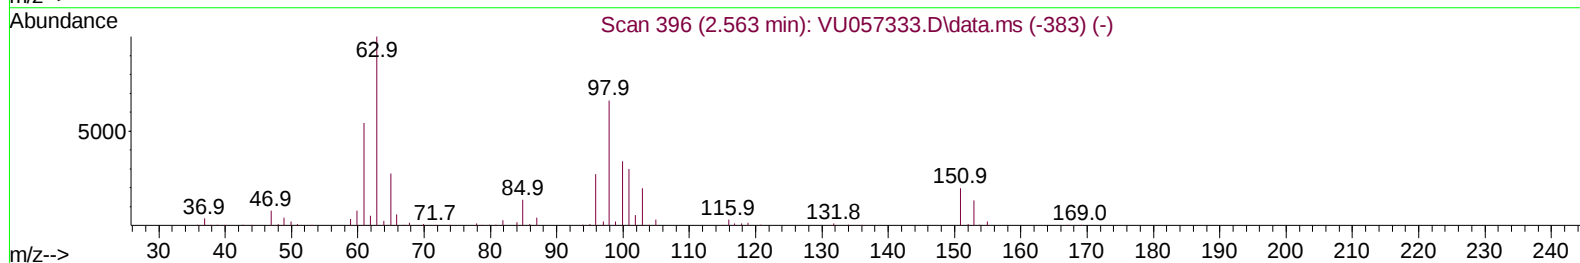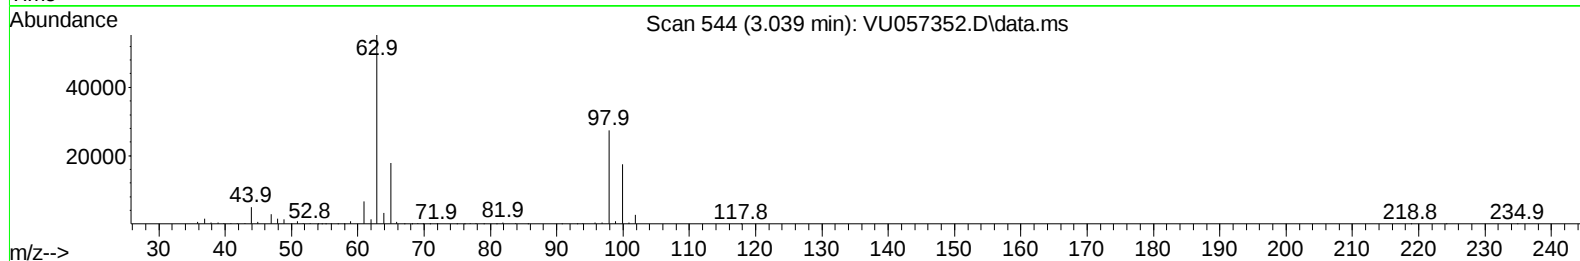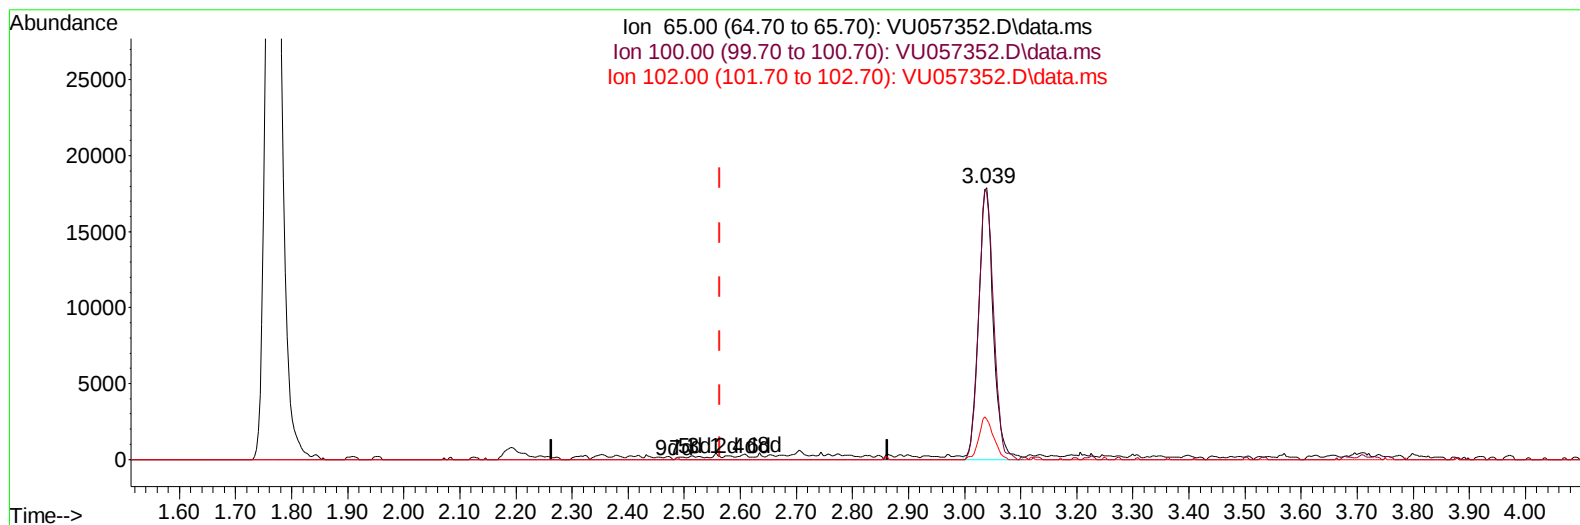

TIC: VU057352.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.039min (+ 0.476) 4.53 ug/L m

response 32631

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	138.90	0.00#
102.00	21.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

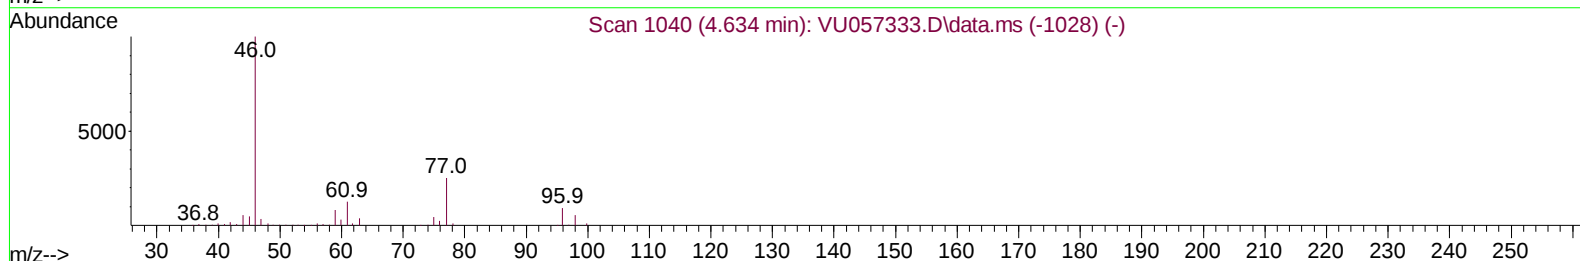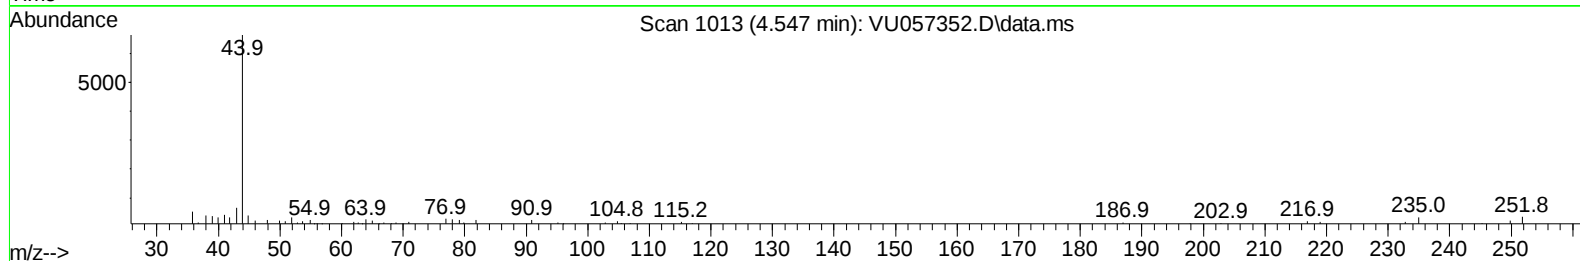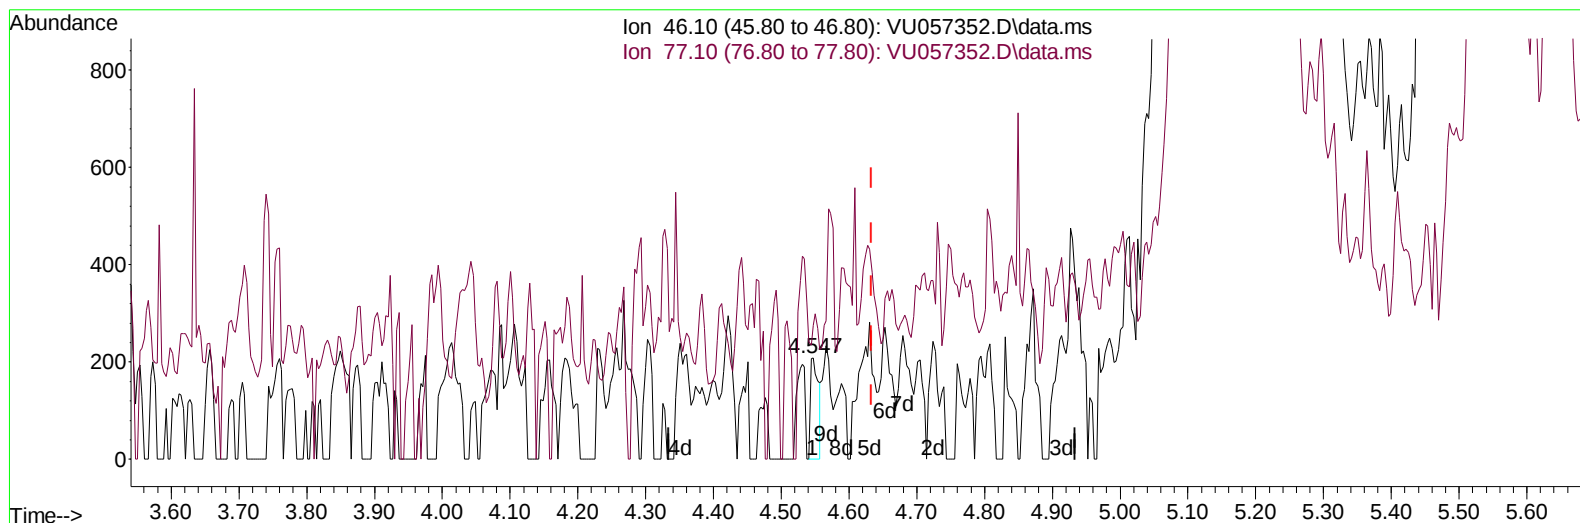

TIC: VU057352.D\data.ms

(20) 2-Butanone-d5 (S)

4.547min (-0.087) 0.04 ug/L

response 176

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.80	20.45
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

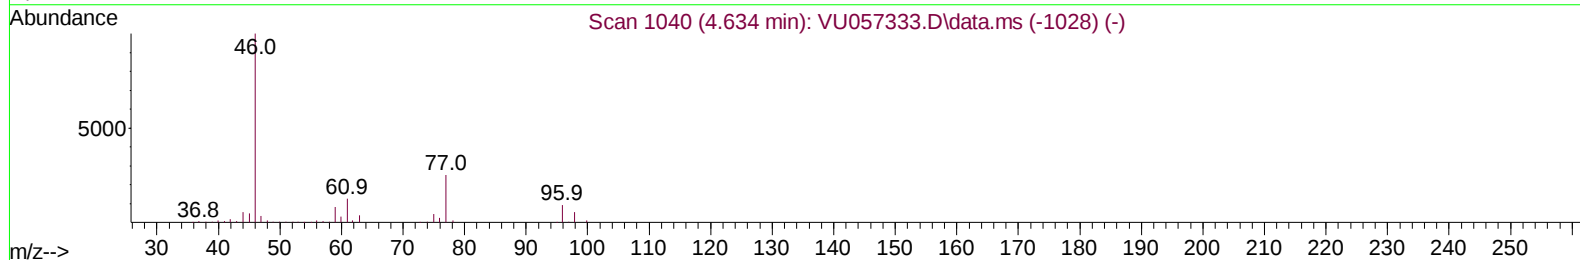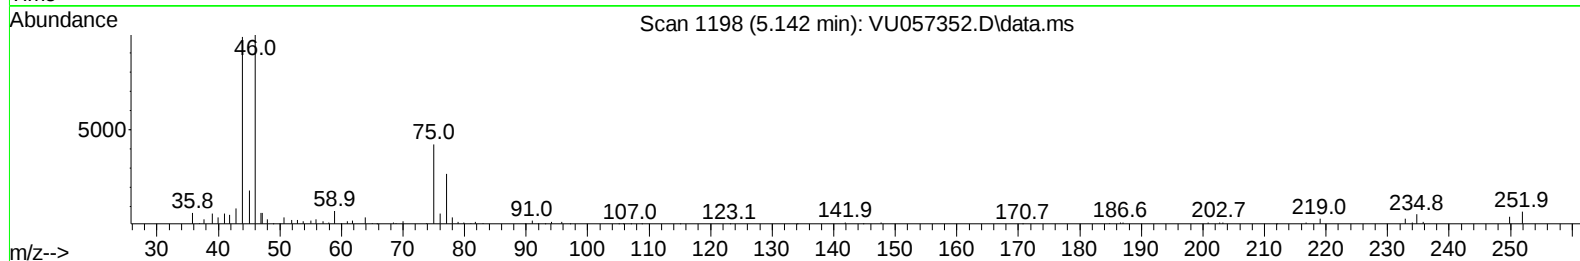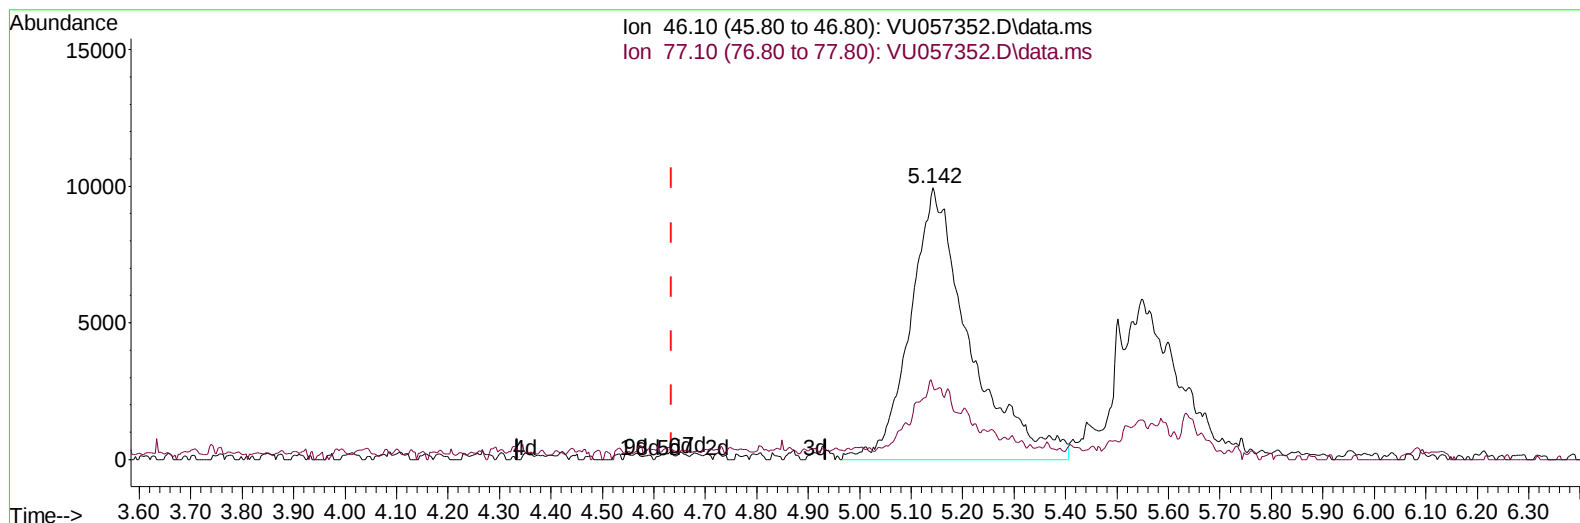

TIC: VU057352.D\data.ms

(20) 2-Butanone-d5 (S)

5.142min (+ 0.508) 19.38 ug/L m

response 79518

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	25.80	0.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

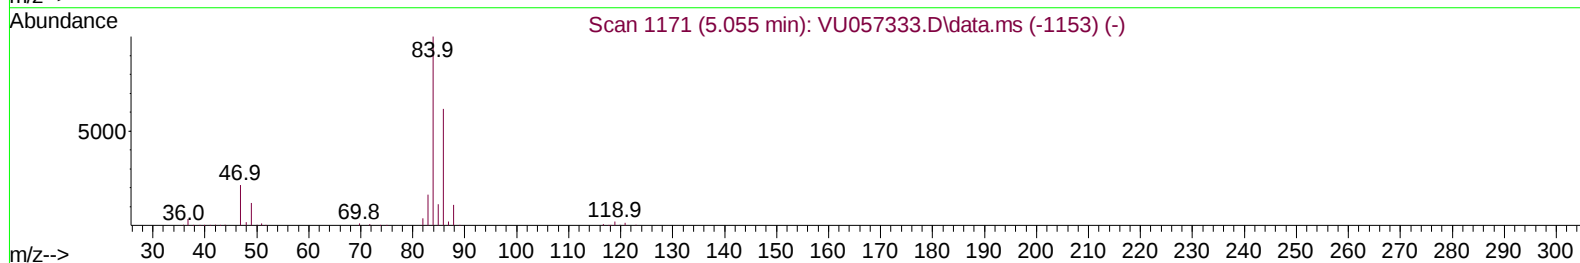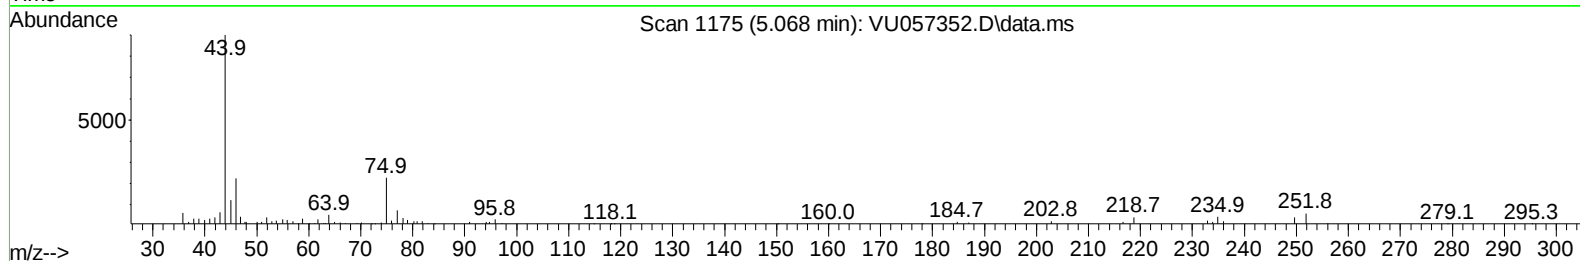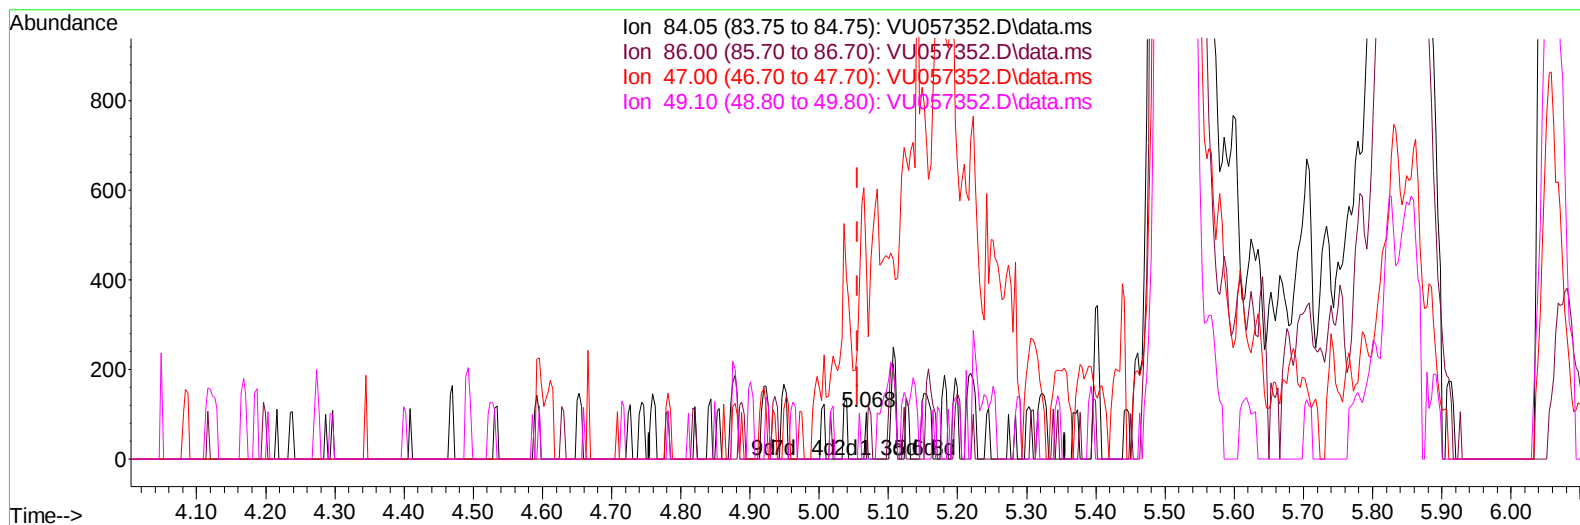

TIC: VU057352.D\data.ms

(24) Chloroform-d (S)

5.068min (+ 0.013) 0.00 ug/L

response 20

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	63.90	215.00#
47.00	38.50	1280.00#
49.10	23.40	100.00#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

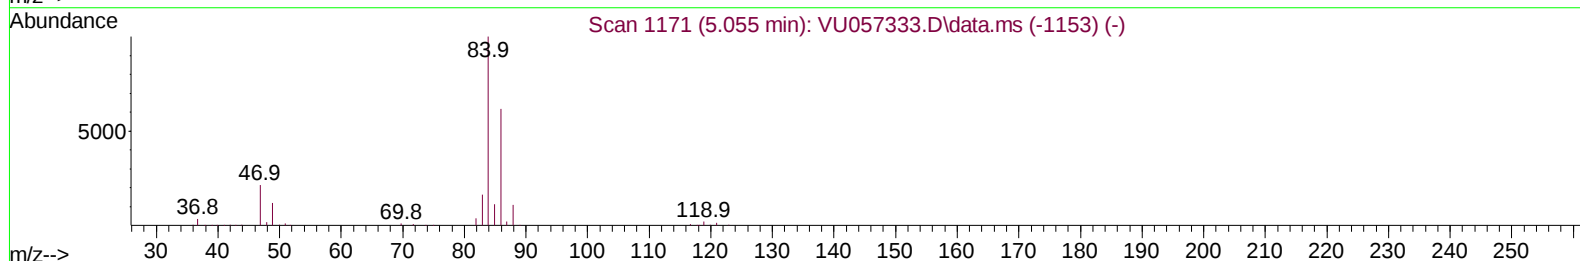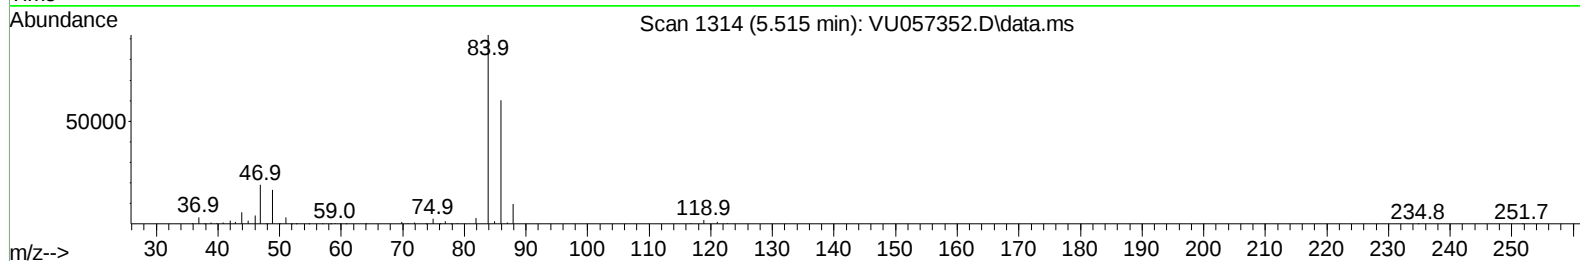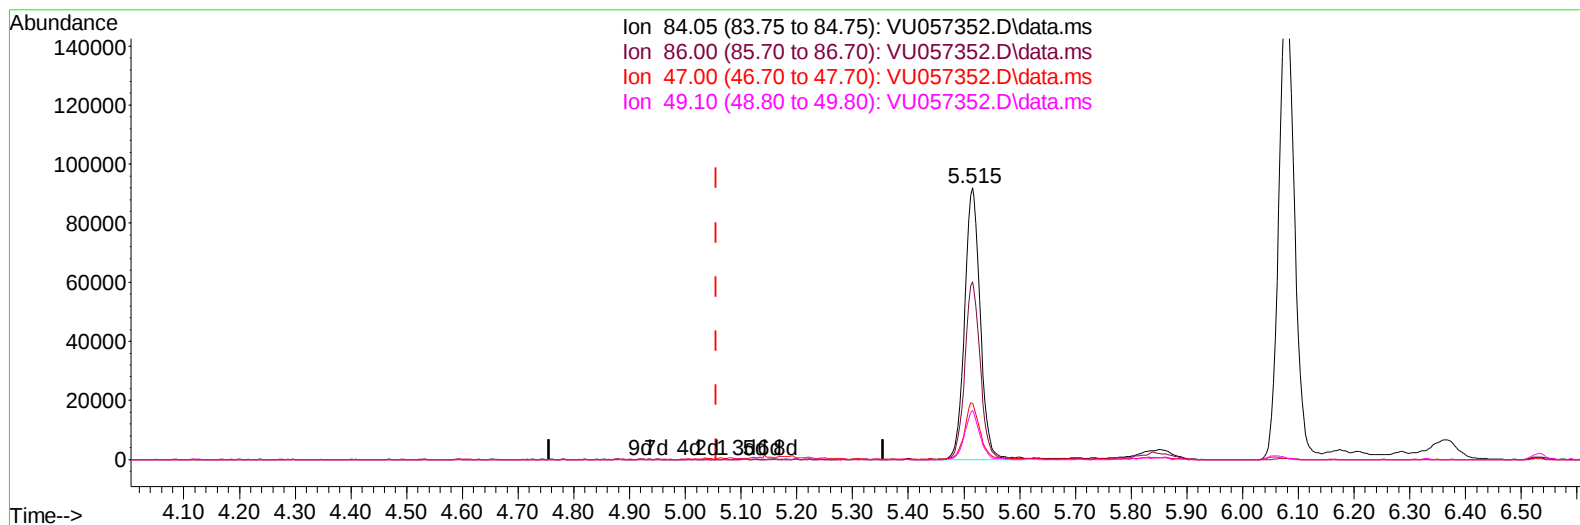

TIC: VU057352.D\data.ms

(24) Chloroform-d (S)

5.515min (+ 0.460) 5.56 ug/L m

response 179055

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	63.90	0.02#
47.00	38.50	0.14#
49.10	23.40	0.01#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

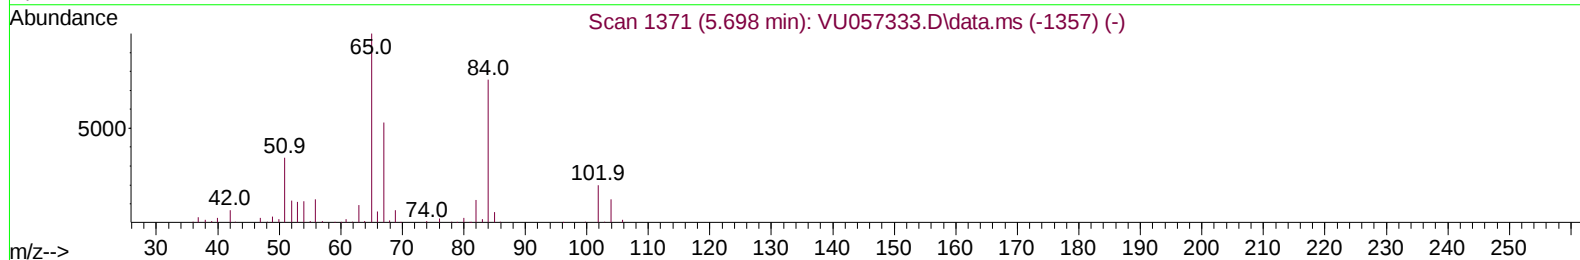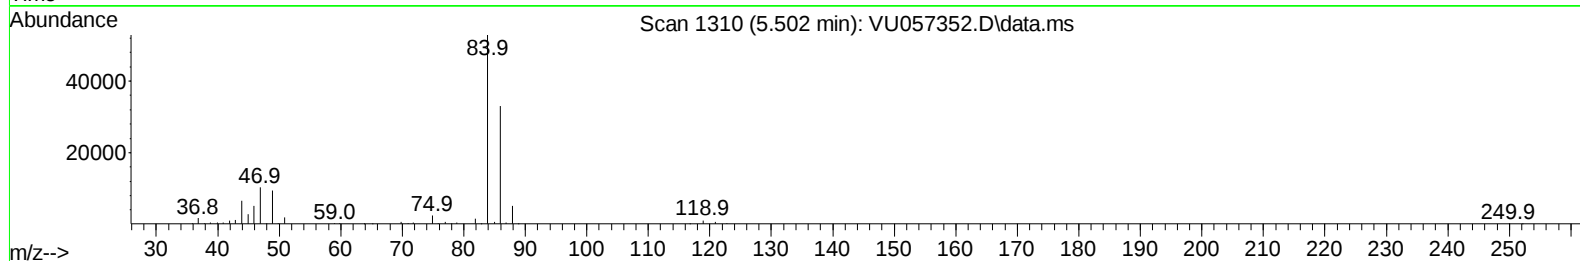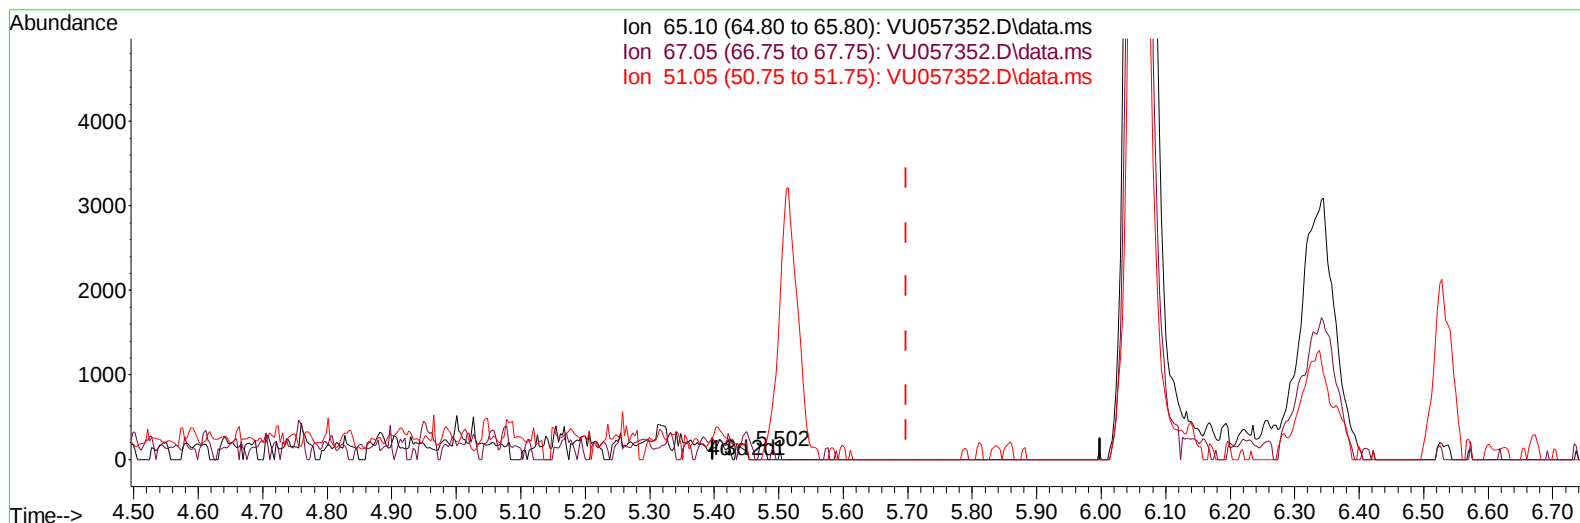

TIC: VU057352.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

5.502min (-0.196) 0.00 ug/L

response 21

Ion	Exp%	Act%
65.10	100.00	100.00
67.05	55.00	209.52#
51.05	33.90	30676.19#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

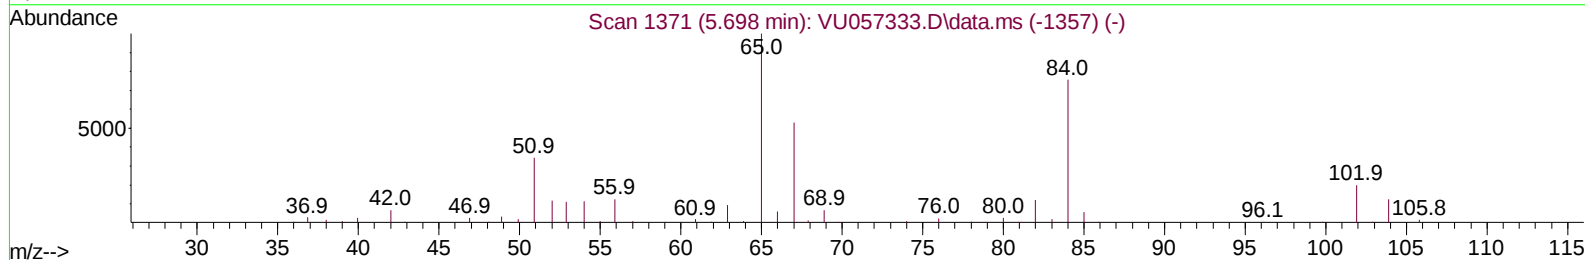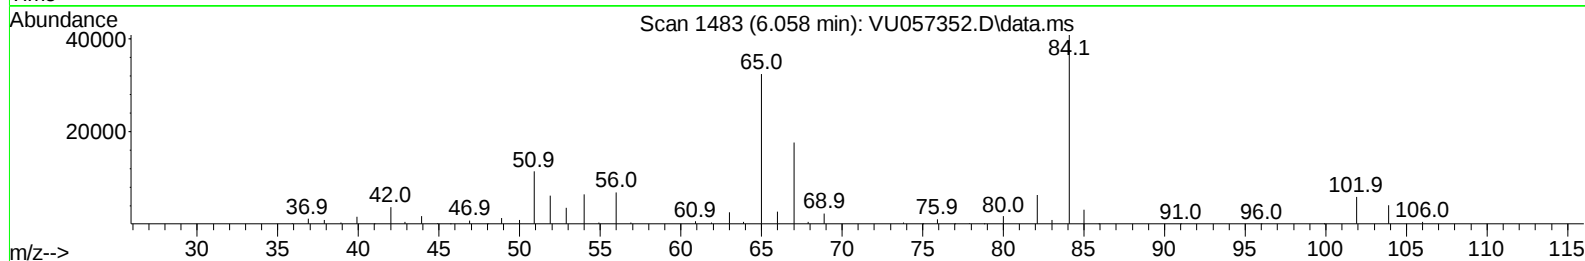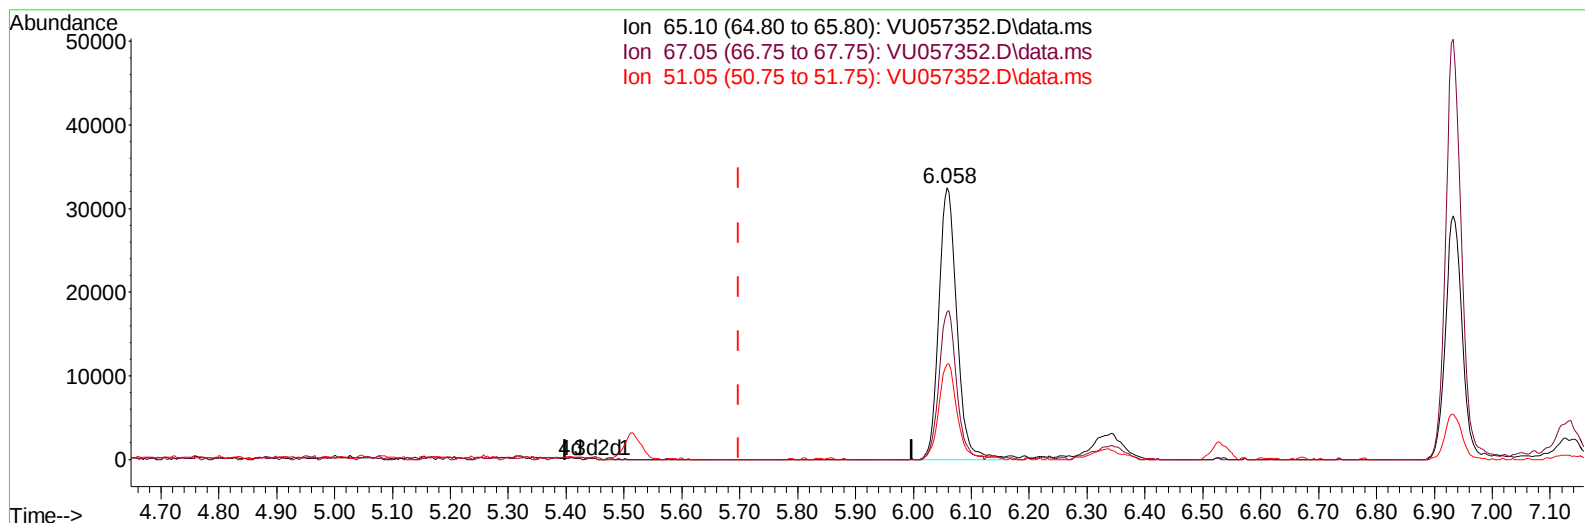

TIC: VU057352.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

6.058min (+ 0.360) 4.28 ug/L m

response 70512

Ion	Exp%	Act%
65.10	100.00	100.00
67.05	55.00	0.06#
51.05	33.90	9.14#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

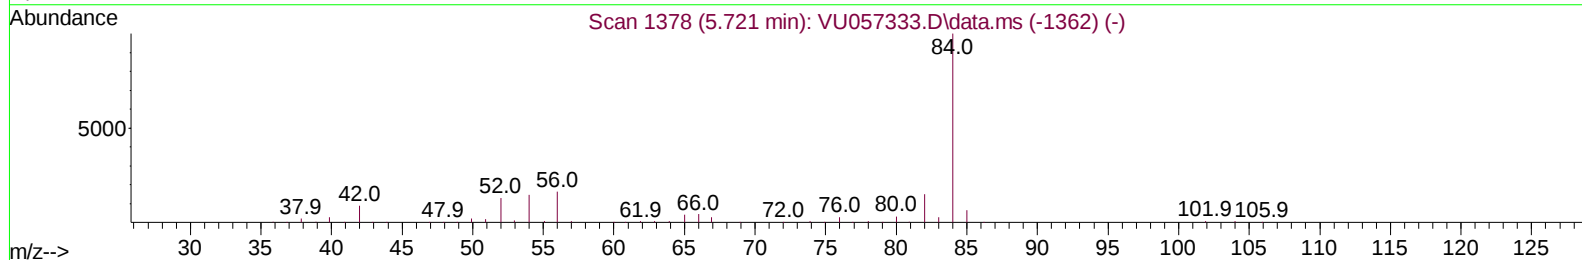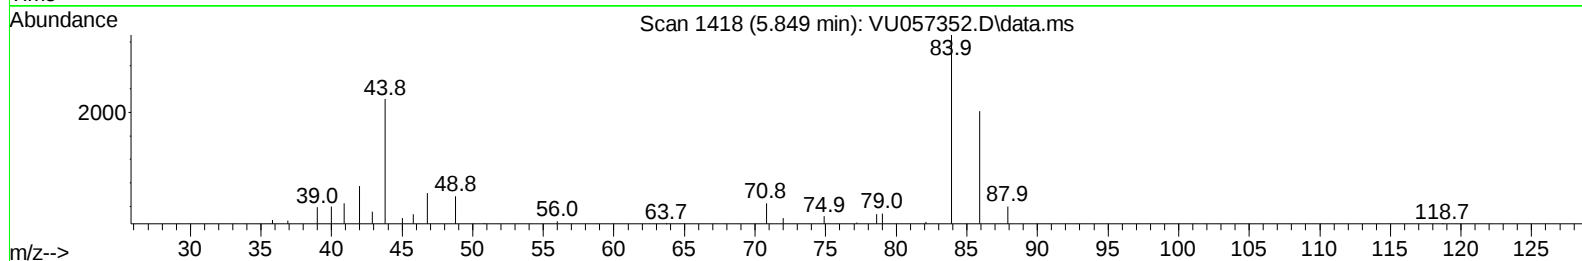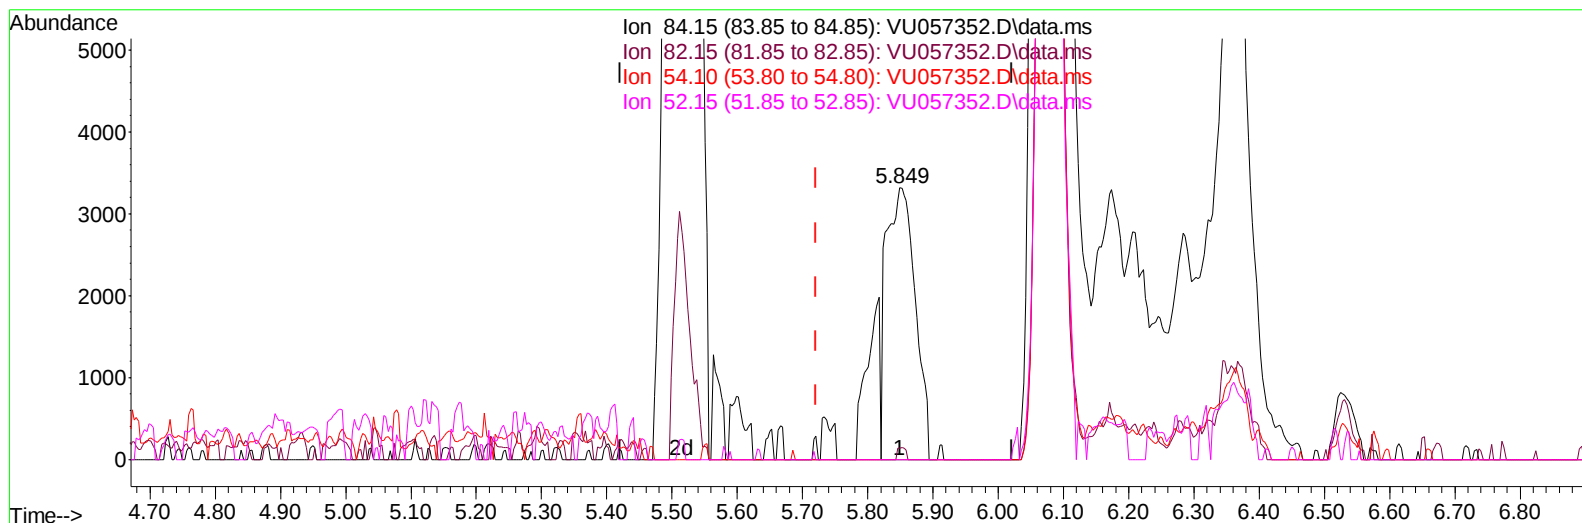

TIC: VU057352.D\data.ms

(32) Benzene-d6 (S)

5.849min (+ 0.129) 0.18 ug/L

response 10237

Ion	Exp%	Act%
84.15	100.00	100.00
82.15	15.10	0.00#
54.10	14.10	0.21#
52.15	13.20	0.20#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057352.D
Acq On : 28 Dec 2023 22:48
Operator : MD/SY
Sample : 06020-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

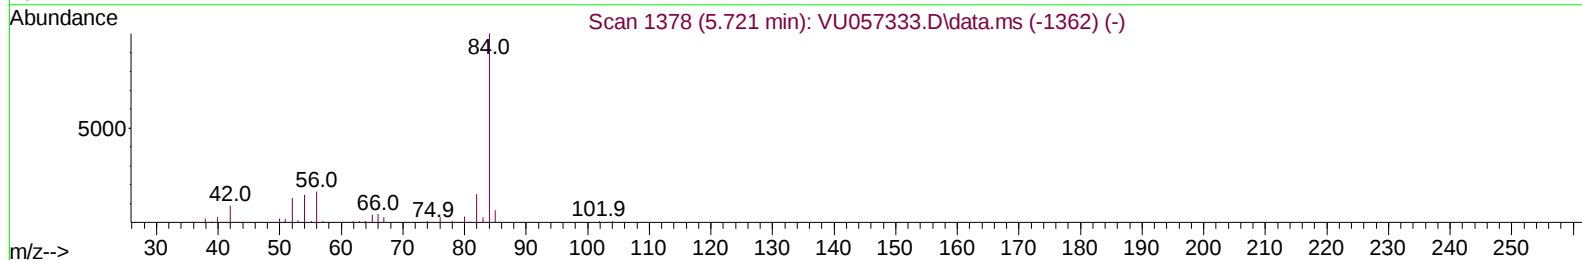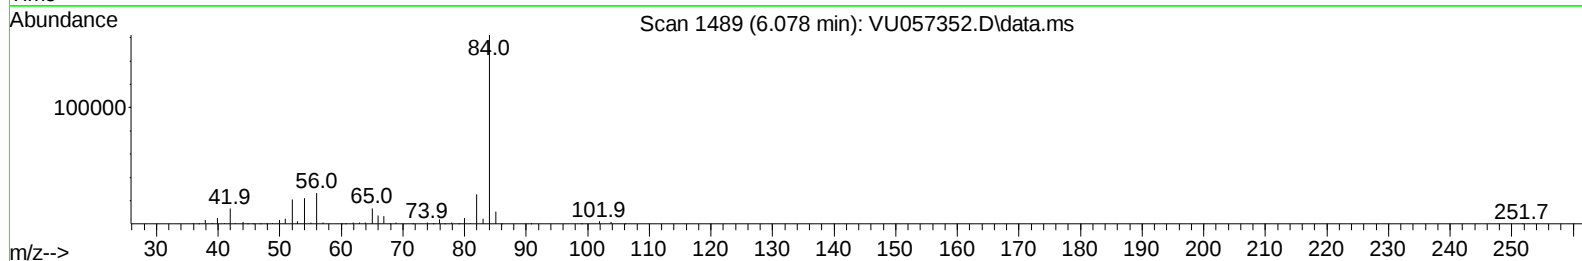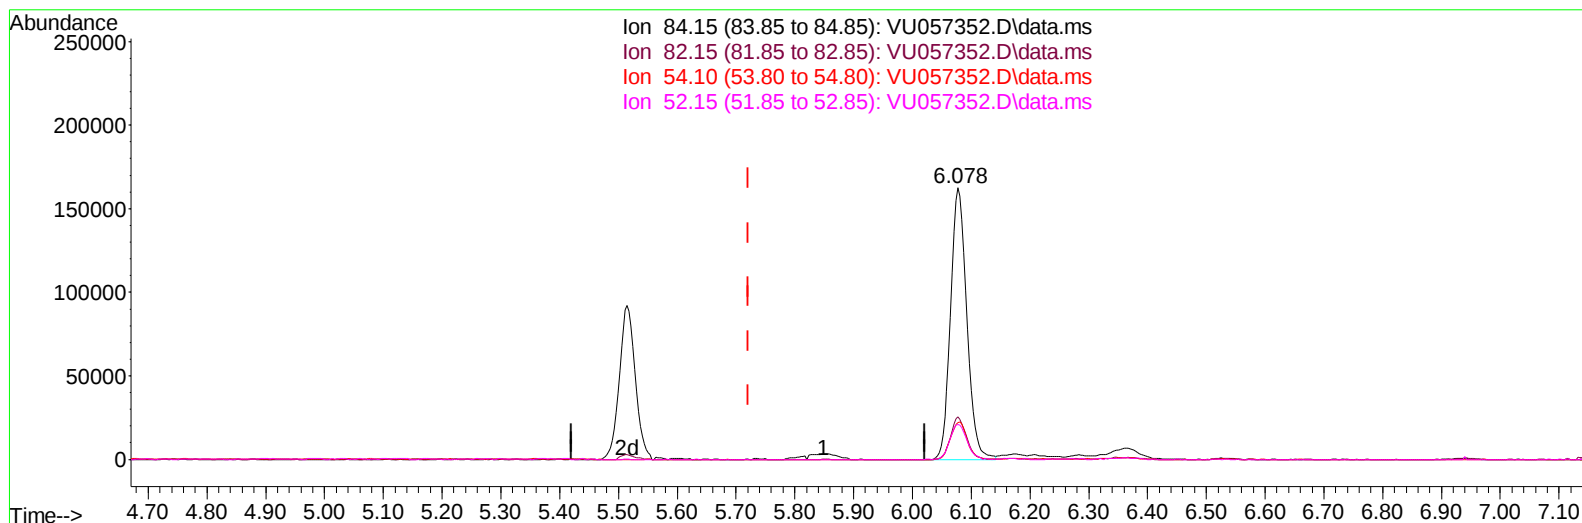

TIC: VU057352.D\data.ms

(32) Benzene-d6 (S)

6.078min (+ 0.357) 5.40 ug/L m

response 310164

Ion	Exp%	Act%
84.15	100.00	100.00
82.15	15.10	0.00#
54.10	14.10	0.01#
52.15	13.20	0.01#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

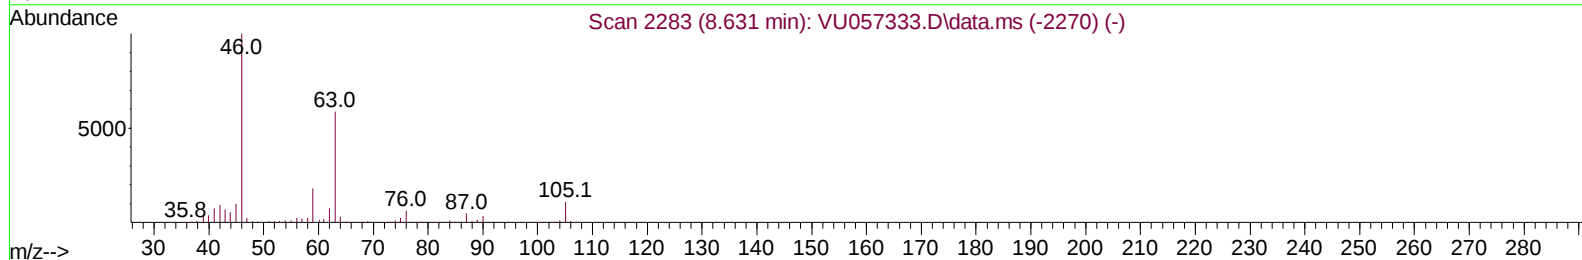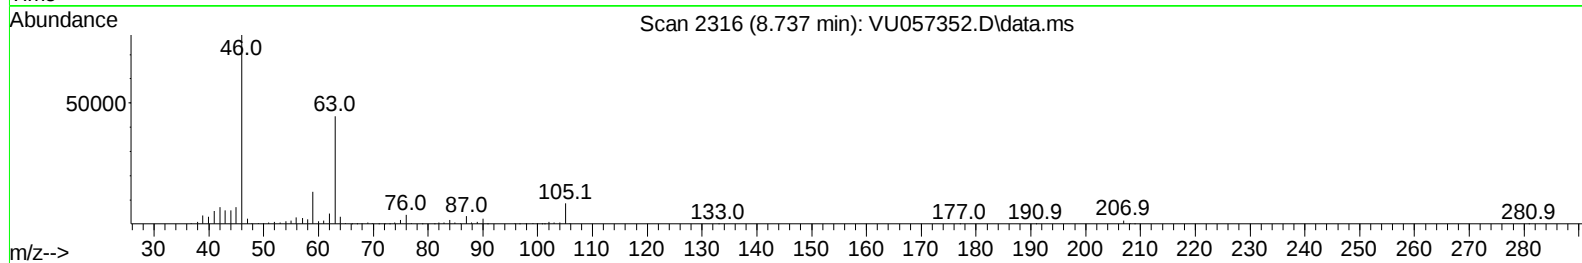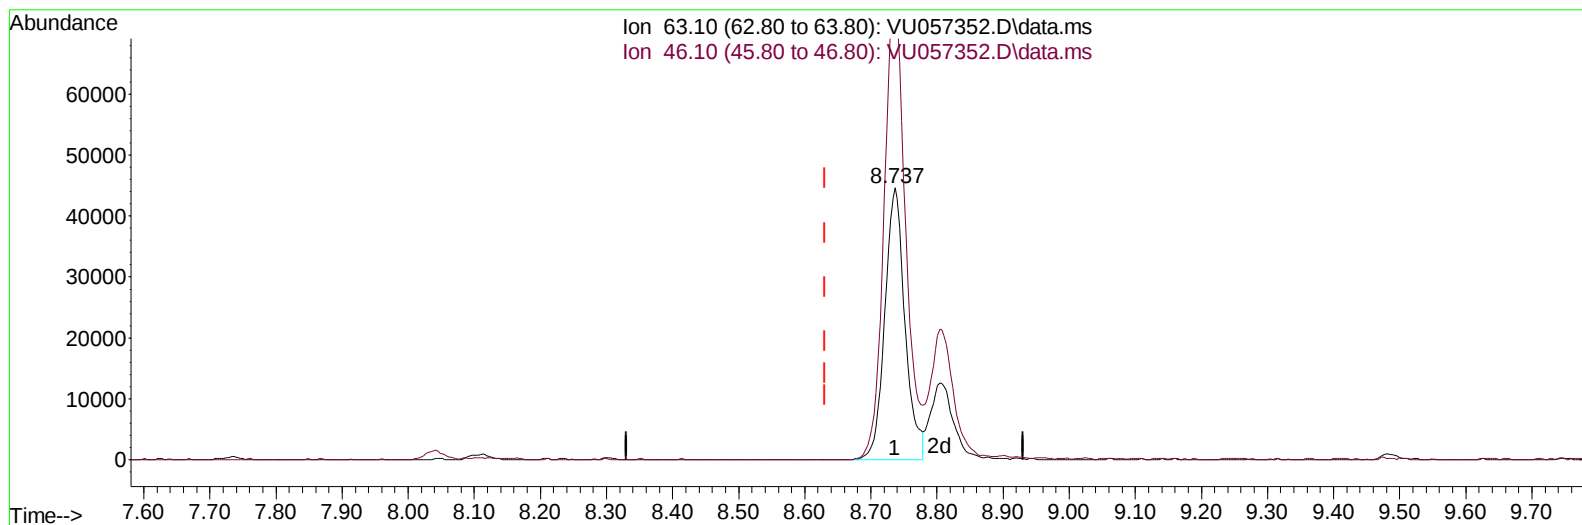

TIC: VU057352.D\data.ms

(46) 2-Hexanone-d5 (S)

8.737min (+ 0.106) 28.81 ug/L

response 94221

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	165.60	182.34
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

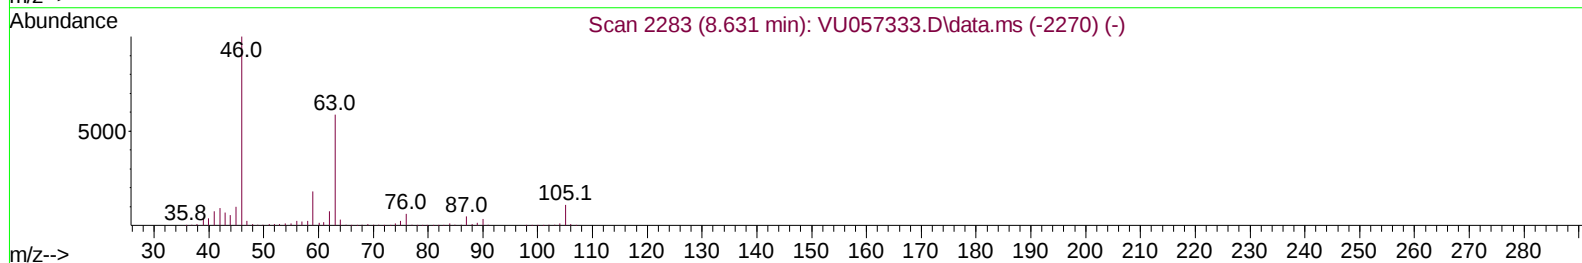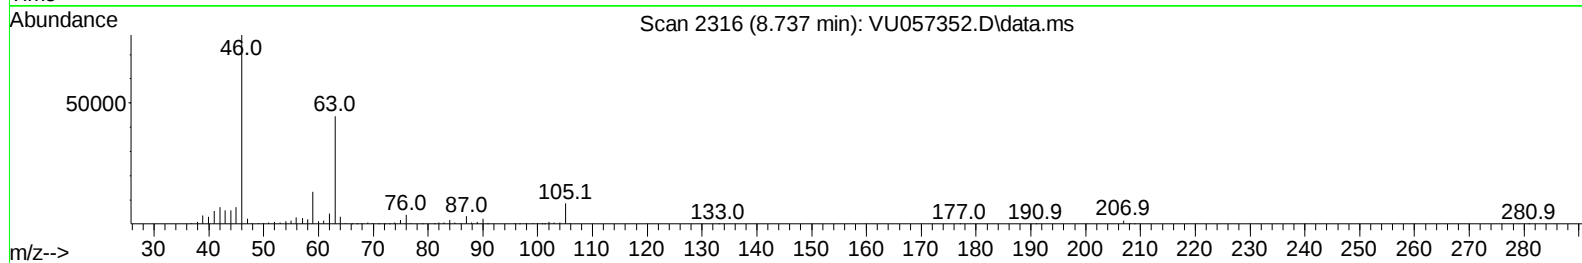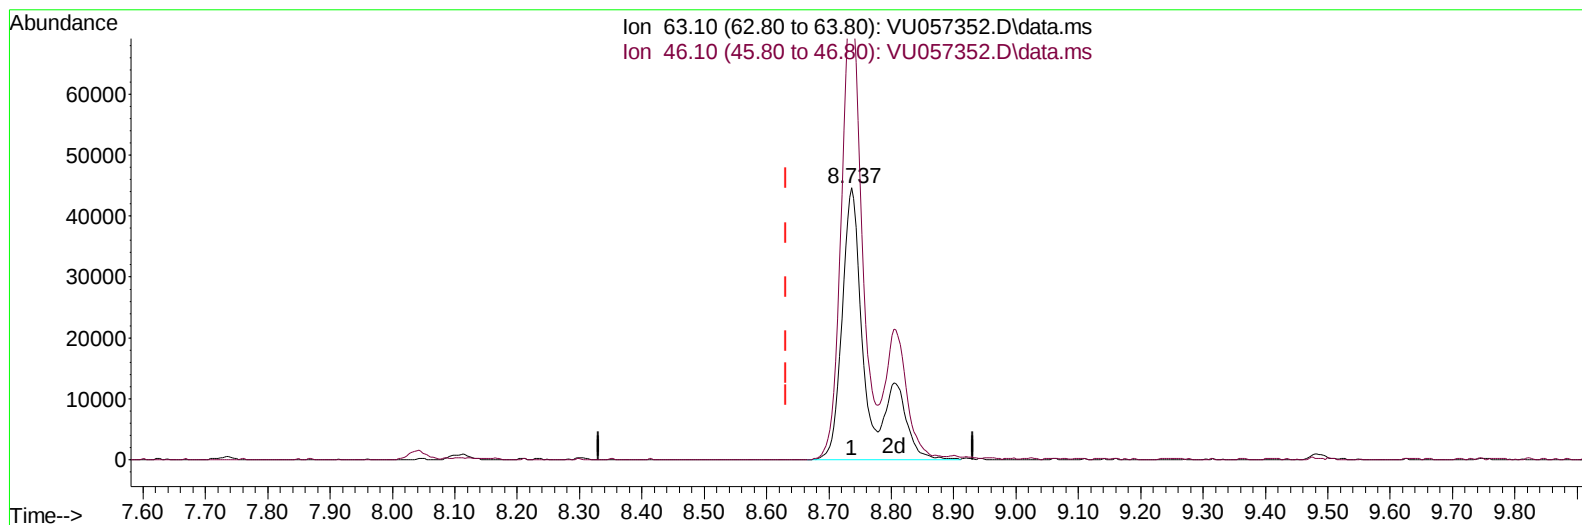

TIC: VU057352.D\data.ms

(46) 2-Hexanone-d5 (S)

8.737min (+ 0.106) 38.16 ug/L m

response 124821

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	165.60	137.64
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057352.D
 Acq On : 28 Dec 2023 22:48
 Operator : MD/SY
 Sample : 06020-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7Y1

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 12/29/2023
 Supervised By : Mahesh Dadoda 12/29/2023

Quant Time: Dec 29 00:06:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.531	114	210727m	5.000	ug/L	0.29
28) Chlorobenzene-d5	9.486	117	201490	5.000	ug/L	0.07
58) 1,4-Dichlorobenzene-d4	11.827	152	90382	5.000	ug/L	0.02
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.766	65	112698	6.221	ug/L	0.17
Spiked Amount 5.000	Range 40 - 130		Recovery = 124.400%			
7) Chloroethane-d5	2.190	69	84959m	5.839	ug/L	0.28
Spiked Amount 5.000	Range 65 - 130		Recovery = 116.800%			
11) 1,1-Dichloroethene-d2	3.039	65	32631m	4.526	ug/L	0.48
Spiked Amount 5.000	Range 60 - 125		Recovery = 90.600%			
20) 2-Butanone-d5	5.142	46	79518m	19.380	ug/L	0.51
Spiked Amount 50.000	Range 40 - 130		Recovery = 38.760%#			
24) Chloroform-d	5.515	84	179055m	5.558	ug/L	0.46
Spiked Amount 5.000	Range 70 - 125		Recovery = 111.200%			
26) 1,2-Dichloroethane-d4	6.058	65	70512m	4.283	ug/L	0.36
Spiked Amount 5.000	Range 70 - 130		Recovery = 85.600%			
32) Benzene-d6	6.078	84	310164m	5.400	ug/L	0.36
Spiked Amount 5.000	Range 70 - 125		Recovery = 108.000%			
36) 1,2-Dichloropropane-d6	6.933	67	93452	5.192	ug/L	0.25
Spiked Amount 5.000	Range 60 - 140		Recovery = 103.800%			
41) Toluene-d8	8.039	98	226357	4.568	ug/L	0.14
Spiked Amount 5.000	Range 70 - 130		Recovery = 91.400%			
43) trans-1,3-Dichloroprop...	8.299	79	27143	3.759	ug/L	0.13
Spiked Amount 5.000	Range 55 - 130		Recovery = 75.200%			
46) 2-Hexanone-d5	8.737	63	124821m	38.162	ug/L	0.11
Spiked Amount 50.000	Range 45 - 130		Recovery = 76.320%			
56) 1,1,2,2-Tetrachloroeth...	10.782	84	66855	4.423	ug/L	0.03
Spiked Amount 5.000	Range 65 - 120		Recovery = 88.400%			
66) 1,2-Dichlorobenzene-d4	12.206	152	85720	5.208	ug/L	0.02
Spiked Amount 5.000	Range 80 - 120		Recovery = 104.200%			

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057352.D
Acq On : 28 Dec 2023 22:48
Operator : MD/SY
Sample : 06020-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7Y1

Manual IntegrationsAPPROVED

Quant Time: Dec 29 00:06:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

