




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057355.D
 Acq On : 29 Dec 2023 00:51
 Operator : MD/SY
 Sample : 05998-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7A81

Manual IntegrationsAPPROVED

Quant Time: Dec 29 01:37:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

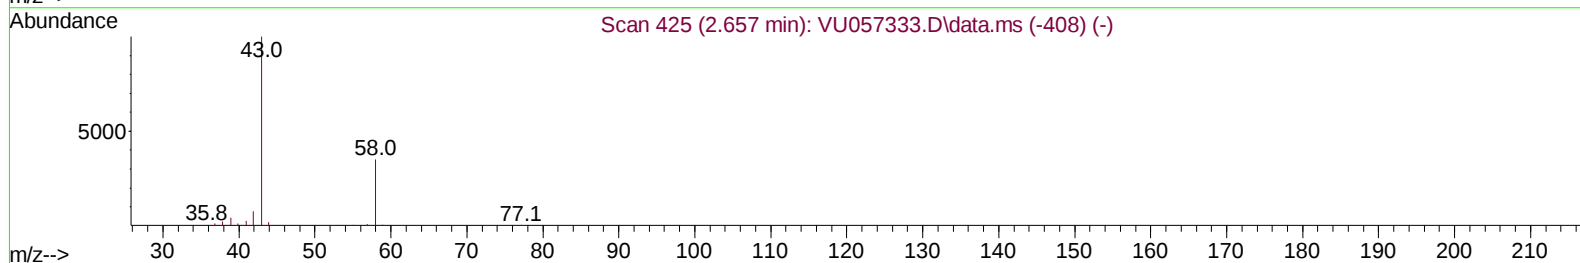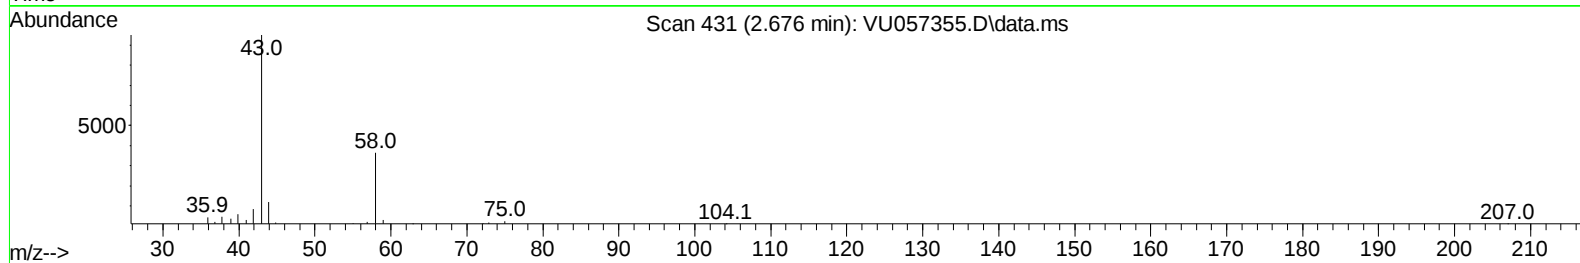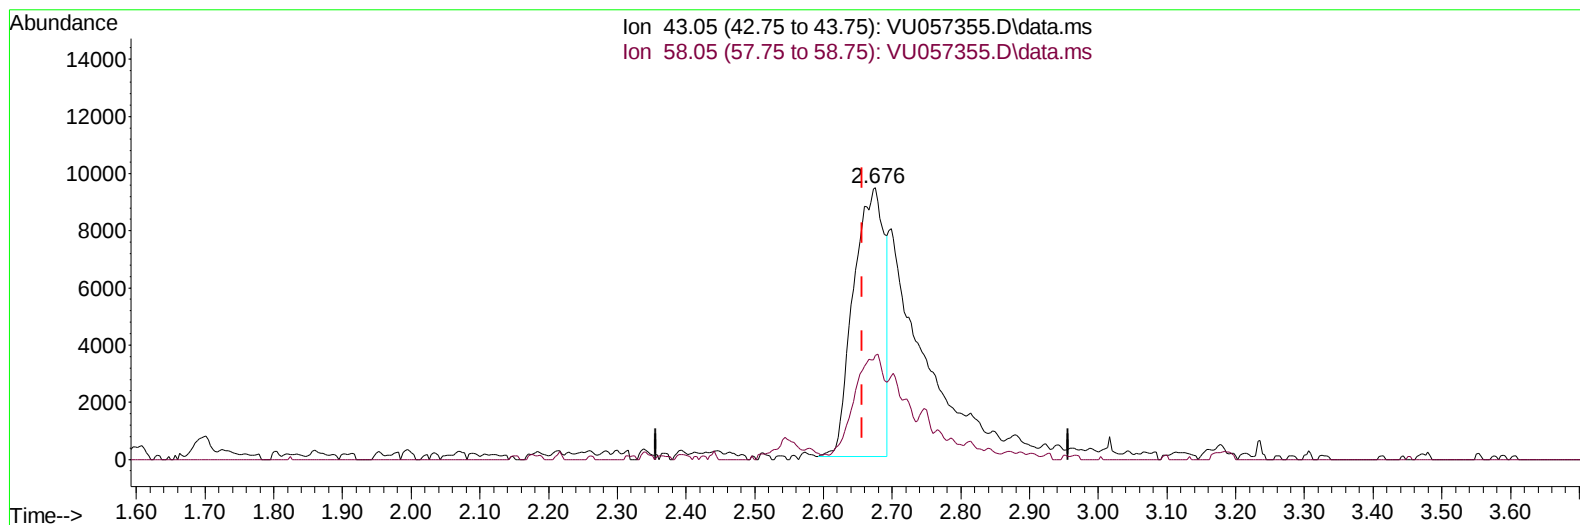

TIC: VU057355.D\data.ms

(13) Acetone (T)

2.676min (+ 0.019) 9.87 ug/L

response 29086

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	35.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057355.D
 Acq On : 29 Dec 2023 00:51
 Operator : MD/SY
 Sample : 05998-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7A81

Manual IntegrationsAPPROVED

Quant Time: Dec 29 01:37:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

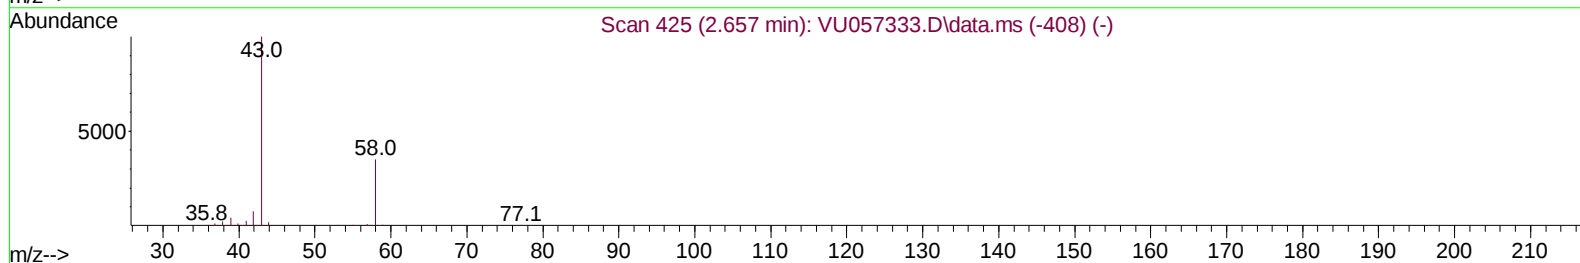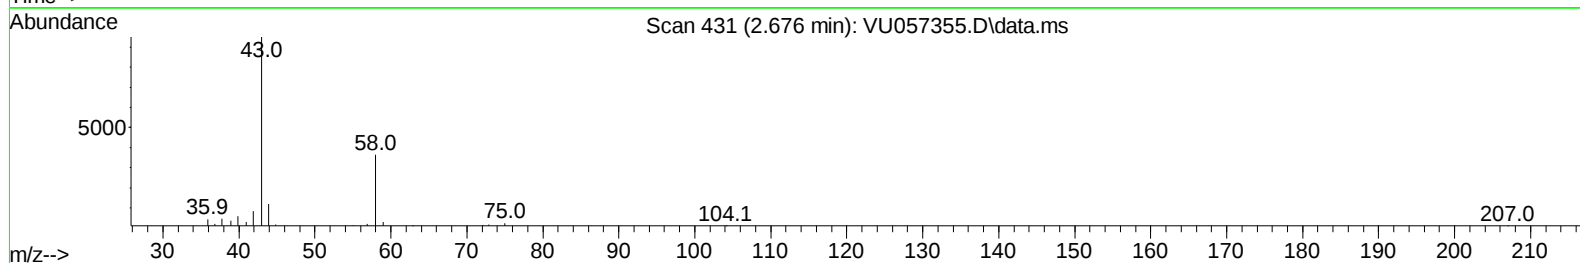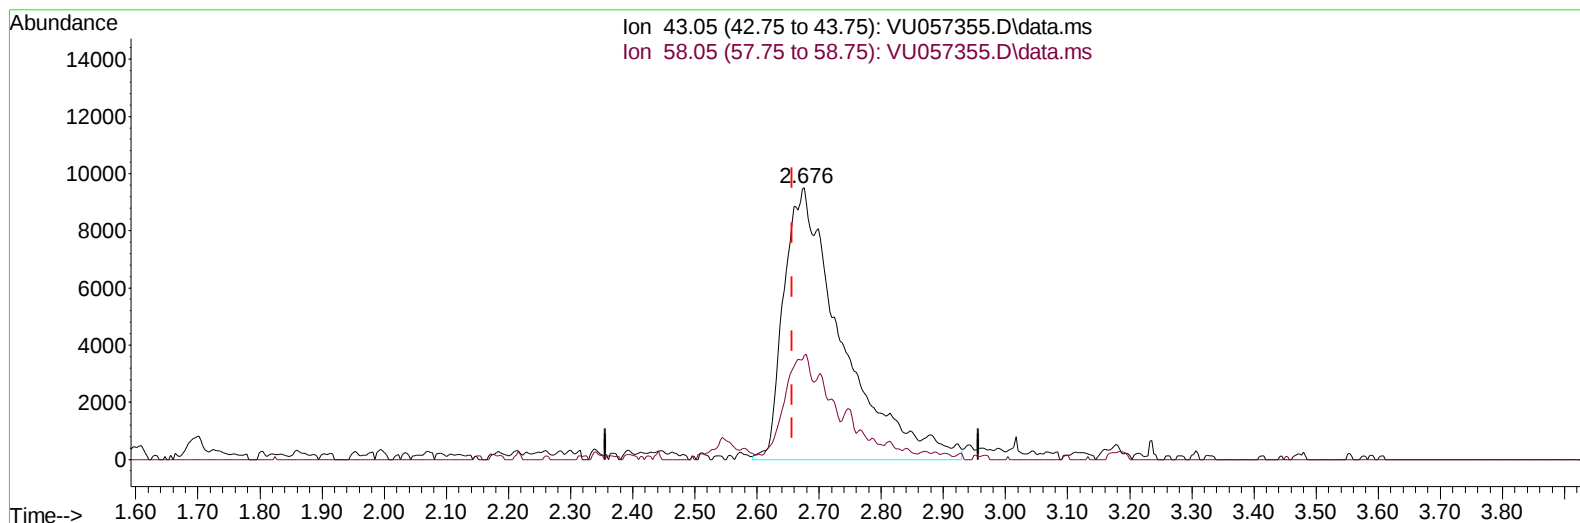

TIC: VU057355.D\data.ms

(13) Acetone (T)

2.676min (+ 0.019) 21.01 ug/L m

response 61906

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	16.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
 Data File : VU057355.D
 Acq On : 29 Dec 2023 00:51
 Operator : MD/SY
 Sample : 05998-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7A81

Manual IntegrationsAPPROVED

Quant Time: Dec 29 01:37:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 28 21:37:03 2023
 Response via : Initial Calibration

Reviewed By : John Carlone 12/29/2023
 Supervised By : Mahesh Dadoda 12/29/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		232194	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		234647	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		90056	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.599	65		97359	4.877	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	97.600%		
7) Chloroethane-d5	1.911	69		84710	5.284	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	105.600%		
11) 1,1-Dichloroethene-d2	2.560	65		38639	4.863	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	97.200%		
20) 2-Butanone-d5	4.644	46		221351	48.960	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	97.920%		
24) Chloroform-d	5.055	84		184905	5.209	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	104.200%		
26) 1,2-Dichloroethane-d4	5.695	65		91941	5.068	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	101.400%		
32) Benzene-d6	5.721	84		343607	5.137	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	102.800%		
36) 1,2-Dichloropropane-d6	6.685	67		111667	5.328	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	106.600%		
41) Toluene-d8	7.894	98		250671	4.344	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	86.800%		
43) trans-1,3-Dichloroprop...	8.174	79		37260	4.430	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	88.600%		
46) 2-Hexanone-d5	8.634	63		149234	39.179	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	78.360%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84		84900	4.823	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	96.400%		
66) 1,2-Dichlorobenzene-d4	12.187	152		87783	5.353	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	107.000%		
Target Compounds							
13) Acetone	2.676	43		61906m	21.009	ug/L	
42) Toluene	7.965	91		30701	0.422	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057355.D
Acq On : 29 Dec 2023 00:51
Operator : MD/SY
Sample : 05998-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7A81

Manual IntegrationsAPPROVED

Quant Time: Dec 29 01:37:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 28 21:37:03 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

