
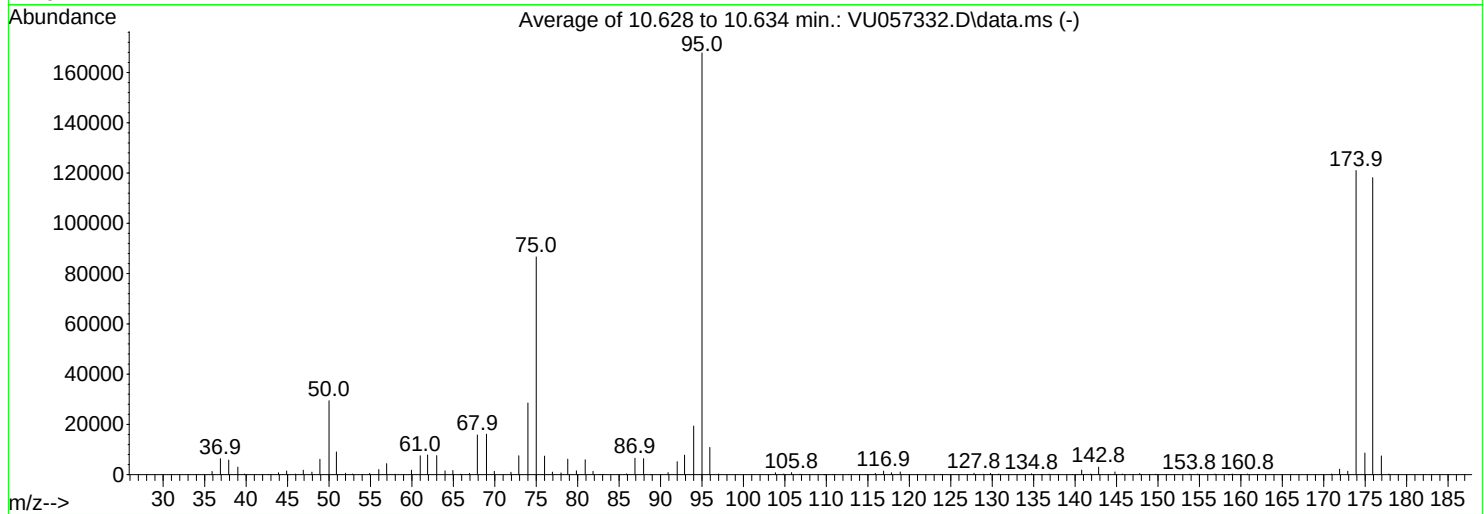


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122823\
Data File : VU057332.D
Acq On : 28 Dec 2023 13:46
Operator : MD/SY
Sample : BFB103
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB103

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 28 21:37:03 2023

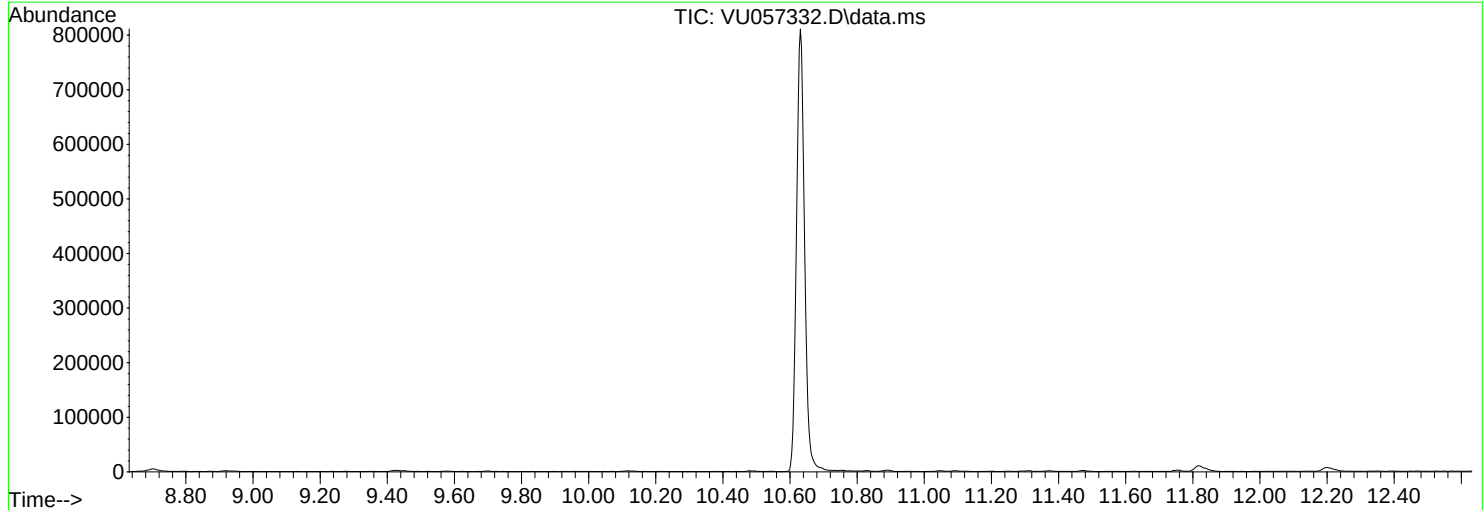

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	29440	PASS
75	95	30	80	51.6	86621	PASS
95	95	100	100	100.0	167829	PASS
96	95	5	9	6.5	10840	PASS
173	174	0.00	2	1.1	1344	PASS
174	95	50	120	72.1	121029	PASS
175	174	5	9	7.1	8587	PASS
176	174	95	101	97.6	118157	PASS
177	176	5	9	6.3	7483	PASS

m/z	Abundance
39.70	240.0
43.90	373.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	1123.0
36.90	6067.0
37.90	5632.0
39.00	3161.0
39.90	526.0
43.00	118.0
43.90	1029.0
44.90	1580.0
45.90	264.0
46.90	1796.0
47.90	986.0
48.90	6374.0
50.00	29688.0
50.90	9338.0
52.00	515.0
52.80	249.0
54.90	514.0
56.00	1874.0
56.90	4455.0
57.90	154.0
60.00	1709.0
61.00	7872.0
61.90	7510.0
63.00	7462.0
64.00	1521.0
65.00	1659.0
65.90	156.0
66.90	450.0
67.90	16131.0
69.00	16232.0
70.00	1189.0
71.90	945.0
72.90	7599.0
74.00	27968.0
75.00	85632.0
76.00	7572.0
77.00	994.0
78.00	693.0
78.80	6181.0
79.80	1391.0
80.90	5949.0
81.80	1373.0
82.70	204.0
85.90	339.0
86.90	6610.0
87.90	6221.0
90.90	811.0
92.00	5283.0
92.90	7594.0
94.00	19376.0
95.00	164928.0
96.00	11344.0
97.00	234.0
103.90	652.0
104.90	286.0
105.80	807.0
106.80	217.0
110.80	127.0
112.70	174.0
114.80	175.0
115.90	539.0
116.90	1197.0
117.80	759.0
118.90	1127.0
123.80	126.0
127.80	568.0
128.90	217.0
129.80	595.0
130.80	273.0
134.80	342.0
135.90	101.0
137.00	204.0
139.70	134.0
140.80	1774.0
141.90	281.0
142.80	2959.0
143.90	181.0
144.80	1112.0
145.70	287.0
146.70	128.0
147.80	465.0
149.70	154.0
153.80	166.0
154.80	341.0
156.00	173.0
156.90	230.0
158.50	110.0
159.00	137.0
160.80	273.0
171.10	245.0
171.90	2044.0
172.90	1262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

173.90	116872.0
174.90	8300.0
175.90	113752.0
177.00	7717.0
177.80	247.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	1343.0
36.90	6605.0
37.90	5936.0
39.00	3141.0
39.90	511.0
42.70	147.0
43.90	1126.0
44.90	1486.0
45.90	267.0
46.90	1825.0
47.90	1028.0
48.90	6260.0
50.00	30216.0
50.90	9447.0
52.00	572.0
52.80	264.0
54.90	492.0
56.00	2113.0
57.00	4559.0
58.00	208.0
59.90	1891.0
61.00	7645.0
61.90	8164.0
63.00	7807.0
64.00	1594.0
64.90	1739.0
65.90	194.0
66.90	501.0
67.90	16192.0
69.00	16408.0
69.90	1378.0
71.90	1013.0
72.90	7804.0
74.00	29488.0
75.00	89408.0
76.00	7529.0
76.90	1061.0
78.00	718.0
78.80	6356.0
79.80	1552.0
80.90	6052.0
81.80	1388.0
82.70	129.0
85.90	354.0
86.90	6736.0
88.00	6571.0
88.80	109.0
90.90	816.0
92.00	5395.0
92.90	8029.0
94.00	20040.0
95.00	172800.0
96.00	11210.0
97.00	276.0
103.90	787.0
104.80	247.0
105.80	860.0
106.80	190.0
109.70	101.0
110.80	135.0
112.70	132.0
114.80	158.0
115.90	522.0
116.90	1382.0
117.80	777.0
118.90	1093.0
123.80	188.0
127.80	606.0
129.00	200.0
129.80	541.0
130.80	283.0
134.70	424.0
136.80	216.0
140.80	1950.0
141.90	272.0
142.90	3052.0
144.00	147.0
144.80	1090.0
145.70	221.0
146.60	134.0
147.80	470.0
149.70	181.0
153.80	219.0
154.80	366.0
156.00	168.0
156.90	268.0
159.00	254.0
160.80	291.0
170.90	268.0
171.90	2198.0
172.90	1395.0
173.90	124720.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

174.90	8802.0
175.90	121984.0
177.00	7709.0
177.90	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	1402.0
36.90	6436.0
37.90	5809.0
39.00	2675.0
39.90	434.0
42.90	188.0
43.90	1216.0
44.90	1312.0
46.00	229.0
46.90	1715.0
48.00	980.0
48.90	5763.0
50.00	28416.0
50.90	8445.0
52.00	569.0
52.90	232.0
54.90	449.0
56.00	2181.0
56.90	4201.0
58.00	238.0
59.90	1832.0
61.00	7110.0
61.90	7791.0
63.00	7564.0
64.00	1483.0
64.90	1647.0
65.80	204.0
67.00	527.0
67.90	15120.0
69.00	15654.0
69.90	1388.0
72.00	999.0
72.90	7131.0
74.00	28096.0
75.00	84824.0
76.00	6980.0
76.90	1046.0
78.00	672.0
78.80	5944.0
79.90	1653.0
80.90	5777.0
81.90	1345.0
83.10	139.0
85.90	332.0
86.90	6287.0
88.00	6255.0
90.90	789.0
92.00	4859.0
92.90	7724.0
94.00	18752.0
95.00	165760.0
95.90	9965.0
97.00	276.0
103.80	826.0
104.90	220.0
105.80	801.0
106.80	130.0
110.80	152.0
114.70	127.0
115.90	516.0
116.90	1564.0
117.90	728.0
118.90	1054.0
123.80	165.0
127.80	595.0
129.00	243.0
129.80	472.0
130.80	245.0
134.70	398.0
136.80	251.0
140.80	1887.0
141.90	274.0
142.90	2989.0
144.10	172.0
144.80	1077.0
145.70	191.0
147.80	464.0
149.80	187.0
153.80	228.0
155.00	370.0
156.00	143.0
156.90	260.0
158.90	321.0
160.80	280.0
170.80	291.0
171.90	2201.0
172.90	1374.0
173.90	121496.0
175.00	8658.0
175.90	118736.0
176.90	7024.0
177.90	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103