


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122920\
 Data File : VU041828.D
 Acq On : 29 Dec 2020 08:46
 Operator : SY/MD
 Sample : BFB31
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB31

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Dec 30 01:48:43 2020

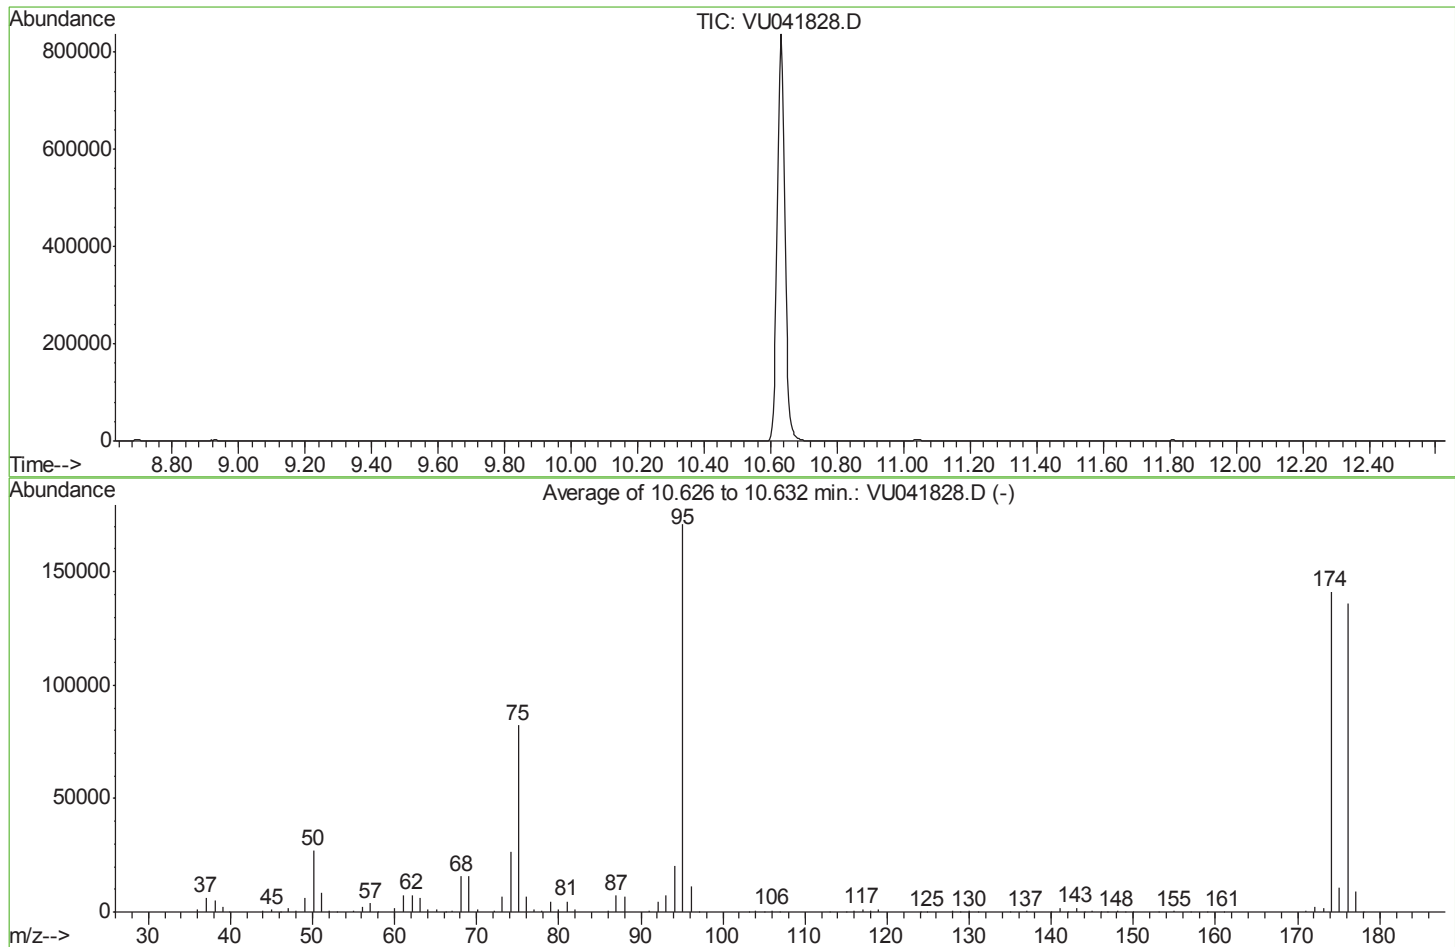

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	26922	PASS
75	95	30	80	48.2	82322	PASS
95	95	100	100	100.0	170901	PASS
96	95	5	9	6.7	11479	PASS
173	174	0.00	2	1.4	1929	PASS
174	95	50	120	82.6	141130	PASS
175	174	5	9	7.5	10609	PASS
176	174	95	101	96.2	135773	PASS
177	176	5	9	6.9	9307	PASS

m/z	Abundance
36.00	1098.0
37.00	6161.0
38.10	4895.0
39.10	2255.0
39.90	101.0
44.00	1111.0
45.10	1057.0
46.10	198.0
47.10	1520.0
48.00	832.0
49.10	5793.0
50.10	24504.0
51.10	8131.0
52.00	371.0
53.00	203.0
55.10	331.0
56.10	2160.0
57.10	3715.0
60.00	1315.0
61.00	6703.0
62.10	6996.0
63.10	6226.0
64.00	1059.0
65.10	1283.0
66.10	106.0
67.00	352.0
68.10	14826.0
69.10	14814.0
70.10	1062.0
72.10	809.0
73.10	6494.0
74.10	25160.0
75.10	77416.0
76.10	6463.0
77.10	960.0
77.90	689.0
79.00	4278.0
80.00	1403.0
81.00	4681.0
82.00	1286.0
86.00	310.0
87.00	6477.0
88.00	6145.0
91.00	521.0
92.10	4323.0
93.10	6842.0
94.10	18624.0
95.10	160960.0
96.10	10824.0
97.10	237.0
104.00	620.0
105.00	175.0
106.00	662.0
114.90	201.0
116.00	576.0
117.10	1181.0
118.00	629.0
119.00	947.0
124.90	116.0
128.10	497.0
129.00	258.0
130.00	548.0
131.10	163.0
135.00	268.0
137.00	334.0
141.10	1326.0
142.00	235.0
143.00	1822.0
144.00	109.0
145.00	548.0
146.00	274.0
146.90	112.0
148.00	350.0
148.90	142.0
149.90	109.0
155.00	441.0
157.00	304.0
159.00	195.0
161.00	139.0
171.00	316.0
172.10	1803.0
173.20	1798.0
174.10	129376.0
175.10	10075.0
176.10	123800.0
177.10	8530.0
178.00	259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	1059.0
37.00	6475.0
38.10	5610.0
39.10	2496.0
39.90	117.0
44.00	1181.0
45.00	1066.0
46.10	157.0
47.10	1612.0
48.00	872.0
49.10	6348.0
50.10	27864.0
51.10	8880.0
52.00	345.0
53.00	193.0
55.00	380.0
56.00	2326.0
57.00	3841.0
58.00	121.0
60.00	1453.0
61.10	7416.0
62.10	7901.0
63.10	6625.0
64.00	1020.0
65.10	1204.0
67.00	426.0
68.10	16143.0
69.10	15995.0
70.10	1156.0
72.10	890.0
73.10	7245.0
74.10	27632.0
75.10	85168.0
76.10	7157.0
77.10	929.0
77.90	701.0
79.00	4561.0
80.00	1465.0
81.00	4956.0
82.00	1392.0
85.90	363.0
87.00	7344.0
88.10	7059.0
91.00	593.0
92.10	4766.0
93.10	7744.0
94.10	20960.0
95.10	176448.0
96.10	11863.0
97.10	249.0
104.00	648.0
105.00	179.0
106.00	720.0
106.90	130.0
114.90	178.0
116.00	552.0
117.00	1236.0
118.00	697.0
119.00	999.0
124.90	120.0
128.00	529.0
129.00	246.0
130.00	564.0
131.10	163.0
135.00	282.0
137.00	340.0
139.90	100.0
141.10	1571.0
142.00	244.0
143.00	1988.0
144.00	131.0
145.00	611.0
146.10	303.0
146.90	121.0
148.00	360.0
149.00	139.0
149.90	162.0
153.00	116.0
155.00	423.0
157.00	289.0
159.00	219.0
161.00	171.0
171.10	320.0
172.10	2062.0
173.20	1962.0
174.10	145408.0
175.10	10886.0
176.10	140032.0
177.10	9695.0
178.00	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	957.0
37.00	6213.0
38.10	5554.0
39.10	2369.0
39.90	150.0
44.00	1134.0
45.00	1089.0
45.90	113.0
47.10	1677.0
48.00	872.0
49.10	6007.0
50.10	28400.0
51.10	8882.0
52.00	295.0
53.00	127.0
55.00	374.0
56.10	2165.0
57.00	3557.0
58.00	143.0
60.00	1563.0
61.10	7252.0
62.10	7968.0
63.10	6351.0
64.00	952.0
65.10	1109.0
66.20	100.0
67.00	395.0
68.10	16070.0
69.10	16037.0
70.10	1178.0
72.10	885.0
73.10	7281.0
74.10	27576.0
75.10	84384.0
76.10	7368.0
77.00	937.0
78.00	667.0
79.00	4240.0
80.00	1381.0
81.00	4651.0
82.00	1357.0
85.90	316.0
87.00	7509.0
88.10	7013.0
90.90	540.0
92.10	4813.0
93.10	7645.0
94.10	20856.0
95.10	175296.0
96.10	11750.0
97.00	243.0
103.10	102.0
104.00	647.0
105.00	180.0
106.00	727.0
106.90	191.0
113.00	100.0
115.00	142.0
116.00	473.0
117.00	1156.0
118.00	652.0
119.00	984.0
124.00	120.0
127.90	559.0
128.90	221.0
130.00	556.0
131.10	176.0
135.00	277.0
137.00	302.0
141.10	1673.0
142.10	217.0
143.10	1930.0
144.00	147.0
145.00	622.0
146.10	285.0
146.90	119.0
148.10	347.0
149.00	157.0
149.90	177.0
153.00	157.0
154.90	393.0
157.00	274.0
159.10	234.0
161.00	174.0
171.10	279.0
172.10	2155.0
173.20	2027.0
174.10	148608.0
175.10	10866.0
176.10	143488.0
177.10	9696.0
178.00	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Scan 2874 (10.581 min): VU041828.D
BFB31

m/z	Abundance
43.90	281.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31