

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122921\
 Data File : VU046637.D
 Acq On : 29 Dec 2021 19:25
 Operator : SY/MD
 Sample : M5193-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU046637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rVB	44516	51412	15.71%	2.168%
2	1.919	168	180	197	rBV	32063	44464	13.59%	1.875%
3	2.572	372	383	403	rVB	71434	115886	35.42%	4.888%
4	3.054	522	533	545	rBV4	4946	9267	2.83%	0.391%
5	4.645	1014	1028	1066	rBV	37478	138305	42.27%	5.833%
6	5.067	1143	1159	1175	rBV	57807	126497	38.66%	5.335%
7	5.729	1344	1365	1386	rBV2	109588	286017	87.41%	12.063%
8	6.253	1513	1528	1549	rBV	75732	142231	43.47%	5.999%
9	6.694	1651	1665	1686	rBV	70496	135787	41.50%	5.727%
10	7.568	1924	1937	1951	rBV2	33443	56824	17.37%	2.397%
11	7.903	2023	2041	2056	rBV	120538	209400	64.00%	8.832%
12	8.182	2119	2128	2143	rVB	21363	35036	10.71%	1.478%
13	8.475	2209	2219	2226	rBV4	2227	3600	1.10%	0.152%
14	8.636	2257	2269	2307	rBV	181110	327207	100.00%	13.801%
15	8.915	2345	2356	2368	rBV3	5416	9497	2.90%	0.401%
16	9.420	2497	2513	2529	rBV	122974	202681	61.94%	8.548%
17	10.758	2918	2929	2943	rBV	60291	94690	28.94%	3.994%
18	10.893	2962	2971	2983	rBV2	5273	8137	2.49%	0.343%
19	11.812	3246	3257	3273	rBV	114149	182128	55.66%	7.682%
20	12.195	3363	3376	3389	rBV	117231	188044	57.47%	7.931%
21	12.774	3546	3556	3564	rBV2	2667	3847	1.18%	0.162%




Sum of corrected areas: 2370957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122921\
Data File : VU046637.D
Acq On : 29 Dec 2021 19:25
Operator : SY/MD
Sample : M5193-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

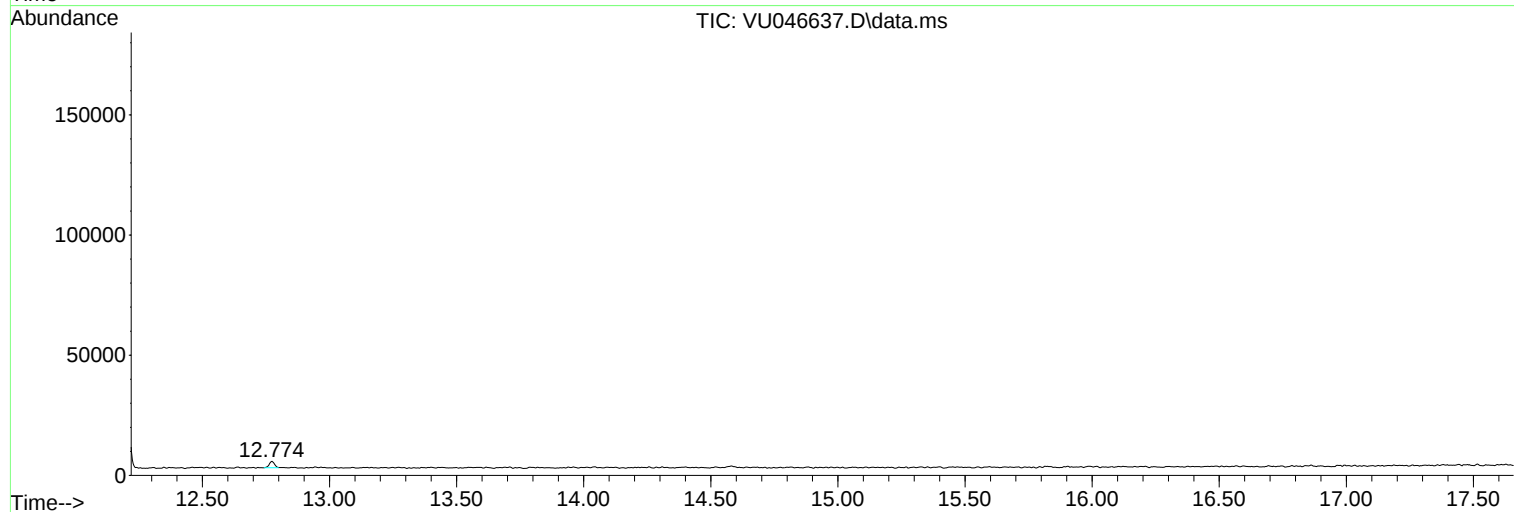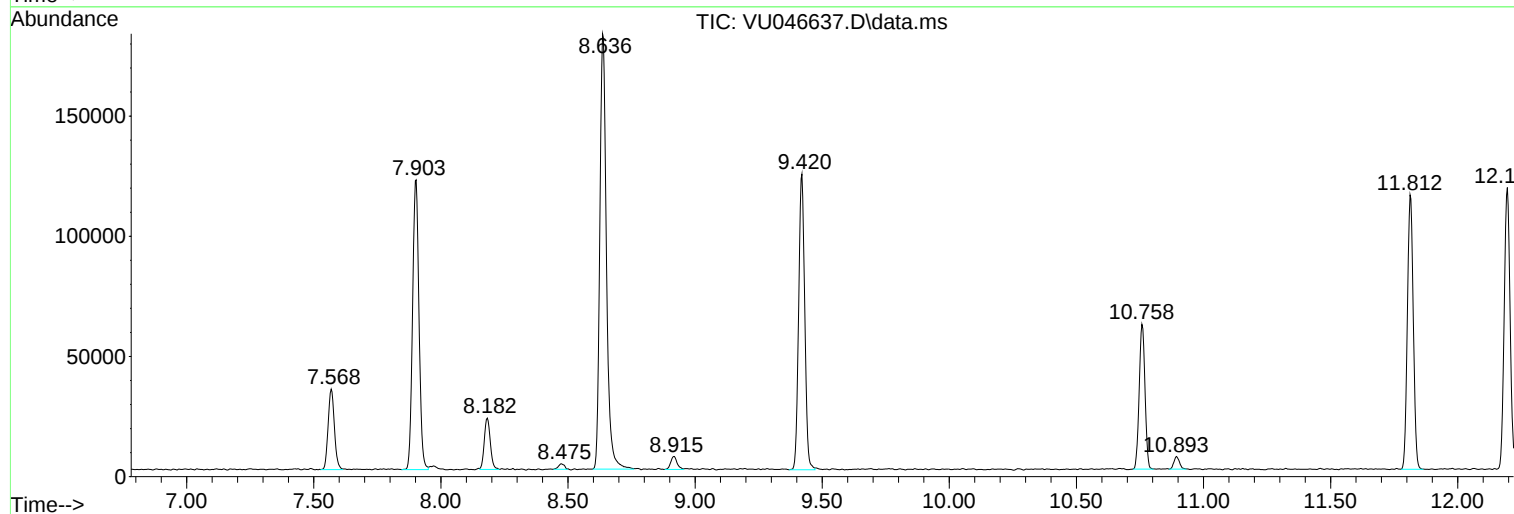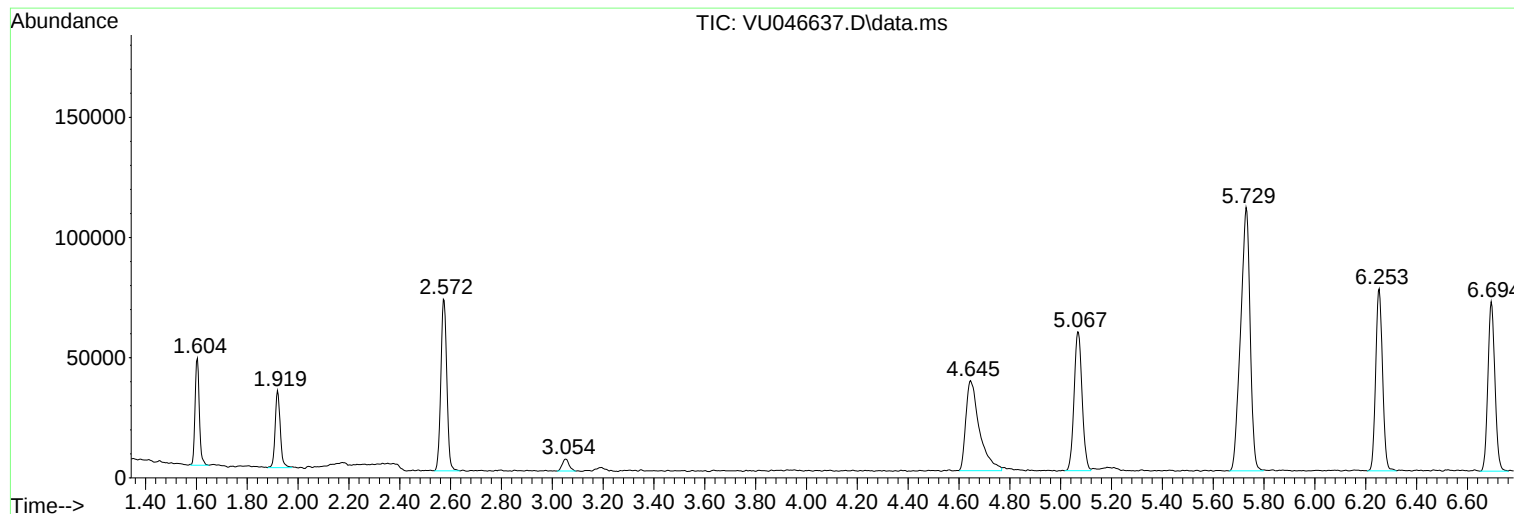

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122921\
Data File : VU046637.D
Acq On : 29 Dec 2021 19:25
Operator : SY/MD
Sample : M5193-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122921\
Data File : VU046637.D
Acq On : 29 Dec 2021 19:25
Operator : SY/MD
Sample : M5193-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
