


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122921\
 Data File : VU046626.D
 Acq On : 29 Dec 2021 09:09
 Operator : SY/MD
 Sample : BFB038
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB038

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 30 04:21:35 2021

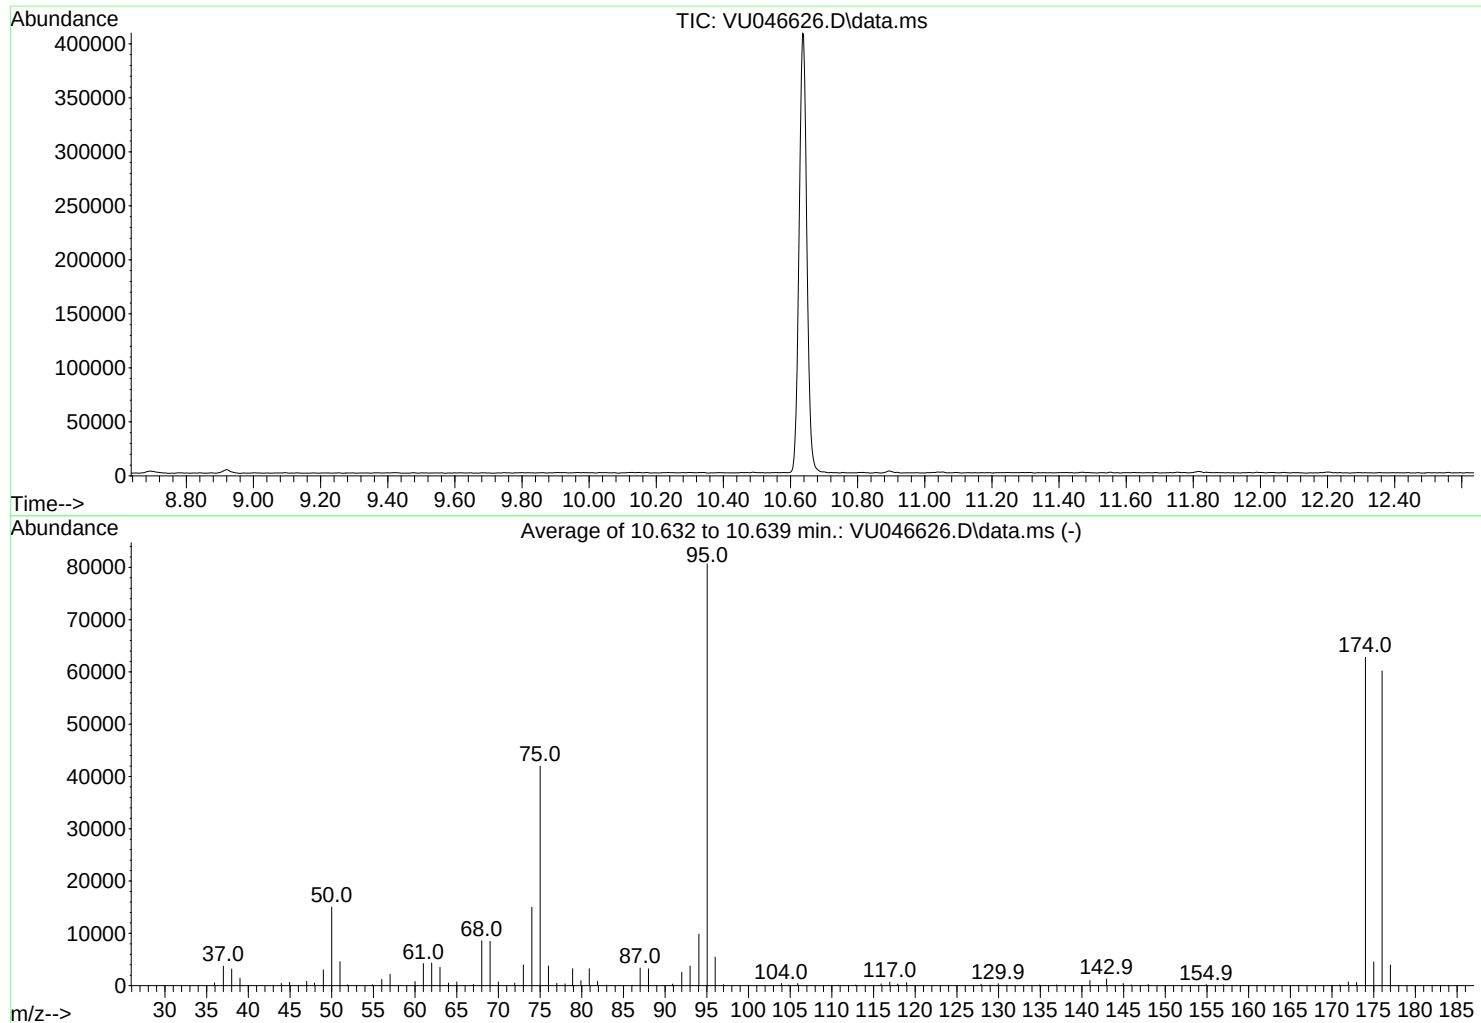

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	15036	PASS
75	95	30	80	52.1	42000	PASS
95	95	100	100	100.0	80675	PASS
96	95	5	9	6.7	5444	PASS
173	174	0.00	2	1.0	612	PASS
174	95	50	120	77.9	62808	PASS
175	174	5	9	7.2	4545	PASS
176	174	95	101	95.9	60208	PASS
177	176	5	9	6.5	3907	PASS

m/z	Abundance
36.00	158.0
39.90	2584.0
43.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
36.00	613.0
37.00	3627.0
38.00	3169.0
39.00	1357.0
39.90	2517.0
44.00	561.0
45.00	586.0
47.00	807.0
47.90	477.0
49.00	2912.0
50.00	14301.0
51.00	4544.0
51.90	146.0
54.90	191.0
56.00	1080.0
57.00	2081.0
60.00	758.0
61.00	4066.0
62.00	4143.0
63.00	3385.0
64.00	479.0
65.00	734.0
67.00	209.0
68.00	8228.0
69.00	8068.0
70.00	676.0
71.90	501.0
73.00	3680.0
74.00	14063.0
75.00	39872.0
76.00	3488.0
77.00	497.0
78.00	334.0
78.90	3128.0
79.90	958.0
80.90	3156.0
81.90	823.0
82.90	112.0
87.00	3246.0
88.00	3004.0
90.90	282.0
92.00	2449.0
93.00	3847.0
94.10	9320.0
95.00	76208.0
96.00	5253.0
97.00	189.0
103.90	390.0
104.80	119.0
105.90	414.0
110.80	107.0
112.80	103.0
115.90	375.0
116.90	665.0
117.90	326.0
119.00	492.0
127.90	277.0
129.00	112.0
129.90	352.0
134.90	123.0
136.90	186.0
141.00	925.0
142.00	117.0
142.90	1268.0
145.00	421.0
145.90	147.0
147.90	173.0
154.90	207.0
157.00	129.0
170.90	122.0
171.90	662.0
173.00	624.0
174.00	57632.0
175.00	4389.0
176.00	54856.0
177.00	3673.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
36.00	691.0
37.00	3884.0
38.00	3292.0
39.00	1487.0
39.90	2571.0
44.00	584.0
44.90	689.0
47.00	826.0
48.00	522.0
49.00	3105.0
50.00	15563.0
51.00	4697.0
51.90	150.0
54.90	211.0
56.00	1241.0
57.00	2250.0
60.00	851.0
61.00	4398.0
62.00	4446.0
63.00	3621.0
64.00	478.0
65.00	739.0
67.00	229.0
68.00	8867.0
69.00	8720.0
70.00	744.0
71.90	512.0
73.00	4134.0
74.00	15565.0
75.00	43320.0
76.00	3908.0
77.00	496.0
78.00	364.0
78.90	3340.0
79.90	977.0
80.90	3350.0
81.90	823.0
83.00	124.0
86.10	105.0
87.00	3488.0
88.00	3340.0
90.90	318.0
92.00	2652.0
93.00	3854.0
94.00	10180.0
95.10	83384.0
96.00	5629.0
97.00	185.0
103.90	452.0
104.80	135.0
105.90	406.0
110.80	110.0
112.80	119.0
115.90	354.0
117.00	695.0
117.90	326.0
118.90	575.0
127.90	270.0
129.00	129.0
129.90	395.0
131.00	126.0
134.90	139.0
136.90	155.0
140.90	1019.0
142.00	108.0
143.00	1350.0
144.00	105.0
144.90	409.0
145.90	158.0
148.00	224.0
154.90	235.0
157.00	148.0
161.00	113.0
170.90	126.0
172.00	752.0
173.00	615.0
174.00	64584.0
175.00	4707.0
176.00	62000.0
177.00	4010.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.90	758.0
37.00	3706.0
38.00	3081.0
39.00	1412.0
39.90	2608.0
44.00	615.0
44.90	683.0
47.00	815.0
48.00	481.0
49.00	3122.0
50.00	15244.0
51.00	4539.0
51.90	142.0
54.90	196.0
56.00	1311.0
57.00	2233.0
60.00	818.0
61.00	4254.0
62.00	4408.0
63.00	3544.0
64.00	483.0
65.00	627.0
67.00	221.0
68.00	8727.0
69.00	8694.0
70.00	700.0
72.00	482.0
73.00	4032.0
74.00	15370.0
75.00	42808.0
76.00	3863.0
77.00	433.0
78.00	341.0
78.90	3308.0
79.90	916.0
80.90	3280.0
81.90	815.0
83.00	122.0
86.00	125.0
87.00	3403.0
88.00	3272.0
90.90	333.0
92.00	2498.0
93.00	3576.0
94.00	10038.0
95.10	82432.0
96.00	5449.0
97.00	156.0
104.00	452.0
104.80	141.0
105.90	395.0
110.80	105.0
112.90	135.0
115.90	328.0
117.00	684.0
117.90	302.0
118.90	610.0
127.90	269.0
129.00	136.0
130.00	391.0
131.00	123.0
134.90	137.0
137.00	158.0
140.90	978.0
141.90	109.0
143.00	1242.0
144.90	380.0
145.90	151.0
148.00	267.0
150.00	107.0
152.80	101.0
154.90	250.0
157.00	144.0
161.00	105.0
170.90	107.0
172.00	747.0
172.90	596.0
174.00	66208.0
175.00	4539.0
176.00	63768.0
177.00	4038.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038