

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122922\
 Data File : VU052615.D
 Acq On : 29 Dec 2022 19:25
 Operator : JC/MD
 Sample : N6189-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	93	rVB	105059	117175	11.66%	1.830%
2	1.774	129	135	147	rVB2	15410	18632	1.85%	0.291%
3	1.916	170	179	194	rBV	94701	124691	12.41%	1.947%
4	2.568	367	382	400	rBV	171908	281612	28.02%	4.397%
5	3.044	521	530	549	rVB2	7714	17357	1.73%	0.271%
6	4.649	1012	1029	1078	rBV	97587	435924	43.38%	6.807%
7	5.060	1141	1157	1176	rBV	144372	319829	31.82%	4.994%
8	5.722	1342	1363	1391	rBV2	299698	779138	77.53%	12.166%
9	6.247	1512	1526	1543	rBV	214967	409789	40.78%	6.399%
10	6.687	1648	1663	1680	rBV	197603	381240	37.94%	5.953%
11	7.562	1922	1935	1951	rBV	81680	146129	14.54%	2.282%
12	7.896	2025	2039	2056	rBV	314749	553169	55.04%	8.637%
13	8.176	2115	2126	2138	rBV	53538	90107	8.97%	1.407%
14	8.632	2255	2268	2302	rBV2	510702	1004974	100.00%	15.692%
15	9.414	2498	2511	2536	rBV	317083	515596	51.30%	8.051%
16	10.751	2914	2927	2944	rBV	155323	246639	24.54%	3.851%
17	10.889	2961	2970	2980	rBV	6579	10622	1.06%	0.166%
18	11.806	3240	3255	3274	rBV	285488	461205	45.89%	7.201%
19	12.188	3362	3374	3393	rBV	308272	490489	48.81%	7.659%




Sum of corrected areas: 6404317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122922\
Data File : VU052615.D
Acq On : 29 Dec 2022 19:25
Operator : JC/MD
Sample : N6189-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

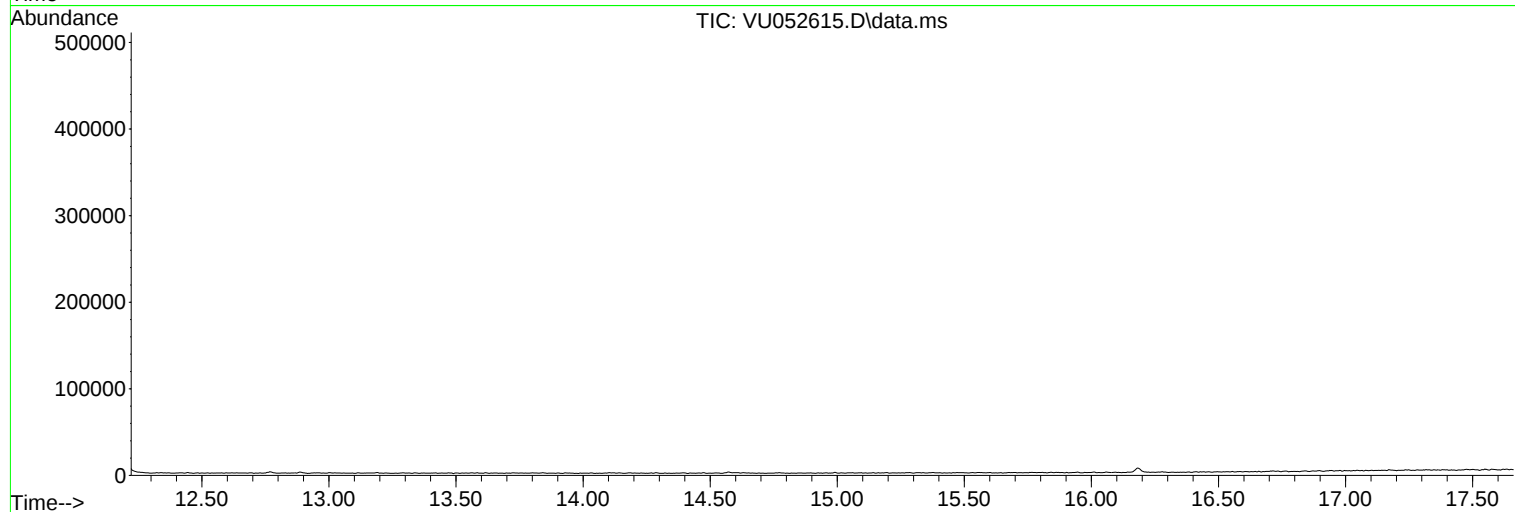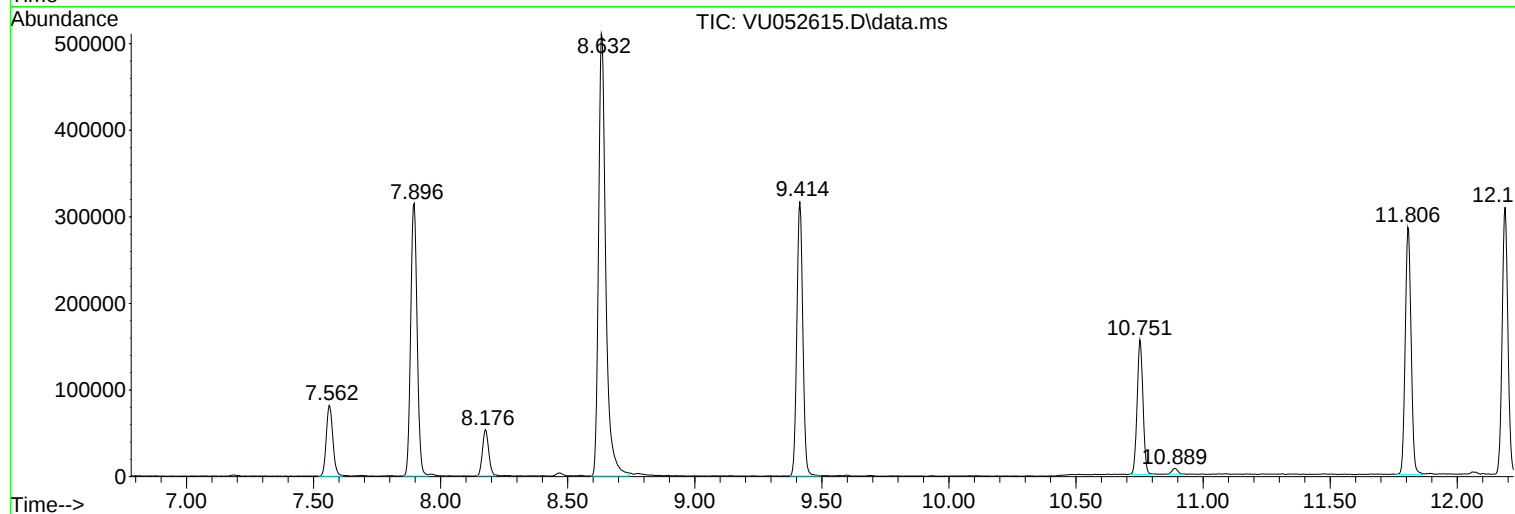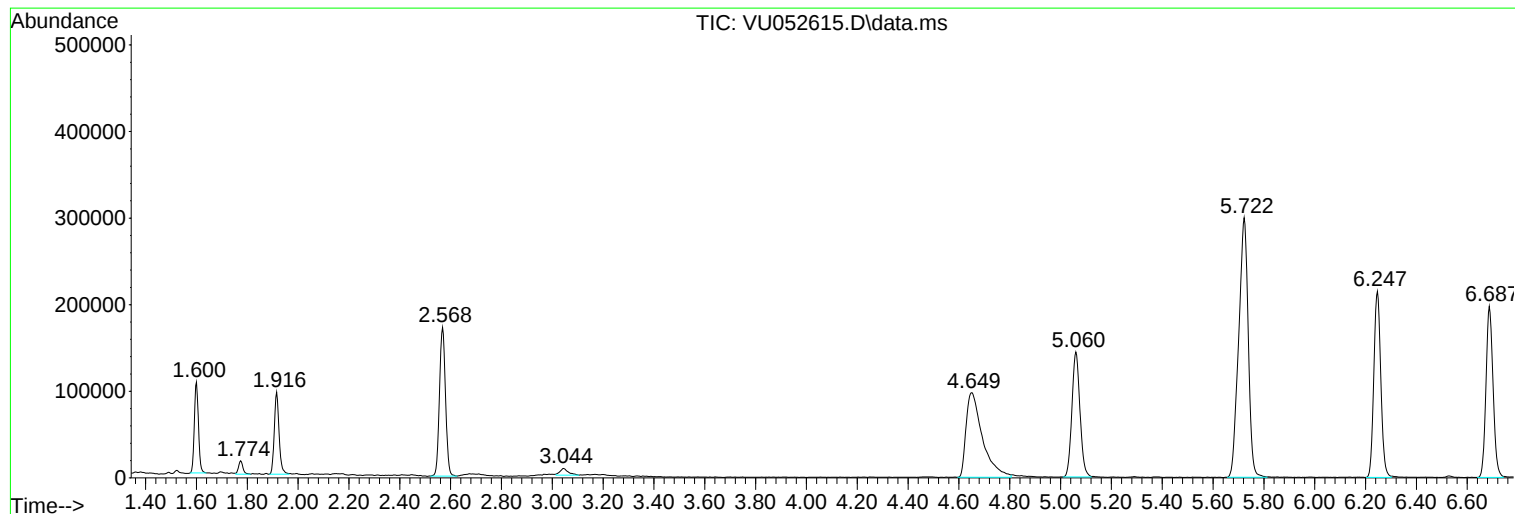

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122922\
Data File : VU052615.D
Acq On : 29 Dec 2022 19:25
Operator : JC/MD
Sample : N6189-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122922\
Data File : VU052615.D
Acq On : 29 Dec 2022 19:25
Operator : JC/MD
Sample : N6189-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
