
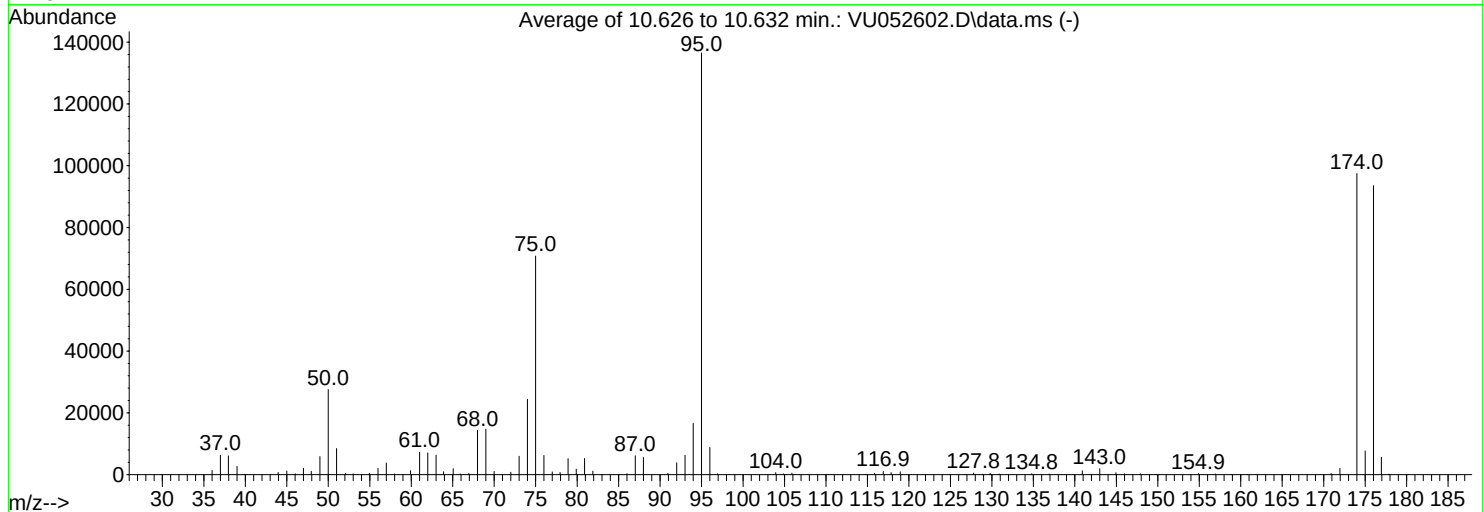


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122922\
 Data File : VU052602.D
 Acq On : 29 Dec 2022 09:38
 Operator : JC/MD
 Sample : BFB187
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB187

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Dec 30 00:58:31 2022

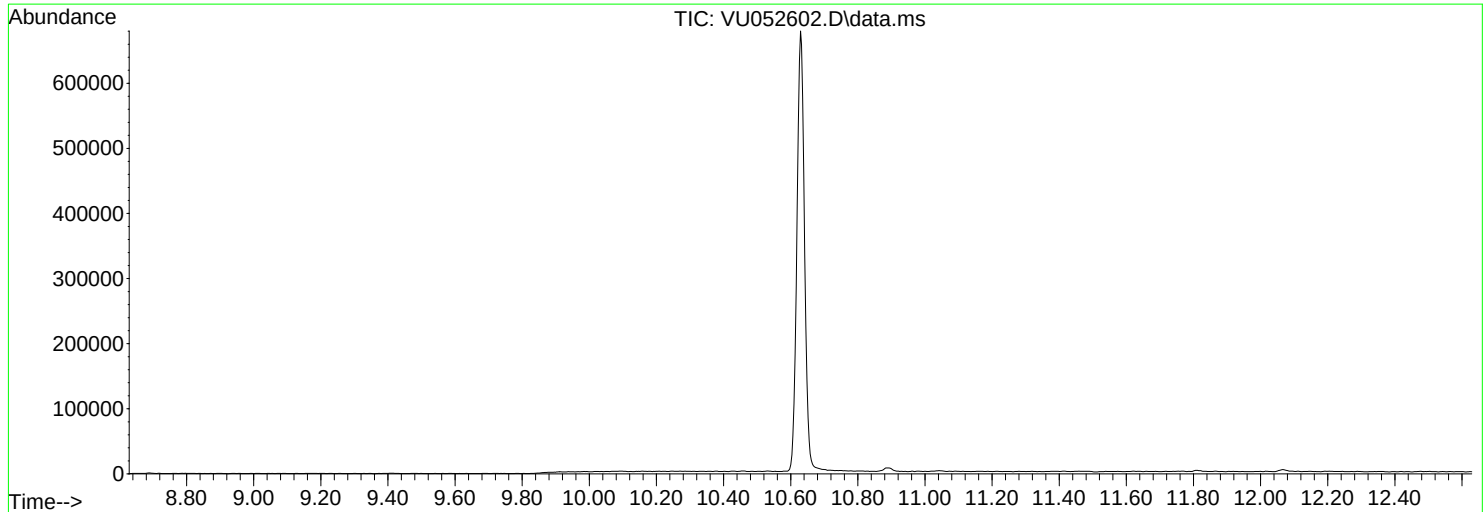

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	27547	PASS
75	95	30	80	51.8	70752	PASS
95	95	100	100	100.0	136555	PASS
96	95	5	9	6.5	8837	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.4	97483	PASS
175	174	5	9	7.9	7671	PASS
176	174	95	101	96.0	93547	PASS
177	176	5	9	6.0	5648	PASS

m/z	Abundance
36.00	2151.0
37.00	215.0
37.90	893.0
39.80	176.0
43.90	528.0
126.70	145.0
127.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
36.00	3466.0
37.00	6458.0
38.00	6743.0
39.00	2652.0
40.00	230.0
43.10	146.0
44.00	1253.0
45.00	1104.0
46.10	270.0
47.00	2095.0
47.90	1050.0
49.00	5711.0
50.00	27016.0
51.00	8173.0
52.10	423.0
53.00	273.0
55.00	465.0
56.00	2068.0
57.00	3605.0
58.00	160.0
59.90	1373.0
61.00	7390.0
62.00	6818.0
63.00	6111.0
63.90	976.0
65.00	1906.0
65.90	235.0
66.90	405.0
68.00	13772.0
69.00	14778.0
70.00	1055.0
72.00	730.0
73.00	5891.0
74.00	23744.0
75.00	68984.0
76.00	6147.0
77.00	883.0
77.90	777.0
78.90	5156.0
79.90	1714.0
80.90	5165.0
81.90	1102.0
86.00	336.0
87.00	6164.0
88.00	5148.0
91.00	462.0
92.00	3814.0
93.00	6188.0
94.00	16288.0
95.00	131456.0
96.00	8784.0
96.90	260.0
104.00	576.0
104.80	271.0
105.90	480.0
114.70	102.0
115.80	445.0
116.90	1036.0
117.80	645.0
118.90	923.0
126.80	237.0
127.90	597.0
128.80	189.0
129.80	419.0
130.90	221.0
134.90	295.0
136.90	222.0
140.90	1143.0
142.00	185.0
143.00	1784.0
144.90	604.0
146.00	225.0
147.90	301.0
154.90	302.0
156.90	200.0
158.90	124.0
160.80	150.0
170.90	347.0
171.90	1914.0
174.00	92224.0
175.00	7233.0
176.00	87392.0
177.00	5293.0
177.90	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
36.00	3554.0
37.00	6608.0
38.00	7226.0
39.00	2761.0
39.90	276.0
43.00	113.0
44.00	1274.0
45.00	1214.0
46.10	258.0
47.00	2148.0
47.90	1157.0
49.00	6002.0
50.00	28576.0
51.00	8743.0
52.10	404.0
53.00	286.0
54.90	514.0
56.00	2080.0
57.00	3962.0
58.00	199.0
59.90	1370.0
61.00	7446.0
62.00	7324.0
63.00	6582.0
63.90	947.0
65.00	1978.0
65.90	224.0
66.90	409.0
68.00	14784.0
69.00	15059.0
70.00	1048.0
72.00	819.0
73.00	6106.0
74.00	25216.0
75.00	73432.0
76.00	6415.0
77.00	936.0
77.90	748.0
78.90	5436.0
79.90	1857.0
80.90	5419.0
81.90	1193.0
83.00	111.0
86.00	315.0
87.00	6250.0
88.00	5760.0
90.90	405.0
92.00	3904.0
93.00	6538.0
94.00	17264.0
95.00	141184.0
96.00	9179.0
96.90	269.0
103.90	702.0
104.80	277.0
105.90	520.0
106.80	111.0
114.80	117.0
115.90	473.0
116.90	1086.0
117.90	711.0
119.00	955.0
126.80	264.0
127.90	632.0
128.90	189.0
129.80	508.0
130.90	244.0
134.80	333.0
136.90	225.0
140.90	1272.0
141.90	183.0
143.00	2028.0
145.00	633.0
146.00	262.0
147.90	273.0
149.80	100.0
153.90	108.0
154.90	357.0
157.00	247.0
158.80	125.0
160.80	129.0
170.90	375.0
172.00	2054.0
174.00	100592.0
175.00	7980.0
176.00	96848.0
177.00	5863.0
177.90	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187

m/z	Abundance
36.00	3552.0
37.00	6381.0
38.00	6875.0
39.00	2724.0
39.90	295.0
44.00	1188.0
45.00	1247.0
46.00	206.0
47.00	1910.0
48.00	1059.0
49.00	5821.0
50.00	27048.0
51.00	8449.0
52.10	386.0
53.00	253.0
54.90	486.0
56.00	1904.0
57.00	3865.0
58.00	208.0
59.90	1173.0
61.00	6950.0
62.00	7069.0
63.00	6279.0
63.90	862.0
65.10	1848.0
65.90	182.0
67.00	376.0
68.00	14460.0
69.00	14264.0
70.00	1009.0
72.00	791.0
73.00	5863.0
74.00	24192.0
75.00	69840.0
76.00	6179.0
77.00	795.0
78.00	658.0
78.90	5030.0
79.90	1801.0
80.90	5203.0
81.90	1190.0
83.00	126.0
86.00	283.0
87.00	5901.0
88.00	5719.0
90.90	366.0
92.00	3778.0
93.00	6094.0
94.00	16366.0
95.00	137024.0
96.00	8547.0
97.00	242.0
103.90	747.0
104.90	252.0
105.90	531.0
106.80	118.0
114.90	125.0
115.80	536.0
116.90	1054.0
117.90	699.0
119.00	897.0
126.80	280.0
127.80	611.0
128.90	162.0
129.80	544.0
130.90	220.0
134.70	300.0
136.90	188.0
140.90	1338.0
141.90	117.0
143.00	2040.0
145.00	592.0
146.00	278.0
147.90	207.0
149.80	119.0
153.90	107.0
154.90	351.0
156.90	229.0
158.80	136.0
170.90	335.0
172.00	2091.0
174.00	99632.0
175.00	7799.0
176.00	96400.0
176.90	5789.0
177.80	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB187