

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U123019\
 Data File : VU036371.D
 Acq On : 30 Dec 2019 15:29
 Operator : JC/MD
 Sample : VU1230WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK09

Quant Time: Dec 31 07:42:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 31 07:33:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	282949	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	272194	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	120306	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	99446	4.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.80%
7) Chloroethane-d5	1.93	69	91747	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.60%
11) 1,1-Dichloroethene-d2	2.59	63	146502	3.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.80%
20) 2-Butanone-d5	4.69	46	285986	54.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.08%
24) Chloroform-d	5.11	84	202594	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.75	65	114984	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
32) Benzene-d6	5.77	84	401523	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
36) 1,2-Dichloropropane-d6	6.73	67	130576	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.93	98	368399	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
43) trans-1,3-Dichloropropene-	8.21	79	56057	4.82	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.40%
46) 2-Hexanone-d5	8.67	63	264674	52.95	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.90%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	108256	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	12.22	152	126697	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%


Target Compounds					Ovalue
13) Acetone	2.68	43	7804	2.310 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU123019\
Data File : VU036371.D
Acq On : 30 Dec 2019 15:29
Operator : JC/MD
Sample : VU1230WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK09

Quant Time: Dec 31 07:42:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 31 07:33:27 2019
Response via : Initial Calibration

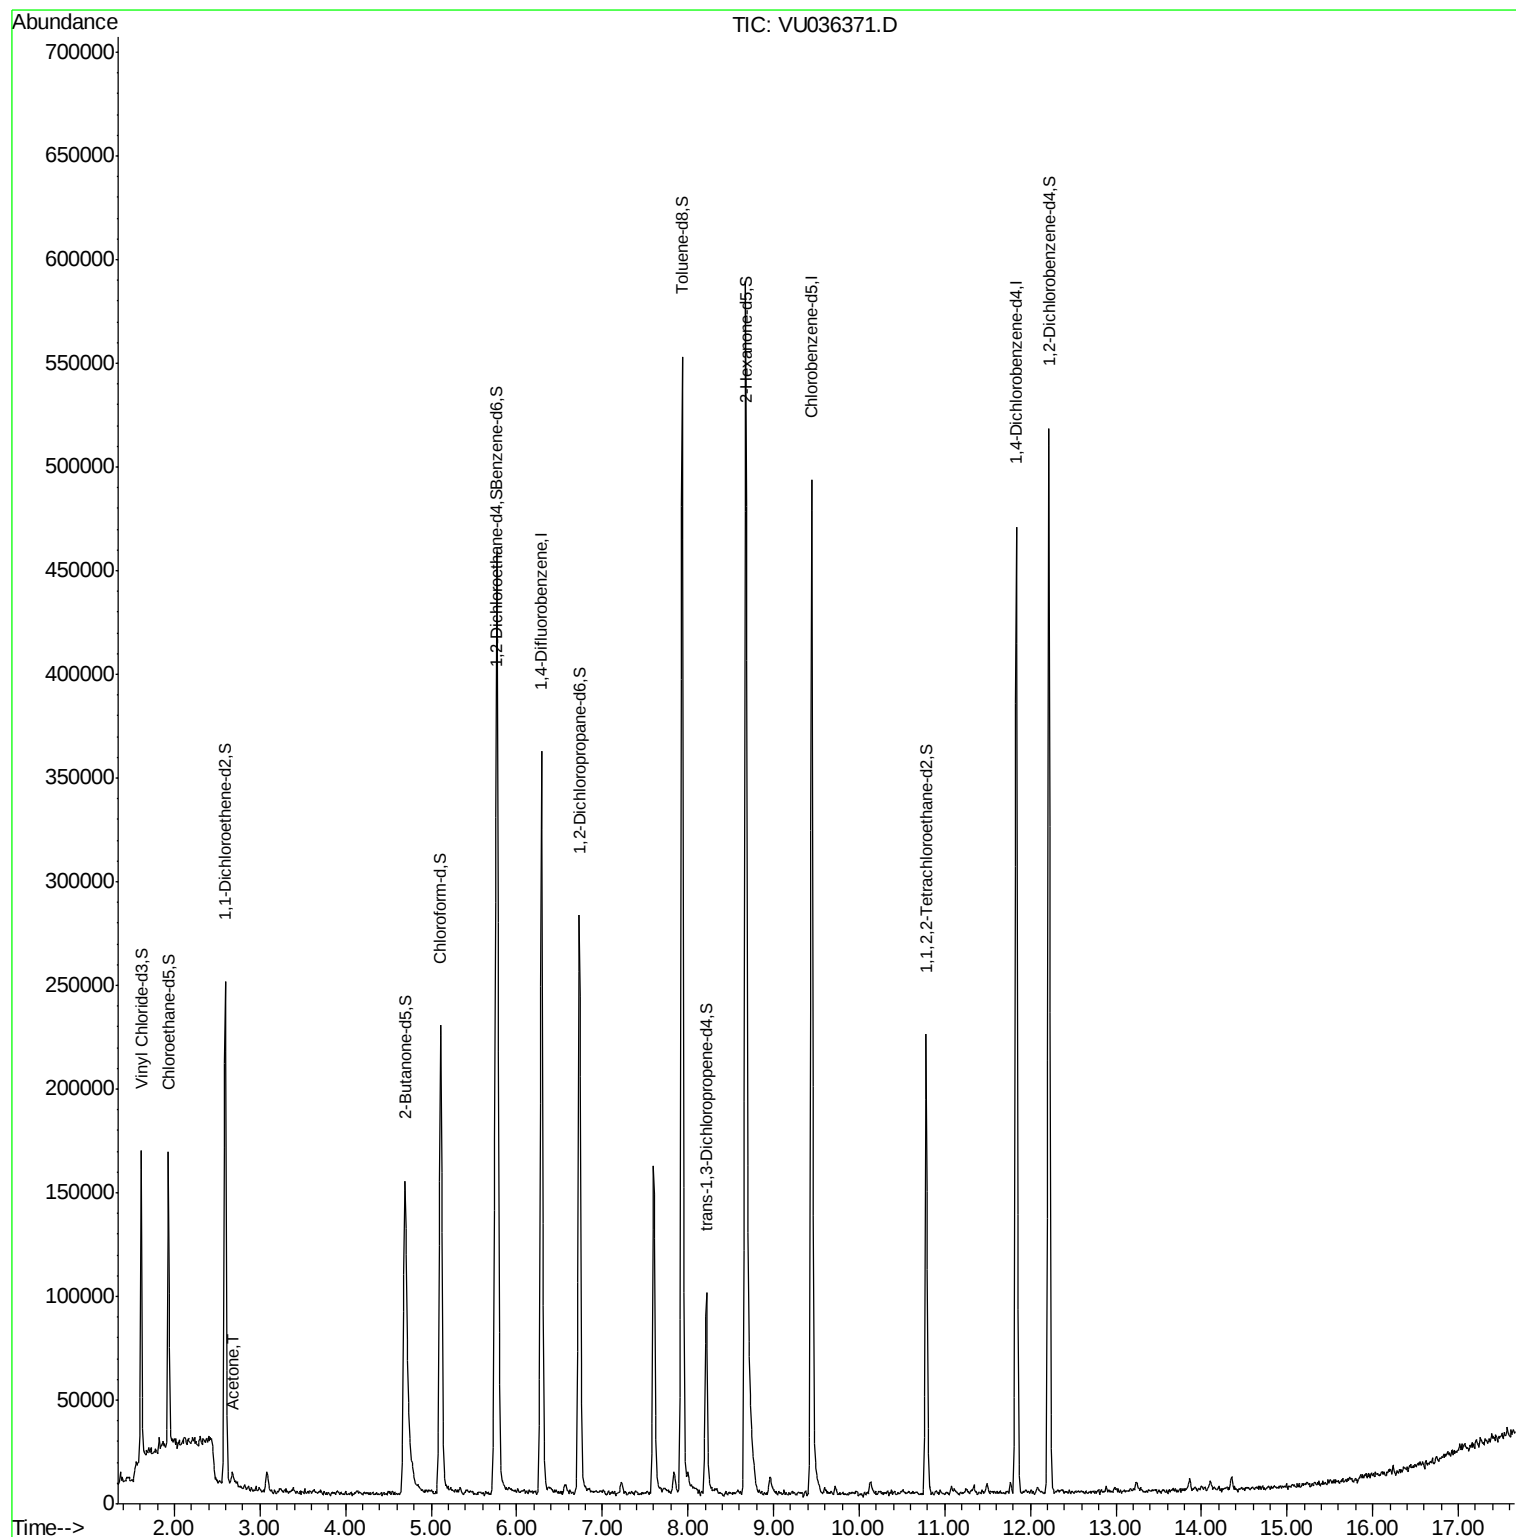

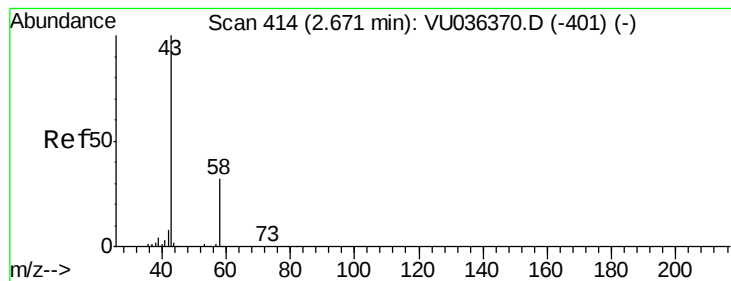

#13

Acetone

Concen: 2.310 ug/L

RT: 2.68 min Scan# 417

Delta R.T. 0.01 min

Lab File: VU036371.D

Acq: 30 Dec 2019 15:29

Instrument :

MSVOA_U

ClientSampleId :

VBLK09

Tot Ion: 43 Resp: 7804

Ion Ratio Lower Upper

43 100

58 41.3 0.0 57.0

