


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU123019\
 Data File : VU036369.D
 Acq On : 30 Dec 2019 11:08
 Operator : JC/MD
 Sample : BFB29
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB29

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jan 03 17:51:02 2020

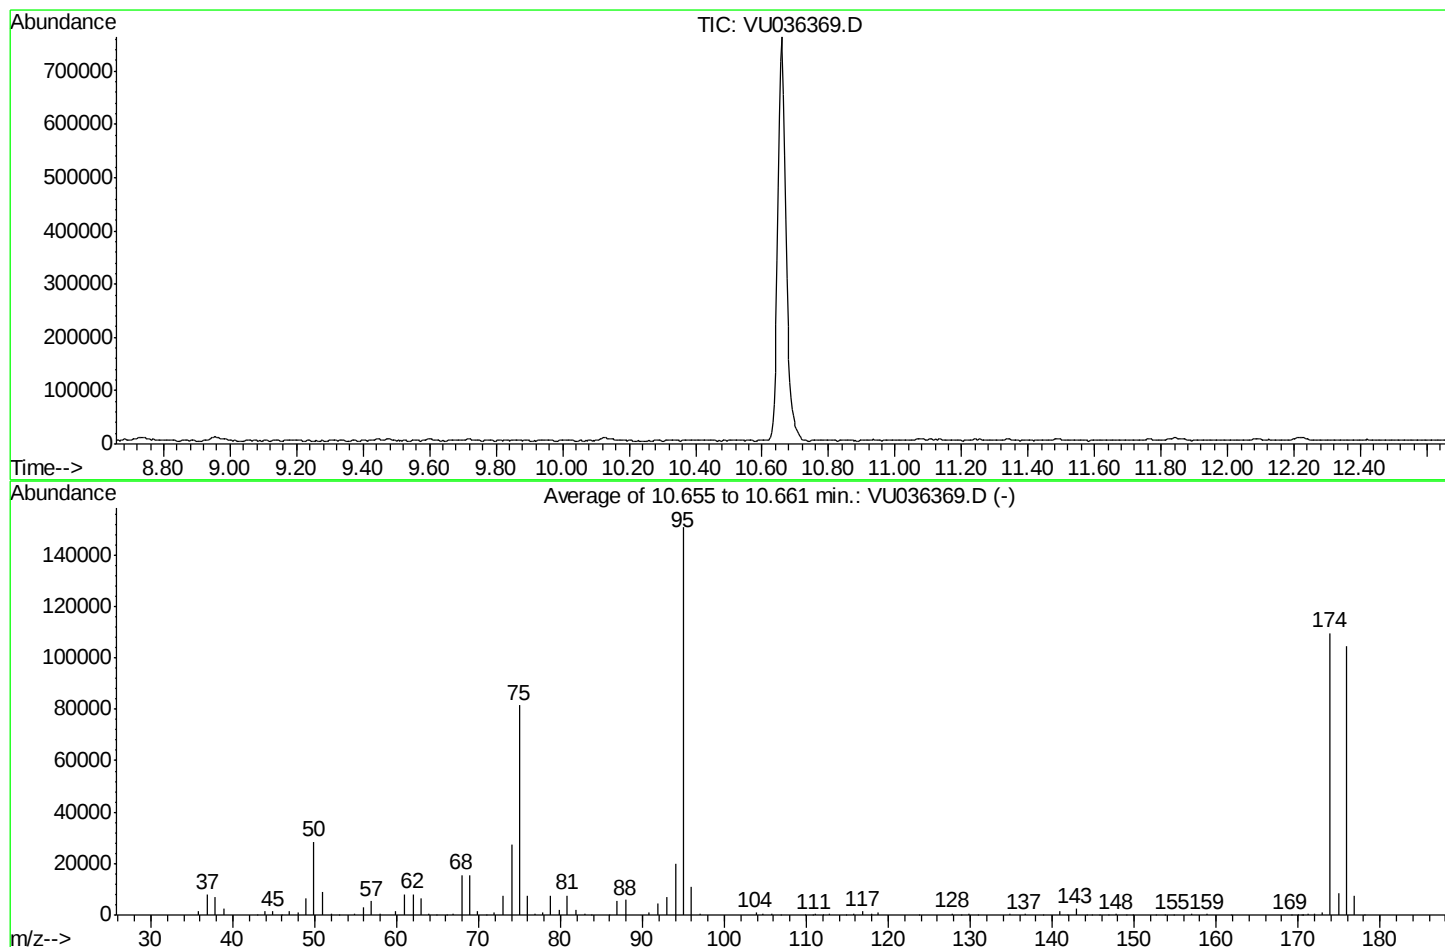

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	28434	PASS
75	95	30	80	54.1	81485	PASS
95	95	100	100	100.0	150720	PASS
96	95	5	9	7.1	10746	PASS
173	174	0.00	2	0.9	961	PASS
174	95	50	120	72.7	109501	PASS
175	174	5	9	7.7	8411	PASS
176	174	95	101	95.3	104394	PASS
177	176	5	9	7.2	7522	PASS

m/z	Abundance
37.90	126.0
38.90	433.0
39.80	316.0
40.90	515.0
41.80	295.0
42.90	377.0
43.90	1060.0
50.20	115.0
52.90	107.0
53.90	126.0
54.90	424.0
55.90	309.0
56.90	390.0
58.70	126.0
68.10	142.0
68.80	216.0
69.90	125.0
71.00	134.0
73.10	153.0
76.80	141.0
83.00	140.0
84.90	203.0
91.00	130.0
92.90	184.0
206.90	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.80	1522.0
36.90	7817.0
37.90	7435.0
38.90	2906.0
39.80	332.0
40.80	435.0
41.90	347.0
43.00	359.0
43.90	2351.0
44.90	1516.0
45.90	170.0
46.90	1464.0
47.90	863.0
48.90	6101.0
49.90	28968.0
50.90	8819.0
52.00	546.0
53.00	183.0
54.90	646.0
56.00	3385.0
57.00	5795.0
57.90	312.0
59.90	1198.0
60.90	7836.0
62.00	7693.0
62.90	6404.0
63.90	669.0
64.90	103.0
66.10	100.0
67.00	690.0
68.00	15543.0
68.90	15611.0
70.00	1754.0
71.00	377.0
71.80	840.0
73.00	7769.0
74.00	26880.0
75.00	80640.0
76.00	7465.0
76.80	930.0
77.90	852.0
78.80	7296.0
79.90	2040.0
80.90	7615.0
81.80	1678.0
83.00	398.0
85.00	129.0
86.00	215.0
86.90	5485.0
87.90	5620.0
90.90	938.0
91.90	4344.0
92.90	7418.0
94.00	18880.0
95.00	148032.0
96.00	10033.0
97.00	486.0
103.90	968.0
104.80	265.0
105.80	651.0
109.90	273.0
111.00	359.0
112.80	285.0
114.90	171.0
115.80	638.0
116.90	1146.0
117.90	559.0
118.80	925.0
123.80	110.0
127.90	676.0
128.90	241.0
129.80	546.0
130.90	228.0
134.70	310.0
136.70	625.0
138.90	157.0
140.90	1619.0
141.80	289.0
142.90	2038.0
144.80	171.0
145.80	162.0
146.80	114.0
147.90	354.0
149.10	261.0
149.90	200.0
152.70	118.0
154.80	200.0
157.00	364.0
159.00	279.0
170.40	194.0
171.40	330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

172.00	257.0
172.90	942.0
173.90	102808.0
174.90	7903.0
175.90	98728.0
176.90	6915.0
178.10	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.80	1728.0
36.90	8024.0
37.90	7557.0
38.90	2881.0
39.90	317.0
40.90	440.0
41.80	258.0
42.90	468.0
43.90	2374.0
44.90	1482.0
45.90	115.0
46.90	1711.0
48.00	1074.0
48.90	6358.0
49.90	29264.0
50.90	9293.0
52.00	547.0
53.00	177.0
54.90	728.0
56.00	3349.0
57.00	5918.0
57.90	355.0
58.70	115.0
59.80	1360.0
60.90	8074.0
62.00	8286.0
62.90	6459.0
64.00	645.0
64.80	115.0
66.90	775.0
67.90	16023.0
68.90	15940.0
70.00	1894.0
70.90	341.0
71.90	886.0
72.90	8073.0
74.00	28464.0
75.00	84464.0
76.00	7418.0
76.80	932.0
77.90	875.0
78.80	7667.0
79.90	2055.0
80.80	7717.0
81.80	1875.0
83.00	436.0
83.80	123.0
85.00	128.0
85.90	275.0
86.90	5612.0
87.90	6093.0
90.80	988.0
91.90	4761.0
93.00	7779.0
94.00	20824.0
95.00	155520.0
95.90	11171.0
96.90	501.0
103.90	1012.0
104.70	280.0
105.80	650.0
109.80	217.0
111.00	317.0
112.00	111.0
112.90	333.0
114.90	151.0
115.80	682.0
116.90	1413.0
117.90	596.0
118.80	1024.0
123.80	202.0
127.80	626.0
128.80	256.0
129.90	497.0
131.00	279.0
134.80	254.0
136.70	447.0
138.90	138.0
140.90	1737.0
141.80	283.0
142.90	2379.0
144.90	213.0
145.70	143.0
146.80	104.0
147.80	301.0
149.10	185.0
149.90	181.0
153.80	146.0
154.80	218.0
157.00	251.0
158.90	298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

161.80	120.0
169.20	129.0
170.40	154.0
171.30	346.0
172.00	287.0
172.90	1025.0
173.90	112896.0
174.90	8811.0
175.90	107464.0
176.90	7781.0
178.10	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.80	1550.0
36.90	7410.0
37.90	6873.0
38.90	2709.0
39.90	279.0
40.90	488.0
41.80	163.0
42.90	561.0
43.90	2321.0
44.90	1422.0
46.90	1695.0
48.00	1119.0
48.90	6476.0
49.90	27072.0
51.00	8515.0
52.00	509.0
53.10	122.0
54.90	725.0
55.90	3100.0
56.90	5377.0
57.90	368.0
58.70	134.0
59.80	1398.0
60.90	7810.0
62.00	8147.0
62.90	5944.0
64.00	550.0
64.70	120.0
66.90	726.0
67.90	15249.0
68.90	15424.0
69.90	1780.0
70.90	259.0
71.90	852.0
72.90	7784.0
74.00	27288.0
75.00	79352.0
75.90	6845.0
76.80	700.0
77.80	751.0
78.80	7543.0
79.90	1847.0
80.90	7243.0
81.80	1923.0
83.00	417.0
83.80	189.0
85.10	109.0
85.80	270.0
86.90	5506.0
87.90	5917.0
90.80	842.0
91.90	4562.0
93.00	7020.0
94.00	20744.0
95.00	148608.0
95.90	11036.0
96.90	425.0
103.80	993.0
104.70	282.0
105.70	699.0
106.80	100.0
109.70	191.0
110.70	215.0
111.10	257.0
112.00	137.0
112.90	361.0
114.80	146.0
115.80	604.0
116.90	1475.0
117.90	577.0
118.80	1007.0
123.80	234.0
127.80	564.0
128.80	223.0
129.80	520.0
131.00	270.0
134.90	260.0
136.80	325.0
140.90	1822.0
141.80	228.0
142.90	2444.0
144.20	103.0
144.90	221.0
145.80	106.0
147.80	288.0
149.70	164.0
153.80	196.0
154.80	264.0
157.00	213.0
158.90	312.0
161.80	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

169.10	118.0
169.90	152.0
170.60	118.0
171.20	277.0
172.10	314.0
172.90	918.0
173.90	112800.0
174.90	8521.0
175.90	106992.0
176.90	7870.0
178.10	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29