
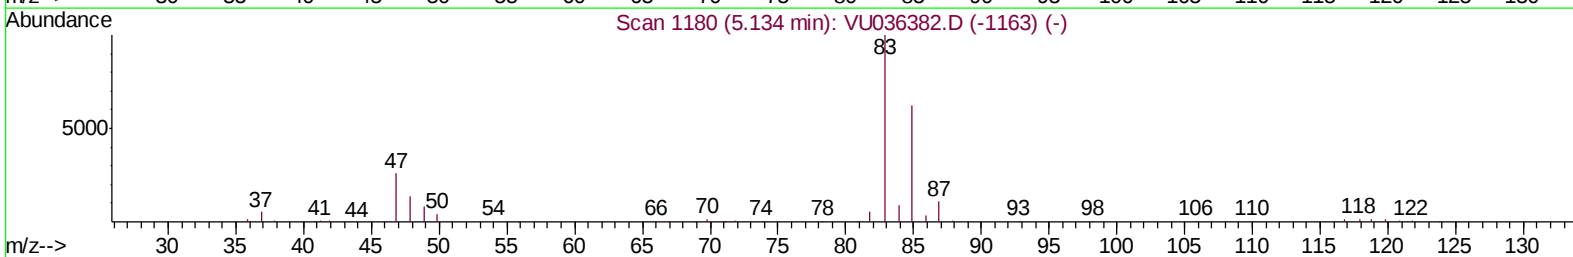
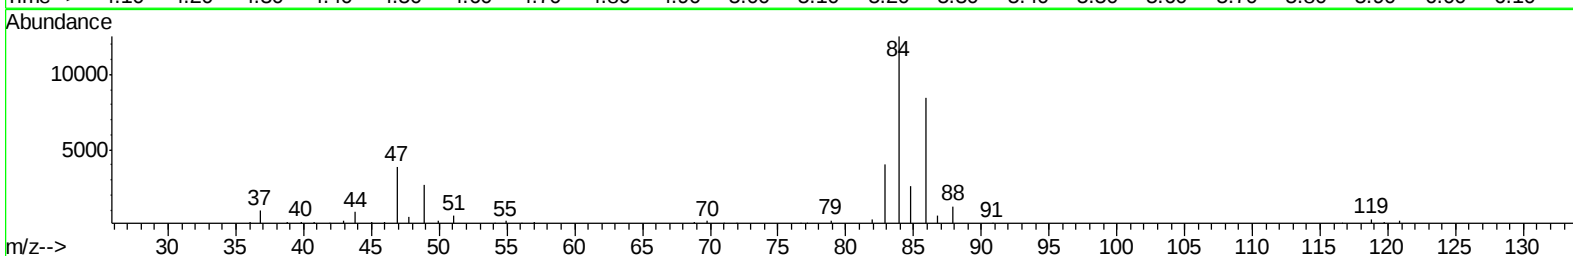


Data File : VU036384.D
Acq On : 31 Dec 2019 12:33
Operator : JC/MD
Sample : K6459-15MS
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 01:22:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jan 01 01:19:59 2020
Response via : Initial Calibration

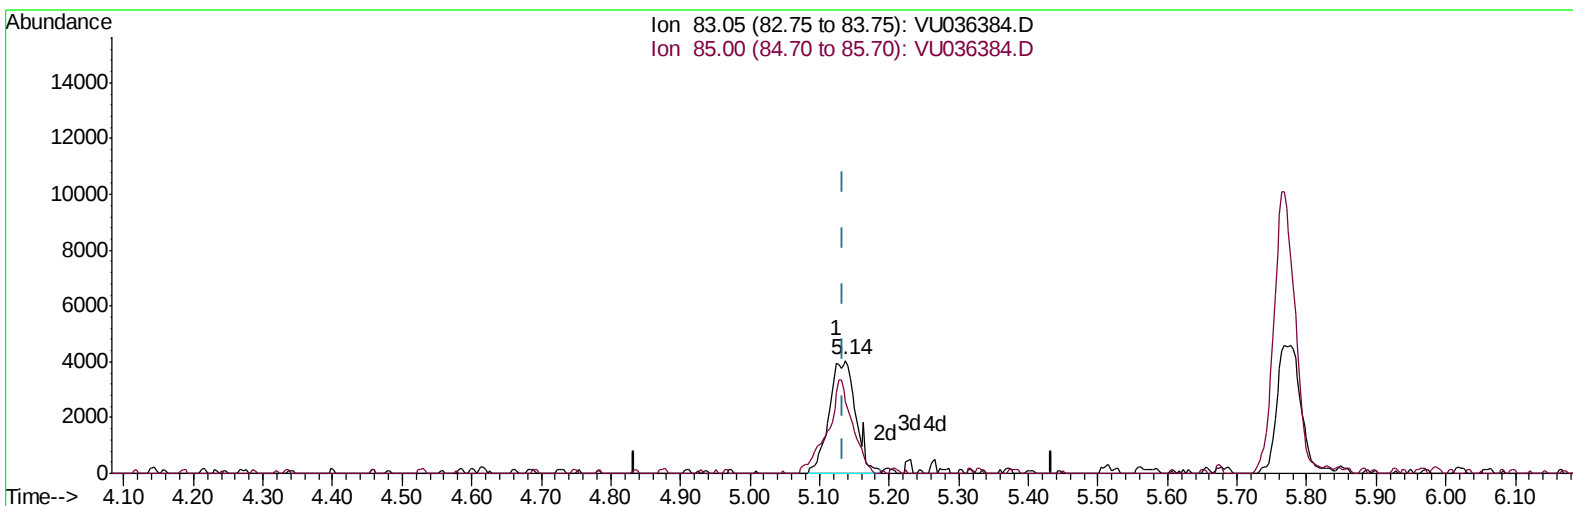

TIC: VU036384.D

(25) Chloroform (T)

5.137min (+0.003) 0.27ug/L m

response 10735

Ion	Exp%	Act%
83.05	100	100
85.00	63.00	63.85
0.00	0.00	0.00
0.00	0.00	0.00