


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU123119\
 Data File : VU036381.D
 Acq On : 31 Dec 2019 09:14
 Operator : JC/MD
 Sample : BFB27
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB27

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR122819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jan 01 01:19:59 2020

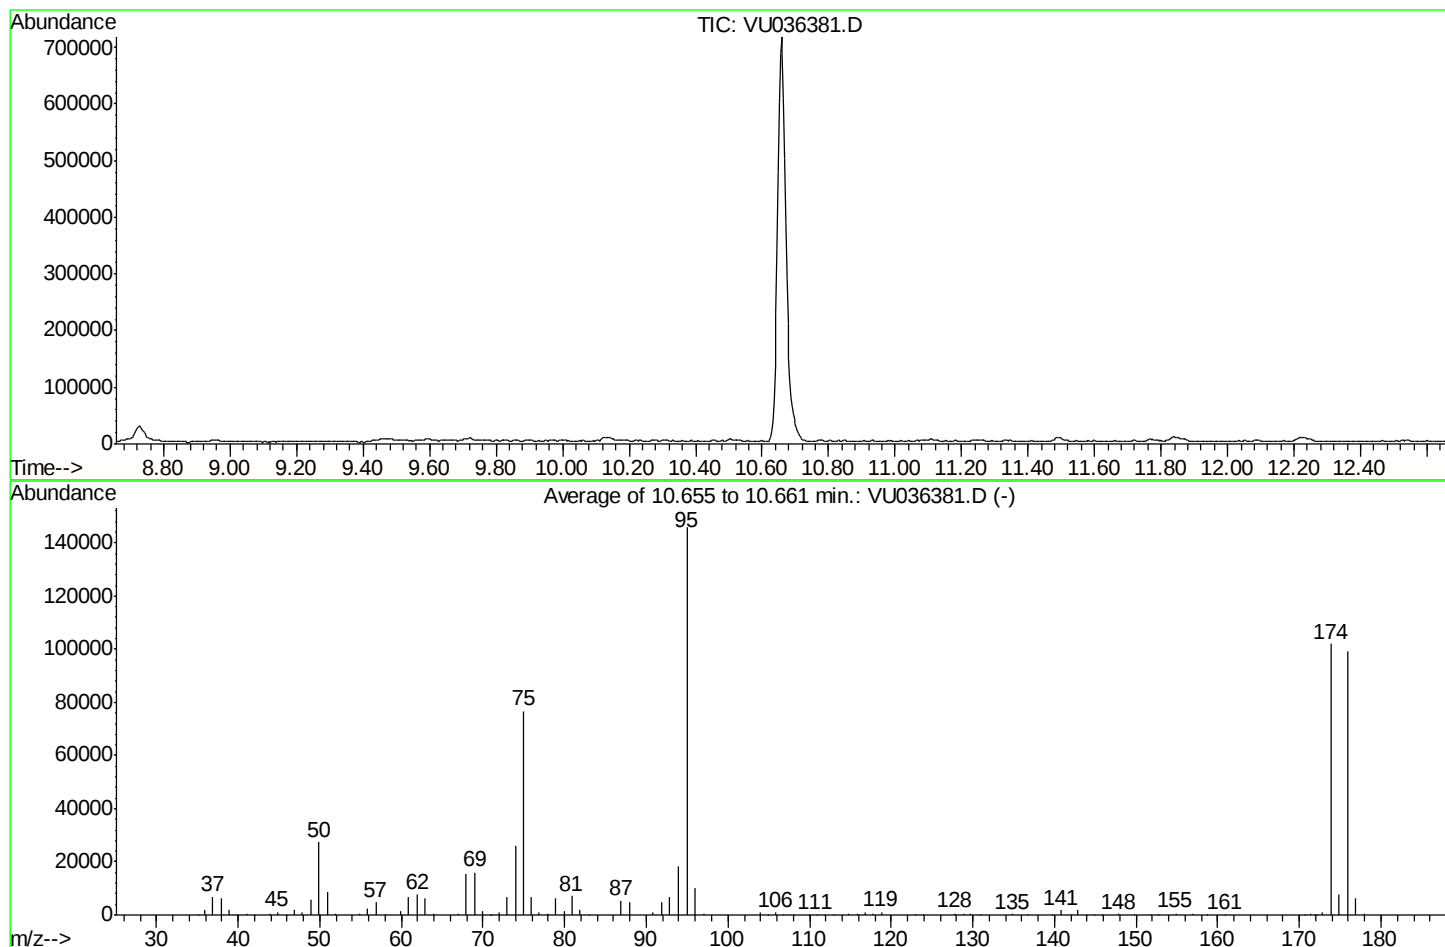

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	27328	PASS
75	95	30	80	52.5	76568	PASS
95	95	100	100	100.0	145834	PASS
96	95	5	9	7.0	10158	PASS
173	174	0.00	2	0.9	951	PASS
174	95	50	120	69.9	101877	PASS
175	174	5	9	7.6	7741	PASS
176	174	95	101	97.6	99408	PASS
177	176	5	9	6.4	6320	PASS

m/z	Abundance
35.90	2376.0
36.90	6983.0
37.90	7245.0
38.90	2498.0
39.80	328.0
41.20	362.0
42.00	119.0
42.90	242.0
43.90	2054.0
44.80	1042.0
46.00	190.0
46.90	1862.0
47.90	928.0
48.90	5751.0
49.90	27720.0
51.00	8652.0
52.00	303.0
54.80	604.0
55.90	2595.0
56.90	4764.0
57.90	184.0
59.80	1371.0
60.90	6820.0
62.00	7603.0
62.90	6065.0
64.10	540.0
67.00	646.0
67.90	15428.0
69.00	16656.0
69.90	1556.0
70.90	179.0
71.90	857.0
72.90	7023.0
74.00	25776.0
75.00	75416.0
75.90	6850.0
76.80	764.0
77.90	310.0
78.90	6375.0
79.90	1658.0
80.90	7473.0
81.80	1502.0
82.90	269.0
86.90	5171.0
88.00	4942.0
90.90	1030.0
91.90	4724.0
92.90	6457.0
94.00	17936.0
95.00	144640.0
96.00	10112.0
97.00	408.0
103.90	849.0
104.90	273.0
105.90	891.0
106.80	191.0
108.10	105.0
109.90	162.0
110.80	188.0
111.80	189.0
112.90	183.0
114.80	302.0
115.80	786.0
116.90	921.0
117.80	700.0
118.80	1111.0
123.80	220.0
127.80	707.0
128.90	321.0
129.70	555.0
130.90	238.0
134.90	284.0
140.90	1688.0
142.10	250.0
142.90	1664.0
143.90	143.0
144.90	155.0
145.80	267.0
147.90	400.0
151.80	149.0
154.90	515.0
156.90	461.0
160.90	140.0
170.60	100.0
171.30	295.0
171.80	342.0
172.90	873.0
173.90	98528.0
174.90	7362.0
175.90	96576.0
176.90	6282.0
178.00	334.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.10	142.0
35.90	2367.0
36.90	7085.0
37.90	6776.0
38.90	2623.0
39.80	339.0
41.10	336.0
42.00	207.0
42.80	313.0
43.90	1967.0
44.80	1119.0
45.90	142.0
46.90	1780.0
47.90	938.0
48.90	5957.0
49.90	27656.0
51.00	9206.0
52.00	387.0
54.90	655.0
55.90	2785.0
56.90	5085.0
58.00	205.0
59.90	1454.0
60.90	7022.0
62.00	8007.0
62.90	6684.0
64.00	552.0
67.00	622.0
68.00	16071.0
69.00	16528.0
69.90	1526.0
70.90	128.0
71.90	792.0
72.90	6884.0
74.00	26936.0
75.00	78912.0
75.90	6668.0
76.90	908.0
77.90	378.0
78.90	6577.0
79.90	1694.0
80.90	7450.0
81.90	1852.0
83.00	345.0
86.90	5611.0
88.00	5172.0
90.90	914.0
91.90	4738.0
92.90	6803.0
94.00	18784.0
95.00	149824.0
96.00	10610.0
97.00	407.0
103.90	854.0
104.90	192.0
105.90	975.0
106.90	222.0
109.90	213.0
110.90	261.0
111.80	258.0
112.90	180.0
114.80	300.0
115.80	713.0
116.90	1046.0
117.80	655.0
118.80	1117.0
123.80	216.0
127.80	686.0
128.90	365.0
129.70	494.0
130.90	227.0
134.80	299.0
139.70	134.0
140.90	1901.0
142.10	238.0
142.90	1893.0
143.90	174.0
144.80	172.0
145.80	199.0
147.90	248.0
149.70	107.0
151.80	131.0
152.70	171.0
154.80	548.0
157.00	364.0
158.70	109.0
160.90	133.0
170.60	183.0
171.30	284.0
171.80	283.0
172.80	973.0
173.90	104904.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

174.90	7858.0
175.90	102264.0
176.90	6502.0
178.00	289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.10	146.0
35.90	2051.0
36.90	6840.0
37.90	6123.0
38.90	2652.0
39.80	378.0
41.10	318.0
41.90	267.0
42.80	377.0
43.90	1996.0
44.90	1069.0
45.80	140.0
46.90	1628.0
47.90	907.0
48.90	5597.0
49.90	26608.0
51.00	8642.0
51.90	407.0
54.90	701.0
55.90	2677.0
57.00	4821.0
58.00	222.0
59.90	1475.0
60.90	6781.0
62.00	7417.0
62.90	6348.0
64.00	509.0
67.00	572.0
68.00	15515.0
69.00	15310.0
69.90	1390.0
71.10	103.0
71.90	687.0
73.00	6490.0
74.00	25864.0
75.00	75376.0
76.00	6335.0
76.90	1008.0
77.90	533.0
78.90	6198.0
79.90	1523.0
80.90	6863.0
81.90	1815.0
83.00	395.0
83.90	111.0
86.90	5479.0
87.90	4913.0
90.80	826.0
92.00	4562.0
92.90	6577.0
94.00	17728.0
95.00	143040.0
96.00	9754.0
97.10	324.0
103.90	757.0
104.80	170.0
105.90	903.0
106.90	236.0
109.90	201.0
110.80	318.0
111.80	206.0
112.90	128.0
114.80	256.0
115.80	540.0
116.80	957.0
117.70	569.0
118.80	963.0
122.90	120.0
123.90	187.0
127.80	621.0
128.90	386.0
129.70	356.0
130.90	195.0
134.80	344.0
136.80	142.0
139.70	130.0
140.80	1949.0
141.90	243.0
142.90	1939.0
143.90	138.0
144.80	149.0
145.90	128.0
147.80	190.0
152.70	184.0
154.80	446.0
157.00	261.0
158.70	119.0
160.90	141.0
170.60	242.0
171.30	256.0
172.10	421.0
172.80	1008.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

173.90	102200.0
174.90	8005.0
175.90	99384.0
176.90	6177.0
178.00	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27

m/z	Abundance
35.90	556.0
37.90	452.0
38.80	446.0
39.80	236.0
40.90	267.0
42.10	132.0
42.80	389.0
43.80	1435.0
50.80	106.0
54.90	236.0
55.90	225.0
56.80	109.0
59.00	101.0
66.90	178.0
69.00	206.0
69.90	120.0
81.10	203.0
82.90	132.0
84.10	110.0
96.90	111.0
101.30	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB27