




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU011724\  
Data File : VU057548.D  
Acq On : 17 Jan 2024 18:40  
Operator : MD/SY  
Sample : P1120-09 10X  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BGWH5

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/18/2024  
Supervised By :Mahesh Dadoda 01/18/2024

Quant Time: Jan 18 01:11:46 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR011124WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Jan 18 01:10:22 2024  
Response via : Initial Calibration

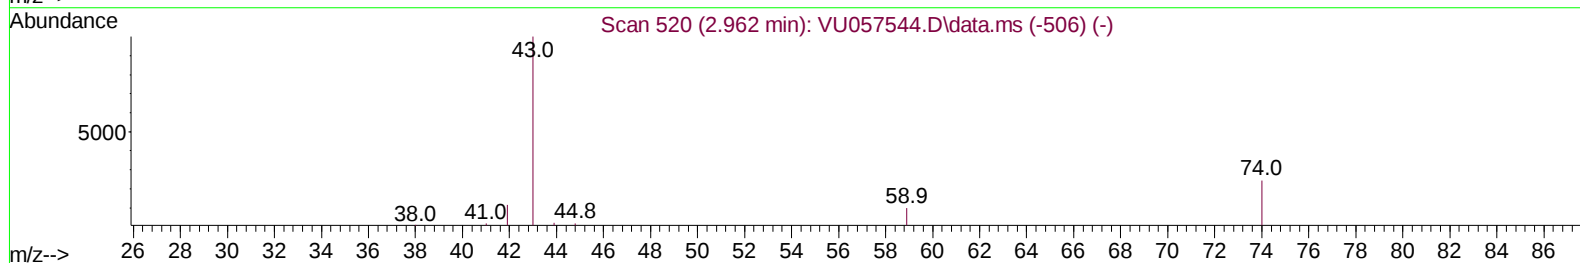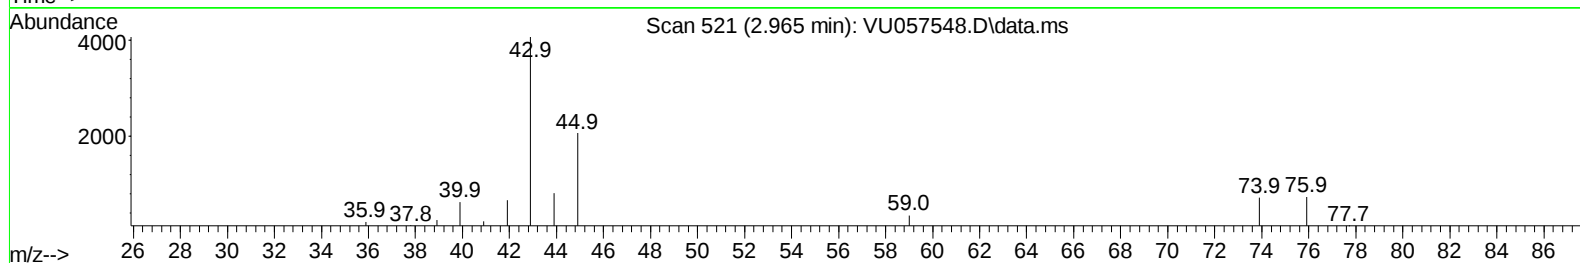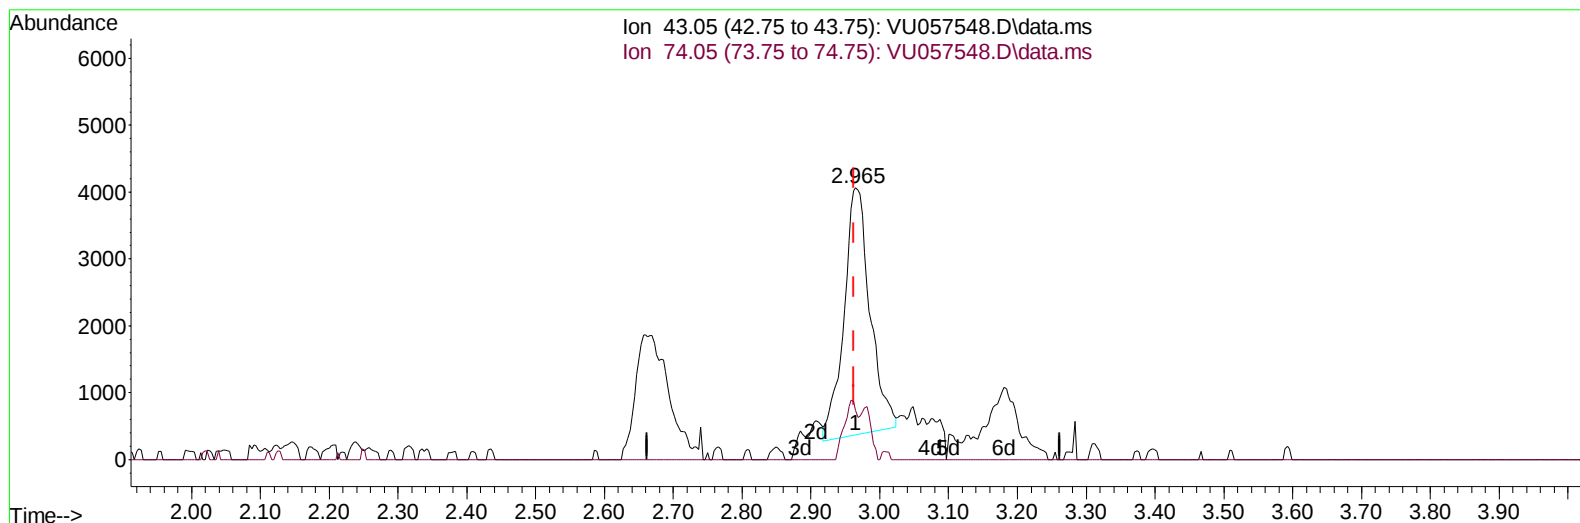

TIC: VU057548.D\data.ms

## (15) Methyl Acetate (T)

2.965min (+ 0.003) 1.37 ug/L

response 9733

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 74.05 | 23.20  | 11.85# |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU011724\  
 Data File : VU057548.D  
 Acq On : 17 Jan 2024 18:40  
 Operator : MD/SY  
 Sample : P1120-09 10X  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BGWH5

Manual IntegrationsAPPROVED

Quant Time: Jan 18 01:11:46 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR011124WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Jan 18 01:10:22 2024  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/18/2024  
 Supervised By :Mahesh Dadoda 01/18/2024

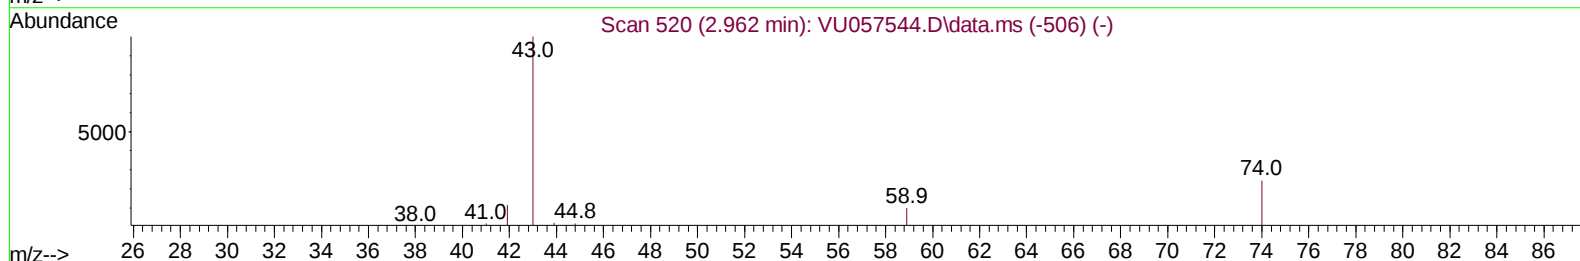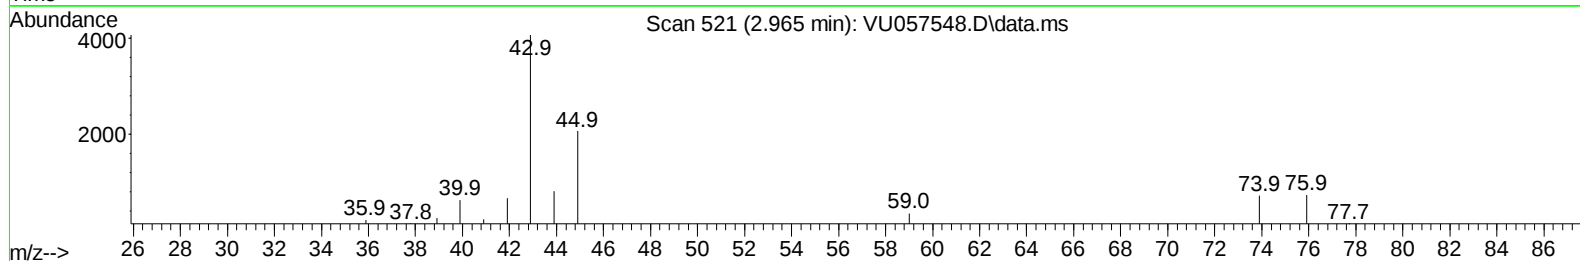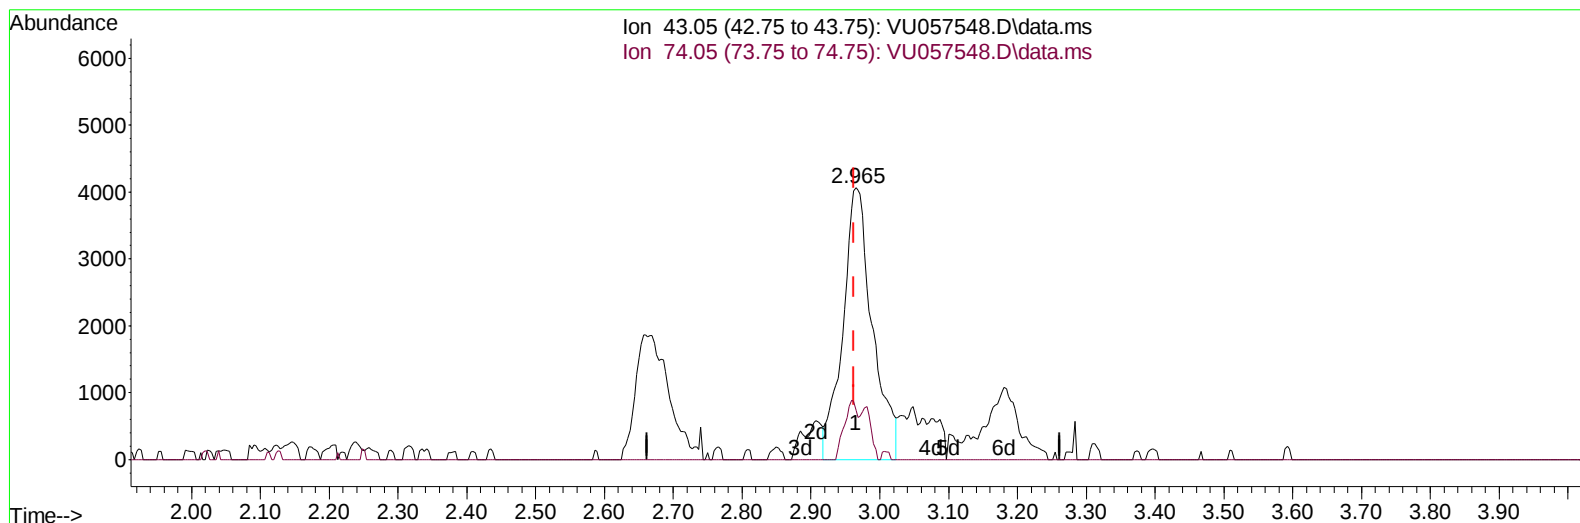

TIC: VU057548.D\data.ms

(15) Methyl Acetate (T)

2.965min (+ 0.003) 1.71 ug/L m

response 12130

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 74.05 | 23.20  | 9.51#  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU011724\  
 Data File : VU057548.D  
 Acq On : 17 Jan 2024 18:40  
 Operator : MD/SY  
 Sample : P1120-09 10X  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BGWH5

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/18/2024  
 Supervised By :Mahesh Dadoda 01/18/2024

Quant Time: Jan 18 01:11:46 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR011124WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Jan 18 01:10:22 2024  
 Response via : Initial Calibration

| Compound                      | R.T.   | Q     | Ion      | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|----------|
| -----                         |        |       |          |          |        |          |          |
| Internal Standards            |        |       |          |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 6.245  | 114   |          | 272183   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 9.412  | 117   |          | 283247   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.807 | 152   |          | 79828    | 5.000  | ug/L     | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.599  | 65    |          | 86761    | 3.142  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 62.800%  |          |
| 7) Chloroethane-d5            | 1.914  | 69    |          | 78416    | 3.649  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 73.000%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.563  | 65    |          | 42139    | 3.609  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 72.200%  |          |
| 20) 2-Butanone-d5             | 4.634  | 46    |          | 199123   | 38.121 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 76.240%  |          |
| 24) Chloroform-d              | 5.058  | 84    |          | 187242   | 3.924  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 78.400%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.695  | 65    |          | 105130   | 4.575  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 91.600%  |          |
| 32) Benzene-d6                | 5.721  | 84    |          | 357927   | 3.465  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 69.200%# |          |
| 36) 1,2-Dichloropropane-d6    | 6.682  | 67    |          | 136518   | 4.239  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 84.800%  |          |
| 41) Toluene-d8                | 7.894  | 98    |          | 255131   | 2.925  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 58.600%# |          |
| 43) trans-1,3-Dichloroprop... | 8.177  | 79    |          | 36097    | 3.224  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 64.400%  |          |
| 46) 2-Hexanone-d5             | 8.631  | 63    |          | 130775   | 32.254 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 64.500%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.749 | 84    |          | 95480    | 4.389  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 87.800%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.190 | 152   |          | 73968    | 4.614  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 92.200%  |          |
| Target Compounds              |        |       |          |          |        |          |          |
| 15) Methyl Acetate            | 2.965  | 43    |          | 12130m   | 1.709  | ug/L     |          |
| 22) cis-1,2-Dichloroethene    | 4.660  | 96    |          | 7324     | 0.399  | ug/L     | 96       |
| -----                         |        |       |          |          |        |          |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU011724\  
Data File : VU057548.D  
Acq On : 17 Jan 2024 18:40  
Operator : MD/SY  
Sample : P1120-09 10X  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BGWH5

## Manual IntegrationsAPPROVED

Quant Time: Jan 18 01:11:46 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR011124WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Jan 18 01:10:22 2024  
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/18/2024  
Supervised By :Mahesh Dadoda 01/18/2024

