


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011724\
Data File : VU057542.D
Acq On : 17 Jan 2024 12:34
Operator : MD/SY
Sample : BFB108
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB108

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 18 01:10:22 2024

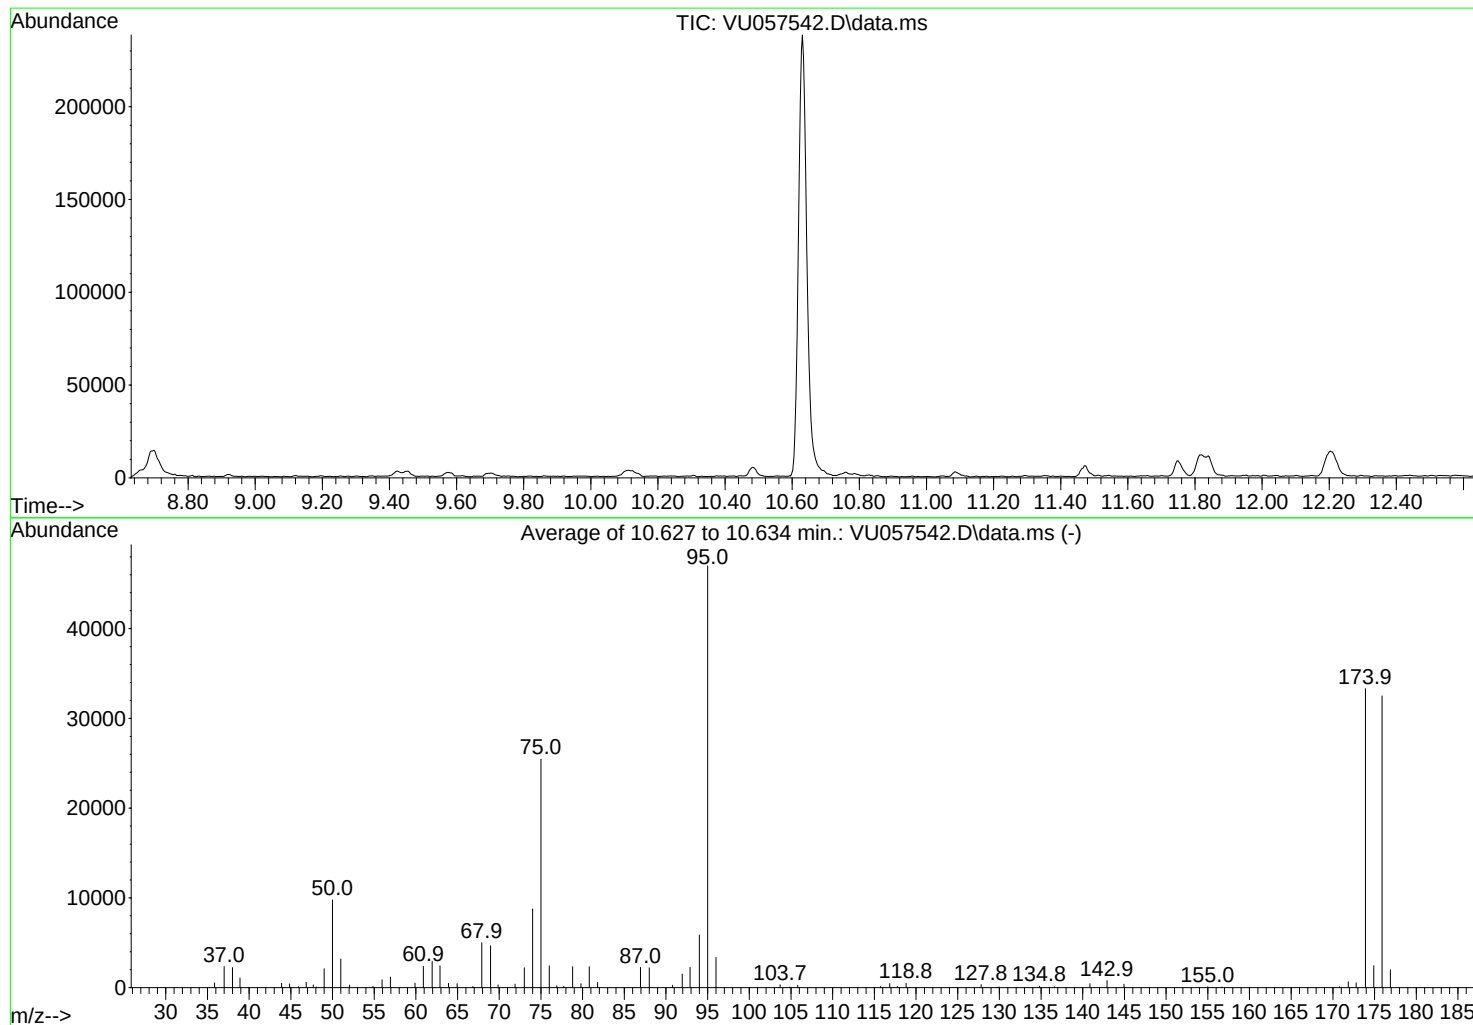

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.8	9764	PASS
75	95	30	80	54.2	25464	PASS
95	95	100	100	100.0	47000	PASS
96	95	5	9	7.2	3365	PASS
173	174	0.00	2	1.6	537	PASS
174	95	50	120	70.9	33315	PASS
175	174	5	9	7.3	2444	PASS
176	174	95	101	97.5	32496	PASS
177	176	5	9	6.1	1988	PASS

m/z	Abundance
39.70	338.0
43.90	498.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108

m/z	Abundance
35.80	556.0
37.00	2360.0
38.00	2292.0
38.90	1114.0
39.90	272.0
43.90	894.0
44.80	395.0
46.90	618.0
47.70	379.0
49.00	2057.0
50.00	9785.0
51.00	3141.0
52.10	233.0
54.80	162.0
55.90	753.0
56.90	1262.0
59.90	539.0
60.90	2638.0
62.00	3124.0
62.90	2466.0
63.90	566.0
65.00	432.0
66.90	158.0
67.90	4996.0
69.00	4412.0
69.90	337.0
71.90	389.0
73.00	2195.0
74.00	8634.0
75.00	25176.0
76.00	2375.0
76.80	233.0
78.80	2353.0
79.80	415.0
80.80	2295.0
81.80	512.0
86.90	2117.0
88.00	2309.0
90.80	248.0
91.90	1609.0
92.90	2177.0
94.00	5609.0
95.00	48088.0
96.00	3388.0
103.70	309.0
104.80	116.0
105.80	294.0
115.80	131.0
116.80	510.0
118.70	504.0
127.80	363.0
130.00	106.0
134.80	151.0
136.60	120.0
137.00	101.0
140.80	489.0
142.80	805.0
145.00	368.0
156.70	110.0
170.80	140.0
171.90	754.0
172.80	488.0
173.90	32056.0
174.90	2526.0
175.90	31656.0
176.90	2135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108

m/z	Abundance
35.80	531.0
37.00	2505.0
38.00	2293.0
38.90	1112.0
39.90	300.0
43.90	1027.0
44.80	433.0
45.90	102.0
46.80	610.0
47.70	301.0
49.00	2229.0
50.00	10168.0
51.00	3321.0
52.10	307.0
54.80	145.0
56.00	910.0
56.90	1187.0
59.90	472.0
60.90	2412.0
62.00	3016.0
62.90	2537.0
63.90	478.0
65.00	443.0
66.90	139.0
67.90	5106.0
68.90	4733.0
69.80	299.0
71.90	448.0
73.00	2246.0
74.00	9001.0
75.00	26184.0
76.00	2470.0
76.90	188.0
77.80	213.0
78.80	2418.0
79.80	447.0
80.80	2390.0
81.80	574.0
86.90	2383.0
88.00	2287.0
90.80	298.0
91.90	1494.0
92.90	2298.0
94.00	6063.0
95.00	48272.0
96.00	3522.0
103.70	324.0
105.80	295.0
115.70	148.0
116.80	451.0
117.80	164.0
118.80	478.0
127.80	369.0
129.90	103.0
134.80	176.0
136.60	144.0
140.90	465.0
142.90	807.0
144.90	403.0
155.00	128.0
156.70	122.0
170.80	131.0
171.90	658.0
172.80	577.0
173.90	34240.0
174.90	2449.0
175.90	33584.0
176.90	2004.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108

m/z	Abundance
35.90	504.0
37.00	2224.0
38.00	2088.0
38.90	986.0
39.90	346.0
43.90	1093.0
44.90	402.0
45.90	157.0
46.80	521.0
47.70	226.0
48.10	209.0
49.00	2025.0
50.00	9340.0
51.00	3098.0
52.00	319.0
54.90	167.0
56.00	981.0
57.00	1075.0
59.90	506.0
60.90	2092.0
61.90	2712.0
62.90	2317.0
63.90	382.0
64.90	489.0
66.80	153.0
67.90	4906.0
68.90	4838.0
69.80	264.0
71.90	361.0
73.00	2180.0
74.00	8696.0
75.00	25032.0
76.00	2445.0
77.00	218.0
77.70	239.0
78.80	2258.0
79.80	470.0
80.80	2308.0
81.80	624.0
87.00	2286.0
88.00	2018.0
90.80	280.0
92.00	1435.0
92.90	2320.0
94.00	5948.0
95.00	44640.0
96.00	3184.0
103.70	326.0
104.90	101.0
105.80	240.0
115.70	163.0
116.90	353.0
117.70	204.0
118.90	477.0
127.80	265.0
129.70	126.0
134.80	178.0
140.90	362.0
143.00	763.0
144.90	392.0
155.00	143.0
171.80	492.0
172.80	545.0
173.90	33648.0
174.90	2356.0
175.90	32248.0
176.90	1824.0

Instrument :
MSVOA_U
ClientSampleId :
BFB108