

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037202.D
 Acq On : 12 Mar 2020 20:24
 Operator : JC/MD
 Sample : L1901-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NC7

Quant Time: Mar 13 08:25:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 13 07:30:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	398887	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	385088	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	163949	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	141301	45.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.54%
7) Chloroethane-d5	1.93	69	117833	47.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.68%
11) 1,1-Dichloroethene-d2	2.59	63	197872	34.94	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.88%
21) 2-Butanone-d5	4.67	46	260220	106.51	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.51%
24) Chloroform-d	5.10	84	281452	47.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.84%
26) 1,2-Dichloroethane-d4	5.74	65	214812	49.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.88%
32) Benzene-d6	5.76	84	518140	48.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.76%
36) 1,2-Dichloropropane-d6	6.72	67	167594	48.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.60%
41) Toluene-d8	7.92	98	475134	46.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.78%
43) trans-1,3-Dichloropropene-	8.20	79	88065	46.63	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.26%
47) 2-Hexanone-d5	8.66	63	178841	99.55	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.55%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	254627	47.37	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.74%
64) 1,2-Dichlorobenzene-d4	12.21	152	175228	51.53	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.06%


Target Compounds					Ovalue
13) Acetone	2.66	43	3709	1.600 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031220\
Data File : VU037202.D
Acq On : 12 Mar 2020 20:24
Operator : JC/MD
Sample : L1901-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NC7

Quant Time: Mar 13 08:25:27 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 13 07:30:58 2020
Response via : Initial Calibration

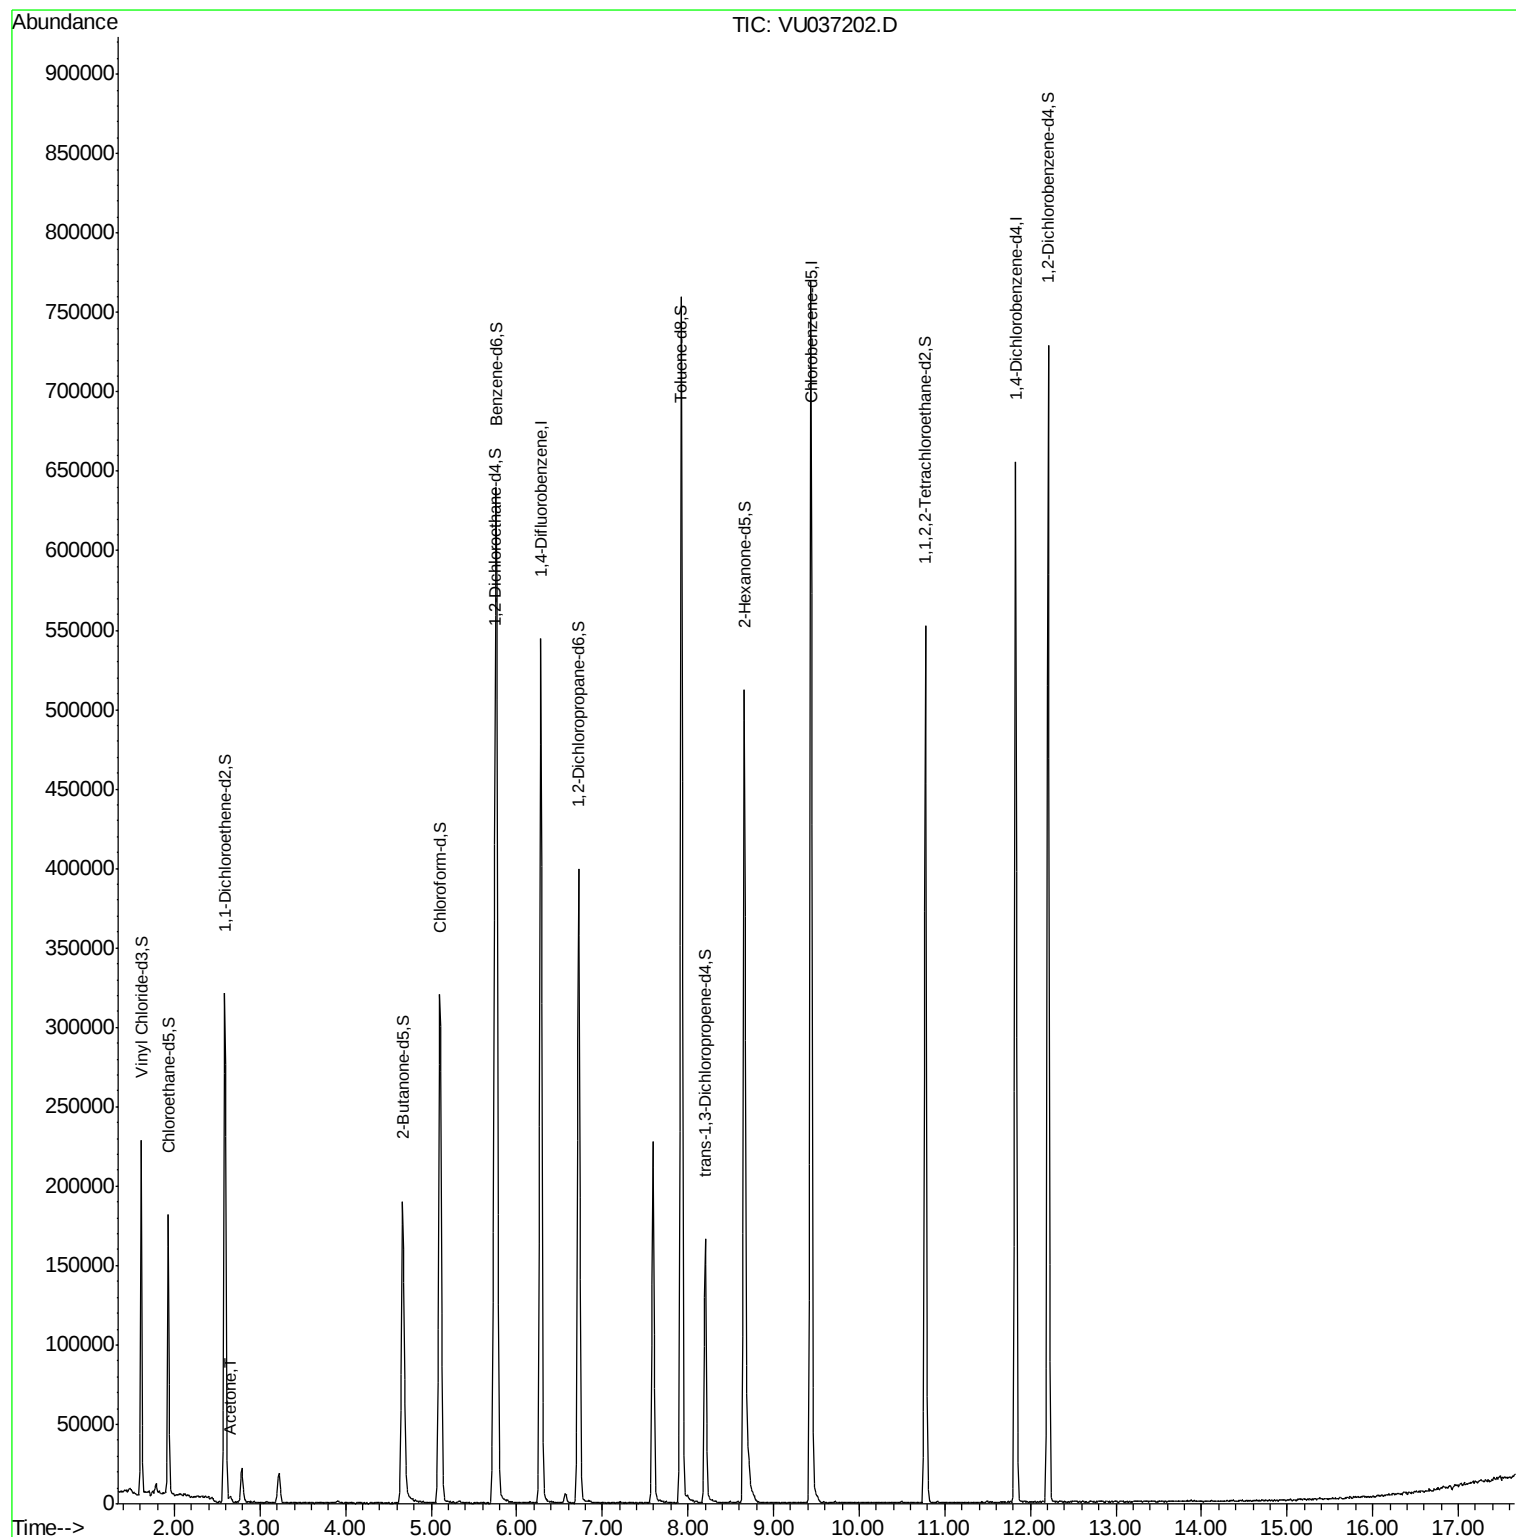

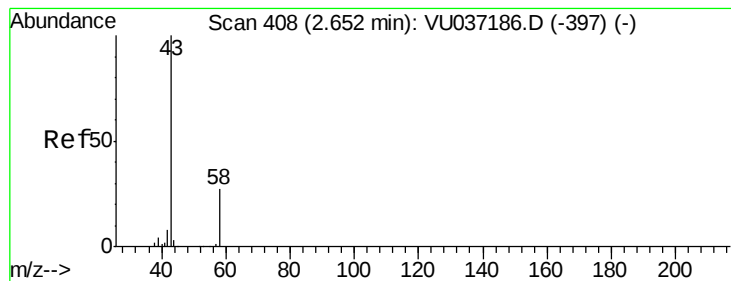

#13
 Acetone
 Concen: 1.600 ug/L
 RT: 2.66 min Scan# 409
 Delta R.T. 0.00 min
 Lab File: VU037202.D
 Acq: 12 Mar 2020 20:24

Instrument :
 MSVOA_U
 ClientSampleId :
 CONC7

Tot Ion: 43 Resp: 3709
 Ion Ratio Lower Upper
 43 100
 58 24.2 0.0 57.2

