

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037195.D
 Acq On : 12 Mar 2020 17:44
 Operator : JC/MD
 Sample : L1784-15DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B03DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	95	rBV	231694	244883	2.41%	1.029%
2	1.929	175	183	196	rVB	184228	238593	2.35%	1.002%
3	2.494	357	359	363	rVB2	644	375	0.00%	0.002%
4	2.591	376	389	406	rBV	349407	571031	5.63%	2.398%
5	2.723	425	430	435	rBV2	954	941	0.01%	0.004%
6	2.793	449	452	456	rVV2	535	525	0.01%	0.002%
7	2.887	478	481	486	rVB3	564	473	0.00%	0.002%
8	2.938	494	497	504	rVB4	536	579	0.01%	0.002%
9	3.073	532	539	553	rVV5	2609	4777	0.05%	0.020%
10	3.221	572	585	601	rVB2	6386	13998	0.14%	0.059%
11	3.356	622	627	630	rBV2	460	435	0.00%	0.002%
12	3.588	696	699	706	rVB2	450	388	0.00%	0.002%
13	3.668	717	724	730	rBV3	595	709	0.01%	0.003%
14	4.109	857	861	866	rVB3	451	410	0.00%	0.002%
15	4.269	903	911	914	rVB2	490	579	0.01%	0.002%
16	4.398	946	951	954	rBV2	381	424	0.00%	0.002%
17	4.668	1019	1035	1066	rBV	188122	454460	4.48%	1.909%
18	4.832	1082	1086	1091	rBV4	679	635	0.01%	0.003%
19	4.980	1128	1132	1139	rVB3	548	658	0.01%	0.003%
20	5.018	1139	1144	1148	rBV2	608	534	0.01%	0.002%
21	5.105	1153	1171	1195	rBV	325481	712173	7.02%	2.991%
22	5.247	1213	1215	1222	rVV4	565	607	0.01%	0.003%
23	5.350	1236	1247	1248	rBV6	5309	6518	0.06%	0.027%
24	5.414	1261	1267	1271	rBV3	804	1082	0.01%	0.005%
25	5.761	1353	1375	1405	rBV2	657643	1750060	17.26%	7.351%
26	5.916	1420	1423	1431	rVB4	864	947	0.01%	0.004%
27	6.067	1468	1470	1473	rVV	836	671	0.01%	0.003%
28	6.083	1473	1475	1481	rVB3	752	629	0.01%	0.003%
29	6.147	1489	1495	1496	rBV2	718	523	0.01%	0.002%
30	6.157	1496	1498	1501	rVB2	673	379	0.00%	0.002%
31	6.282	1521	1537	1564	rVV	556204	1050128	10.35%	4.411%
32	6.420	1577	1580	1584	rVB3	705	570	0.01%	0.002%
33	6.443	1584	1587	1592	rVB4	697	615	0.01%	0.003%
34	6.501	1600	1605	1607	rBV2	518	377	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037195.D
 Acq On : 12 Mar 2020 17:44
 Operator : JC/MD
 Sample : L1784-15DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B03DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

35	6.575	1610	1628	1660	rBV	5432375	10141993	100.00%	42.598%
36	6.723	1662	1674	1695	rVB	415903	826727	8.15%	3.472%
37	6.954	1742	1746	1748	rBV2	609	479	0.00%	0.002%
38	6.967	1748	1750	1755	rVV2	569	455	0.00%	0.002%
39	7.211	1819	1826	1835	rVB5	1121	1737	0.02%	0.007%
40	7.279	1841	1847	1851	rVV4	395	520	0.01%	0.002%
41	7.305	1851	1855	1859	rVB2	744	698	0.01%	0.003%
42	7.330	1859	1863	1866	rBV3	427	365	0.00%	0.002%
43	7.359	1866	1872	1876	rVB2	672	833	0.01%	0.003%
44	7.382	1876	1879	1883	rBV3	635	641	0.01%	0.003%
45	7.449	1896	1900	1904	rBV3	510	559	0.01%	0.002%
46	7.488	1907	1912	1915	rBV2	542	395	0.00%	0.002%
47	7.591	1931	1944	1967	rBV	239783	421438	4.16%	1.770%
48	7.710	1978	1981	1983	rBV	750	577	0.01%	0.002%
49	7.813	2010	2013	2014	rBV	614	380	0.00%	0.002%
50	7.822	2014	2016	2025	rVB2	1973	2044	0.02%	0.009%
51	7.864	2025	2029	2031	rBV	653	494	0.00%	0.002%
52	7.922	2033	2047	2064	rBV	797882	1375391	13.56%	5.777%
53	8.051	2083	2087	2090	rBV4	908	511	0.01%	0.002%
54	8.205	2122	2135	2151	rBV	174759	298542	2.94%	1.254%
55	8.276	2155	2157	2161	rVB2	870	546	0.01%	0.002%
56	8.340	2174	2177	2182	rVB3	531	388	0.00%	0.002%
57	8.427	2197	2204	2210	rVB5	1780	2642	0.03%	0.011%
58	8.459	2210	2214	2220	rVB4	543	590	0.01%	0.002%
59	8.510	2220	2230	2234	rBV3	2128	3063	0.03%	0.013%
60	8.568	2245	2248	2250	rBV3	1339	818	0.01%	0.003%
61	8.658	2261	2276	2323	rBV	558589	1049005	10.34%	4.406%
62	8.841	2331	2333	2342	rVB3	702	563	0.01%	0.002%
63	8.970	2371	2373	2380	rVB4	703	594	0.01%	0.002%
64	9.018	2384	2388	2390	rBV3	627	479	0.00%	0.002%
65	9.089	2407	2410	2415	rVB	616	542	0.01%	0.002%
66	9.231	2451	2454	2458	rBV	617	588	0.01%	0.002%
67	9.436	2504	2518	2545	rBV	787620	1319689	13.01%	5.543%
68	9.591	2560	2566	2570	rVB4	1184	1066	0.01%	0.004%
69	9.613	2570	2573	2577	rBV3	895	811	0.01%	0.003%
70	9.710	2597	2603	2605	rBV3	989	948	0.01%	0.004%
71	9.780	2621	2625	2626	rVV2	640	481	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037195.D
 Acq On : 12 Mar 2020 17:44
 Operator : JC/MD
 Sample : L1784-15DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B03DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

72	9.793	2627	2629	2633	rVB2	495	368	0.00%	0.002%
73	10.118	2725	2730	2731	rBV2	720	513	0.01%	0.002%
74	10.176	2743	2748	2751	rBV	504	427	0.00%	0.002%
75	10.214	2757	2760	2765	rBV	489	389	0.00%	0.002%
76	10.436	2821	2829	2831	rBV2	282	405	0.00%	0.002%
77	10.501	2844	2849	2855	rBV4	841	948	0.01%	0.004%
78	10.642	2890	2893	2898	rBV3	489	547	0.01%	0.002%
79	10.774	2921	2934	2953	rBV	555817	899837	8.87%	3.779%
80	10.957	2985	2991	2994	rBV2	409	372	0.00%	0.002%
81	11.063	3020	3024	3029	rVB2	640	461	0.00%	0.002%
82	11.089	3029	3032	3034	rBV2	604	416	0.00%	0.002%
83	11.333	3103	3108	3110	rBV	505	437	0.00%	0.002%
84	11.484	3153	3155	3163	rVB5	686	577	0.01%	0.002%
85	11.761	3236	3241	3244	rBV3	1344	1481	0.01%	0.006%
86	11.829	3249	3262	3278	rVV	693878	1137650	11.22%	4.778%
87	11.928	3290	3293	3296	rBV2	611	413	0.00%	0.002%
88	12.038	3322	3327	3332	rBV3	572	693	0.01%	0.003%
89	12.208	3367	3380	3395	rBV	756497	1236801	12.19%	5.195%
90	12.452	3451	3456	3458	rBV3	714	651	0.01%	0.003%
91	12.668	3519	3523	3527	rBV3	849	712	0.01%	0.003%
92	12.867	3581	3585	3593	rBV2	834	963	0.01%	0.004%
93	12.906	3594	3597	3604	rVB3	850	621	0.01%	0.003%
94	12.983	3617	3621	3625	rBV3	579	572	0.01%	0.002%
95	13.121	3661	3664	3667	rBV	707	472	0.00%	0.002%
96	13.446	3762	3765	3769	rBV2	617	387	0.00%	0.002%
97	13.600	3811	3813	3819	rVB2	548	466	0.00%	0.002%
98	14.121	3972	3975	3979	rVB2	1550	1023	0.01%	0.004%
99	14.536	4098	4104	4108	rBV5	1059	1212	0.01%	0.005%
100	14.726	4160	4163	4164	rBV2	678	419	0.00%	0.002%


Sum of corrected areas: 23808511

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031220\
Data File : VU037195.D
Acq On : 12 Mar 2020 17:44
Operator : JC/MD
Sample : L1784-15DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B03DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

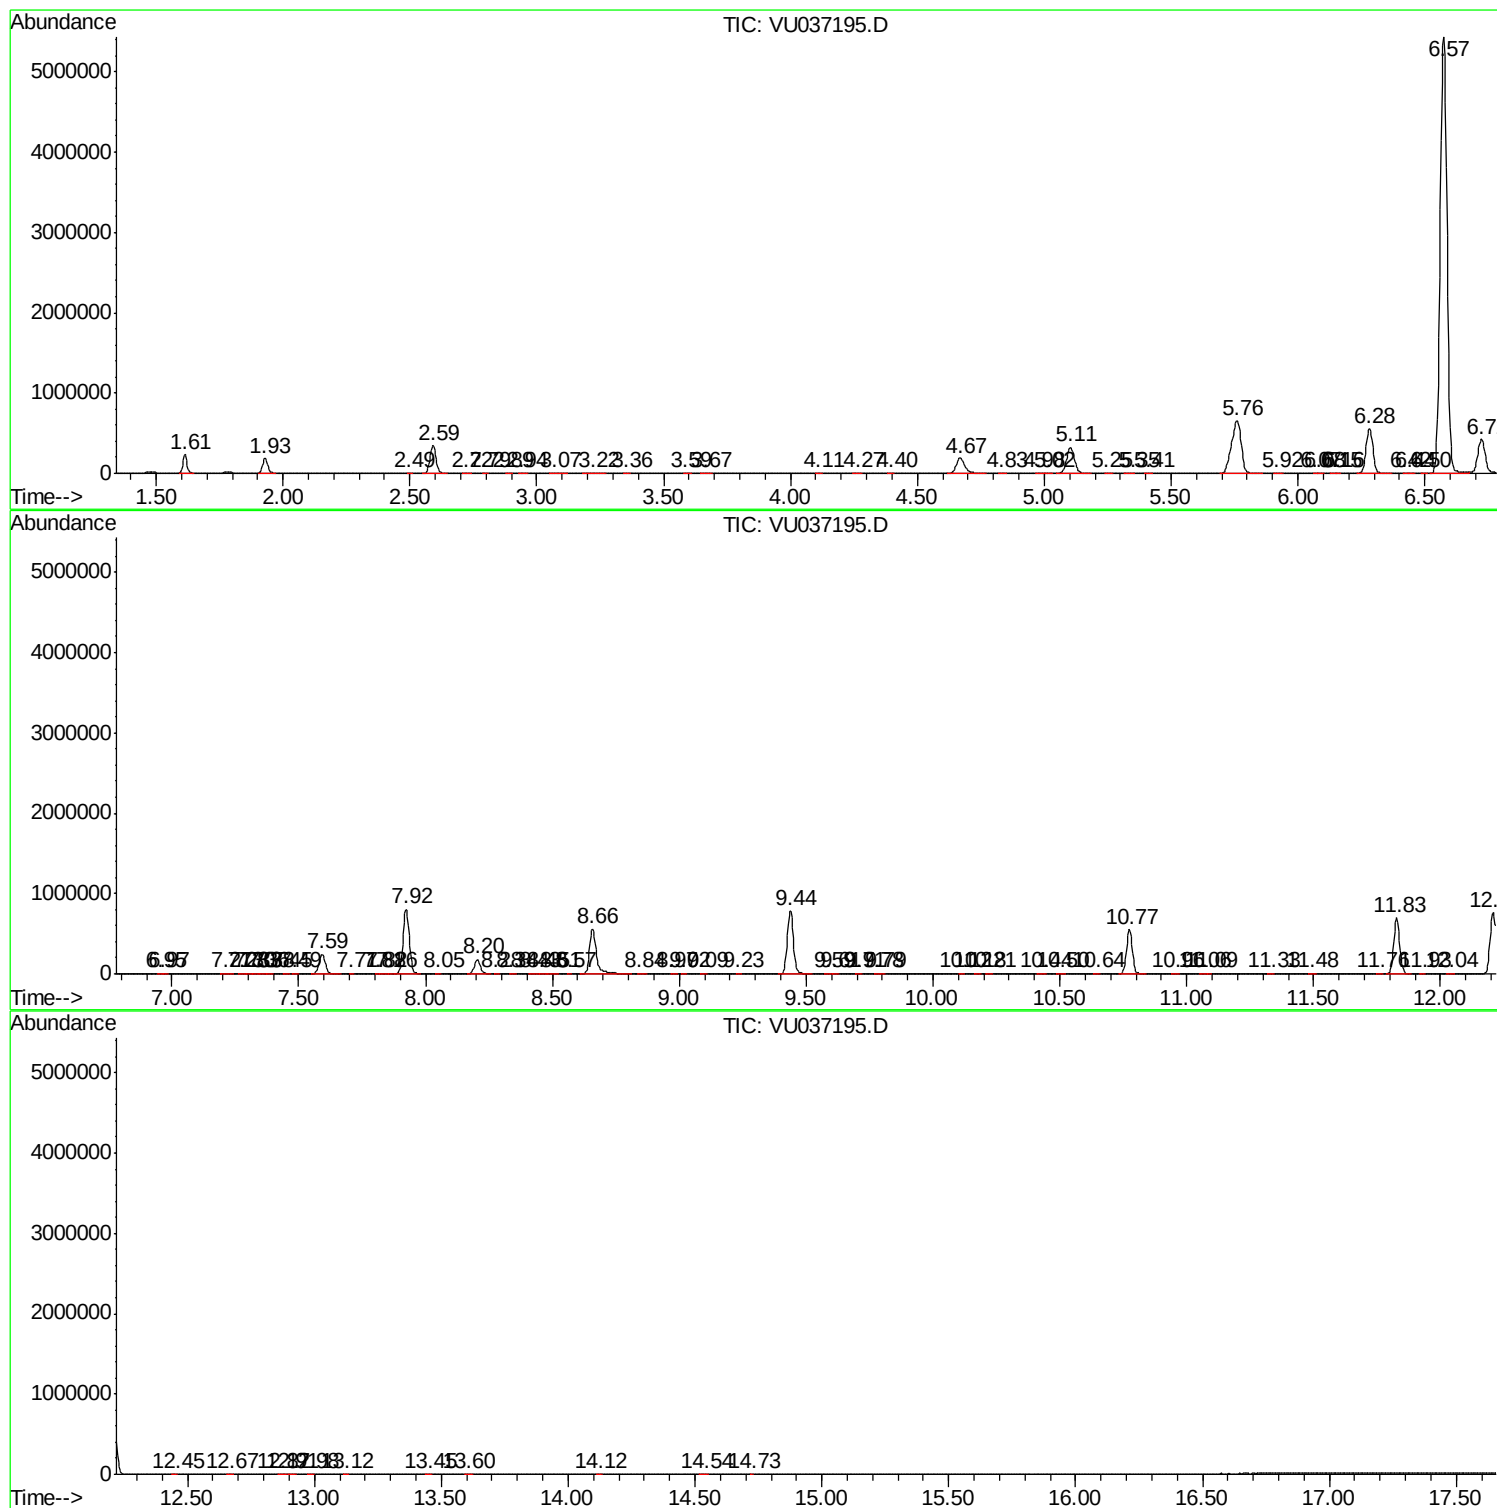

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031220\
Data File : VU037195.D
Acq On : 12 Mar 2020 17:44
Operator : JC/MD
Sample : L1784-15DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B03DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU031220\
Data File : VU037195.D
Acq On : 12 Mar 2020 17:44
Operator : JC/MD
Sample : L1784-15DL 100X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0B03DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc