

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037201.D
 Acq On : 12 Mar 2020 20:01
 Operator : JC/MD
 Sample : L1901-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	98	rVB	217552	231935	14.01%	1.686%
2	1.928	176	183	197	rVB	177203	228137	13.78%	1.658%
3	2.530	366	370	373	rBV	592	563	0.03%	0.004%
4	2.591	376	389	404	rBV2	328069	564005	34.07%	4.099%
5	2.787	440	450	463	rBV	15485	28767	1.74%	0.209%
6	3.153	559	564	565	rBV2	352	272	0.02%	0.002%
7	3.176	569	571	572	rBV	421	136	0.01%	0.001%
8	3.214	574	583	585	rBV2	10499	12740	0.77%	0.093%
9	3.288	604	606	608	rVB	225	92	0.01%	0.001%
10	3.304	608	611	615	rBV2	383	397	0.02%	0.003%
11	3.378	632	634	637	rVB2	322	170	0.01%	0.001%
12	3.446	653	655	658	rVB	359	178	0.01%	0.001%
13	3.459	658	659	661	rBV	285	139	0.01%	0.001%
14	3.645	713	717	720	rBV2	277	211	0.01%	0.002%
15	3.661	720	722	724	rBV	218	130	0.01%	0.001%
16	3.758	748	752	754	rBV	465	365	0.02%	0.003%
17	3.845	776	779	782	rBV2	210	113	0.01%	0.001%
18	3.867	782	786	788	rBV3	356	271	0.02%	0.002%
19	4.073	848	850	852	rVB	198	100	0.01%	0.001%
20	4.092	852	856	858	rBV2	302	243	0.01%	0.002%
21	4.105	858	860	863	rVB2	433	230	0.01%	0.002%
22	4.137	863	870	872	rBV2	240	272	0.02%	0.002%
23	4.176	879	882	885	rVB	280	146	0.01%	0.001%
24	4.282	913	915	918	rVB2	283	121	0.01%	0.001%
25	4.304	918	922	925	rBV	446	398	0.02%	0.003%
26	4.324	926	928	932	rVB2	686	376	0.02%	0.003%
27	4.349	932	936	937	rBV	273	183	0.01%	0.001%
28	4.446	962	966	970	rBV	294	284	0.02%	0.002%
29	4.465	970	972	973	rVV	253	105	0.01%	0.001%
30	4.475	973	975	977	rVB	141	68	0.00%	0.000%
31	4.520	986	989	993	rVB	495	404	0.02%	0.003%
32	4.549	993	998	1003	rBV2	454	478	0.03%	0.003%
33	4.603	1011	1015	1016	rBV	246	151	0.01%	0.001%
34	4.668	1019	1035	1066	rVV	179751	476928	28.81%	3.466%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037201.D
 Acq On : 12 Mar 2020 20:01
 Operator : JC/MD
 Sample : L1901-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

35	5.041	1148	1151	1153	rBV2	308	171	0.01%	0.001%
36	5.102	1153	1170	1194	rVV	314851	683075	41.27%	4.964%
37	5.195	1194	1199	1202	rBV2	599	594	0.04%	0.004%
38	5.272	1219	1223	1227	rBV3	685	682	0.04%	0.005%
39	5.443	1274	1276	1279	rVB2	202	86	0.01%	0.001%
40	5.533	1301	1304	1307	rBV2	278	221	0.01%	0.002%
41	5.600	1322	1325	1328	rBV2	236	108	0.01%	0.001%
42	5.658	1340	1343	1347	rBV2	350	251	0.02%	0.002%
43	5.761	1352	1375	1397	rBV2	618121	1655331	100.00%	12.030%
44	6.060	1465	1468	1469	rBV2	631	392	0.02%	0.003%
45	6.192	1506	1509	1510	rBV2	419	241	0.01%	0.002%
46	6.282	1521	1537	1552	rBV	538509	1009566	60.99%	7.337%
47	6.427	1578	1582	1588	rBV3	806	809	0.05%	0.006%
48	6.571	1613	1627	1648	rBV	356867	669346	40.44%	4.864%
49	6.722	1660	1674	1693	rBV	398071	772023	46.64%	5.611%
50	6.941	1740	1742	1747	rVB3	402	213	0.01%	0.002%
51	7.073	1778	1783	1785	rBV2	517	423	0.03%	0.003%
52	7.205	1820	1824	1834	rVB4	1515	1514	0.09%	0.011%
53	7.272	1843	1845	1848	rVB2	497	246	0.01%	0.002%
54	7.330	1862	1863	1866	rVB	284	140	0.01%	0.001%
55	7.391	1879	1882	1884	rVB2	484	238	0.01%	0.002%
56	7.404	1884	1886	1889	rBV2	269	169	0.01%	0.001%
57	7.427	1889	1893	1898	rVB	500	429	0.03%	0.003%
58	7.455	1898	1902	1905	rBV	401	339	0.02%	0.002%
59	7.533	1924	1926	1928	rBV	410	235	0.01%	0.002%
60	7.594	1931	1945	1961	rBV	227602	400851	24.22%	2.913%
61	7.922	2033	2047	2064	rBV	762609	1313772	79.37%	9.548%
62	8.150	2116	2118	2119	rBV	250	112	0.01%	0.001%
63	8.205	2121	2135	2149	rBV	163447	276385	16.70%	2.009%
64	8.336	2175	2176	2178	rVB	342	79	0.00%	0.001%
65	8.417	2199	2201	2203	rVB	399	143	0.01%	0.001%
66	8.488	2217	2223	2224	rBV2	1023	875	0.05%	0.006%
67	8.552	2242	2243	2247	rBV	429	271	0.02%	0.002%
68	8.578	2247	2251	2253	rVB3	760	514	0.03%	0.004%
69	8.658	2262	2276	2321	rBV	507388	985383	59.53%	7.161%
70	8.928	2357	2360	2363	rBV2	738	508	0.03%	0.004%
71	8.983	2373	2377	2381	rBV2	501	522	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037201.D
 Acq On : 12 Mar 2020 20:01
 Operator : JC/MD
 Sample : L1901-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

72	9.070	2402	2404	2406	rBV	375	192	0.01%	0.001%
73	9.227	2446	2453	2455	rBV3	602	730	0.04%	0.005%
74	9.275	2465	2468	2470	rVB2	346	184	0.01%	0.001%
75	9.327	2481	2484	2488	rBV	352	252	0.02%	0.002%
76	9.346	2488	2490	2491	rBV	187	69	0.00%	0.001%
77	9.378	2497	2500	2504	rBV2	561	472	0.03%	0.003%
78	9.436	2505	2518	2538	rBV	762133	1270360	76.74%	9.232%
79	9.584	2561	2564	2571	rBV4	608	724	0.04%	0.005%
80	9.677	2591	2593	2595	rBV2	304	167	0.01%	0.001%
81	10.005	2689	2695	2697	rBV	331	332	0.02%	0.002%
82	10.127	2727	2733	2737	rBV4	648	613	0.04%	0.004%
83	10.266	2773	2776	2779	rBV2	242	153	0.01%	0.001%
84	10.388	2812	2814	2817	rBV2	264	124	0.01%	0.001%
85	10.587	2873	2876	2881	rVB2	420	291	0.02%	0.002%
86	10.774	2921	2934	2953	rVB	538704	876578	52.95%	6.370%
87	10.877	2963	2966	2968	rBV2	562	430	0.03%	0.003%
88	11.230	3073	3076	3078	rBV2	489	309	0.02%	0.002%
89	11.828	3249	3262	3278	rBV	663097	1097488	66.30%	7.976%
90	12.208	3367	3380	3394	rBV	724972	1185248	71.60%	8.614%


Sum of corrected areas: 13760081

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031220\
Data File : VU037201.D
Acq On : 12 Mar 2020 20:01
Operator : JC/MD
Sample : L1901-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

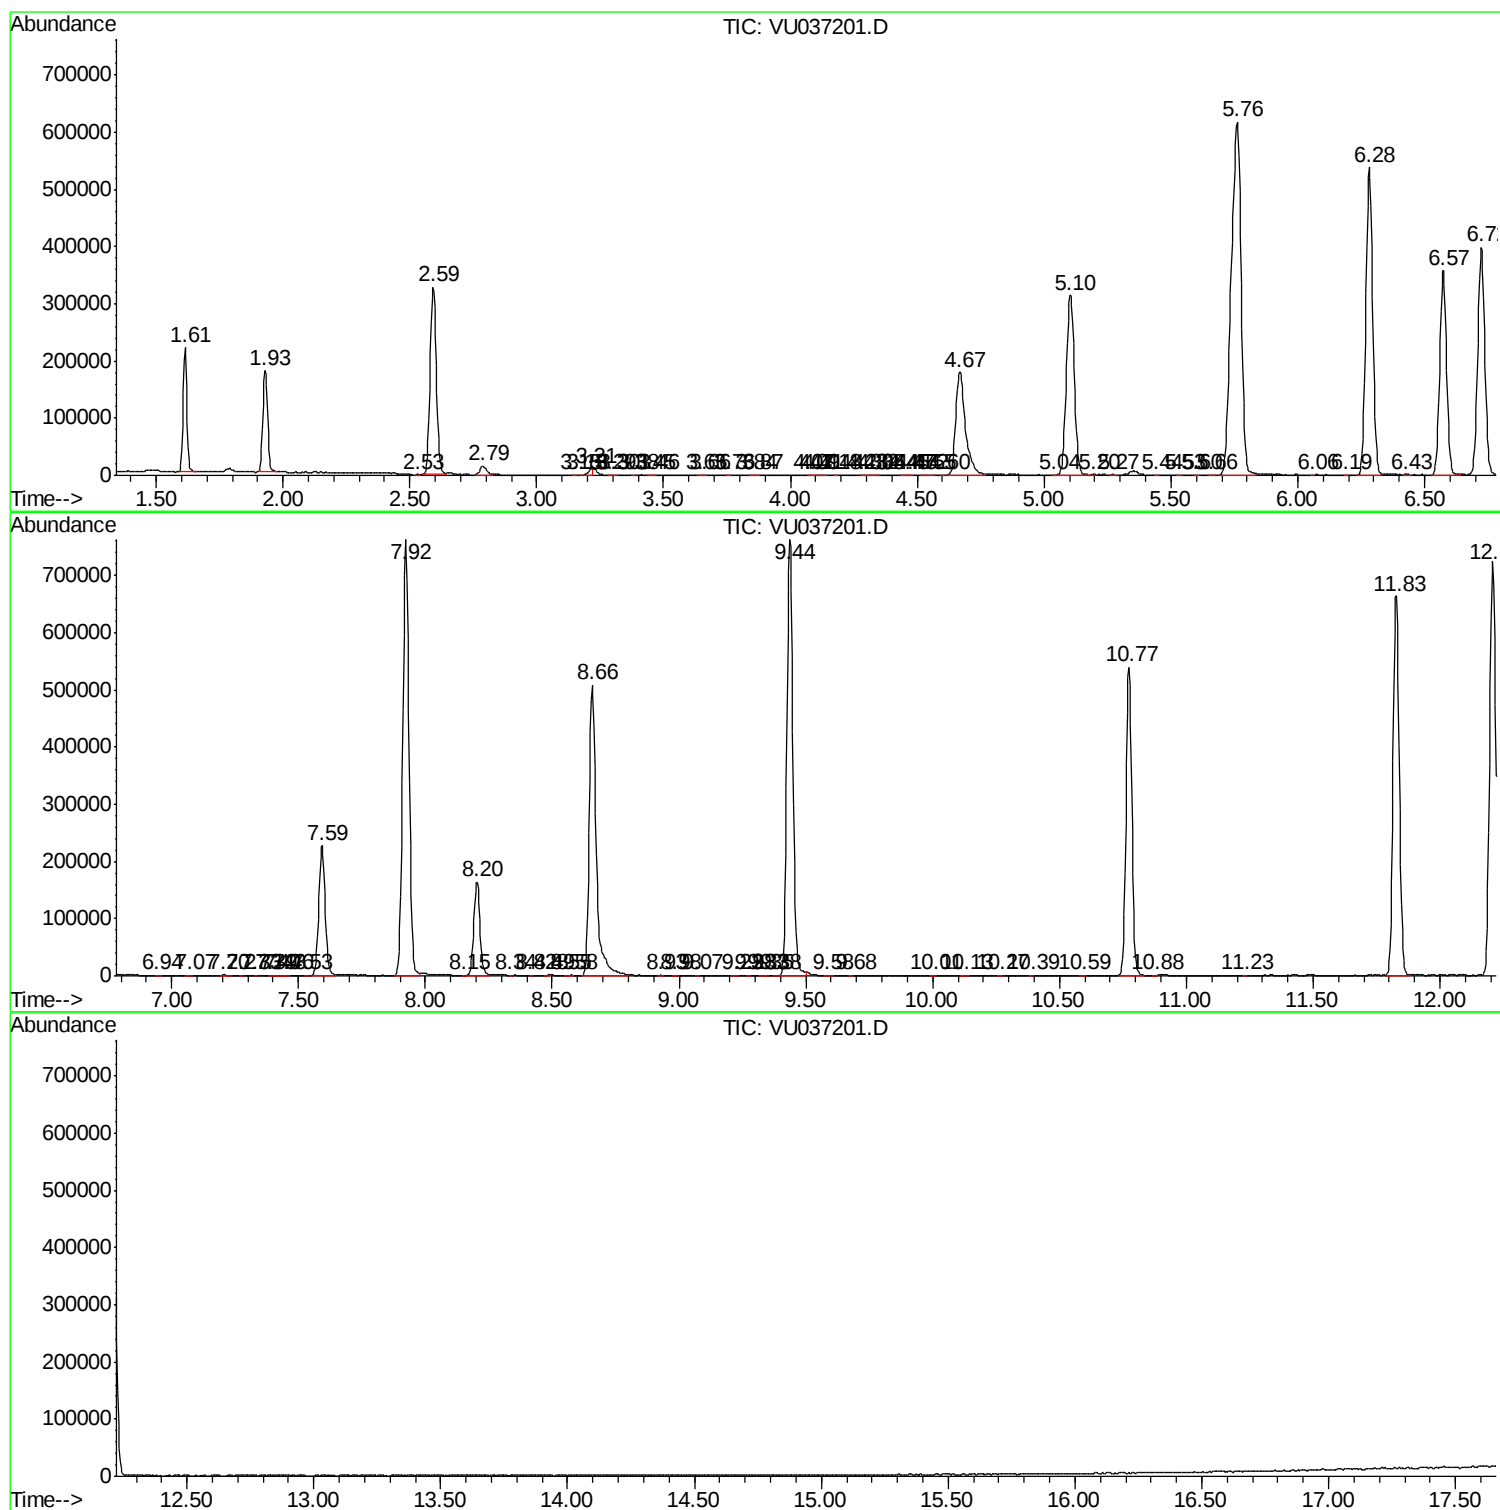

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031220\
Data File : VU037201.D
Acq On : 12 Mar 2020 20:01
Operator : JC/MD
Sample : L1901-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NC6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031220\
Data File : VU037201.D
Acq On : 12 Mar 2020 20:01
Operator : JC/MD
Sample : L1901-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NC6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc