

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037205.D
 Acq On : 12 Mar 2020 21:56
 Operator : JC/MD
 Sample : VU0312WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	94	rBV	230089	244615	14.02%	1.829%
2	1.932	176	184	195	rVB	186464	238634	13.68%	1.784%
3	2.591	377	389	405	rBV	343025	554802	31.80%	4.147%
4	2.887	479	481	486	rBV	466	340	0.02%	0.003%
5	2.957	500	503	505	rBV	529	333	0.02%	0.002%
6	2.990	511	513	514	rBV2	317	152	0.01%	0.001%
7	3.076	534	540	548	rBV7	1199	1870	0.11%	0.014%
8	3.128	555	556	557	rBV	322	80	0.00%	0.001%
9	3.221	574	585	599	rVB3	7210	16297	0.93%	0.122%
10	3.308	609	612	615	rBV2	223	161	0.01%	0.001%
11	3.475	661	664	668	rVB2	512	410	0.02%	0.003%
12	3.498	668	671	673	rBV	273	198	0.01%	0.001%
13	3.575	692	695	697	rBV2	290	180	0.01%	0.001%
14	3.601	701	703	705	rBV2	226	146	0.01%	0.001%
15	3.629	710	712	713	rBV2	186	47	0.00%	0.000%
16	3.761	747	753	756	rBV2	374	355	0.02%	0.003%
17	3.832	771	775	777	rBV	379	299	0.02%	0.002%
18	3.877	787	789	792	rBV	271	181	0.01%	0.001%
19	3.906	795	798	800	rBV	310	215	0.01%	0.002%
20	4.080	847	852	855	rBV2	553	517	0.03%	0.004%
21	4.138	867	870	871	rBV	272	146	0.01%	0.001%
22	4.263	906	909	913	rVB2	352	294	0.02%	0.002%
23	4.285	913	916	917	rBV2	175	102	0.01%	0.001%
24	4.337	929	932	933	rBV	207	141	0.01%	0.001%
25	4.346	933	935	938	rVV	351	226	0.01%	0.002%
26	4.417	956	957	959	rBV2	170	48	0.00%	0.000%
27	4.449	965	967	970	rBV2	435	292	0.02%	0.002%
28	4.575	1004	1006	1007	rBV	161	52	0.00%	0.000%
29	4.668	1019	1035	1064	rBV	188034	449141	25.75%	3.357%
30	5.105	1153	1171	1198	rBV	319274	709986	40.70%	5.307%
31	5.366	1250	1252	1257	rVB2	449	338	0.02%	0.003%
32	5.433	1270	1273	1276	rBV3	447	255	0.01%	0.002%
33	5.472	1283	1285	1288	rVB3	434	225	0.01%	0.002%
34	5.514	1296	1298	1304	rVB2	480	352	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037205.D
 Acq On : 12 Mar 2020 21:56
 Operator : JC/MD
 Sample : VU0312WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

35	5.555	1309	1311	1318	rVB2	608	595	0.03%	0.004%
36	5.591	1318	1322	1327	rBV2	466	425	0.02%	0.003%
37	5.617	1327	1330	1332	rVB2	291	171	0.01%	0.001%
38	5.633	1333	1335	1338	rBV	296	127	0.01%	0.001%
39	5.652	1338	1341	1344	rBV2	332	195	0.01%	0.001%
40	5.761	1352	1375	1402	rBV2	654487	1744566	100.00%	13.041%
41	6.282	1520	1537	1567	rBV2	538438	1010887	57.94%	7.557%
42	6.401	1572	1574	1577	rBV2	1004	577	0.03%	0.004%
43	6.491	1600	1602	1606	rBV2	392	184	0.01%	0.001%
44	6.571	1615	1627	1637	rVB2	5796	12030	0.69%	0.090%
45	6.639	1645	1648	1653	rVB2	567	430	0.02%	0.003%
46	6.665	1653	1656	1658	rBV	279	142	0.01%	0.001%
47	6.723	1659	1674	1697	rBV	413708	802344	45.99%	5.998%
48	6.825	1704	1706	1707	rBV	902	377	0.02%	0.003%
49	6.957	1744	1747	1749	rBV	410	244	0.01%	0.002%
50	7.083	1781	1786	1787	rBV	320	269	0.02%	0.002%
51	7.115	1793	1796	1799	rVB2	290	178	0.01%	0.001%
52	7.137	1800	1803	1805	rVB2	428	246	0.01%	0.002%
53	7.153	1805	1808	1811	rVB2	512	312	0.02%	0.002%
54	7.170	1811	1813	1818	rVB2	283	207	0.01%	0.002%
55	7.195	1818	1821	1822	rBV	641	377	0.02%	0.003%
56	7.295	1850	1852	1855	rVB2	359	190	0.01%	0.001%
57	7.334	1861	1864	1867	rBV	207	162	0.01%	0.001%
58	7.372	1871	1876	1880	rVV4	455	432	0.02%	0.003%
59	7.481	1908	1910	1913	rVB	473	175	0.01%	0.001%
60	7.497	1913	1915	1917	rBV	131	42	0.00%	0.000%
61	7.510	1917	1919	1920	rBV	167	88	0.01%	0.001%
62	7.533	1924	1926	1929	rBV	231	120	0.01%	0.001%
63	7.591	1929	1944	1965	rBV	231080	413659	23.71%	3.092%
64	7.822	2008	2016	2023	rVB6	2088	3343	0.19%	0.025%
65	7.854	2023	2026	2029	rVB2	593	342	0.02%	0.003%
66	7.870	2029	2031	2033	rBV	237	138	0.01%	0.001%
67	7.922	2033	2047	2067	rBV	799409	1378434	79.01%	10.304%
68	8.202	2120	2134	2155	rBV	171736	297589	17.06%	2.225%
69	8.369	2184	2186	2188	rVB	540	115	0.01%	0.001%
70	8.411	2196	2199	2202	rBV3	457	345	0.02%	0.003%
71	8.427	2202	2204	2205	rBV	297	128	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031220\
 Data File : VU037205.D
 Acq On : 12 Mar 2020 21:56
 Operator : JC/MD
 Sample : VU0312WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis

72	8.658	2262	2276	2320	rBV	538381	1024518	58.73%	7.659%
73	8.954	2359	2368	2376	rBV5	1626	2486	0.14%	0.019%
74	9.005	2382	2384	2386	rBV	325	158	0.01%	0.001%
75	9.031	2389	2392	2397	rVB2	468	403	0.02%	0.003%
76	9.060	2397	2401	2404	rBV3	538	412	0.02%	0.003%
77	9.436	2505	2518	2558	rVB	757601	1264140	72.46%	9.450%
78	9.706	2598	2602	2604	rBV	1109	994	0.06%	0.007%
79	9.758	2616	2618	2621	rVB	298	145	0.01%	0.001%
80	9.931	2670	2672	2674	rBV2	433	190	0.01%	0.001%
81	10.263	2772	2775	2778	rVB	536	297	0.02%	0.002%
82	10.314	2789	2791	2792	rBV	178	80	0.00%	0.001%
83	10.330	2793	2796	2799	rBV2	311	241	0.01%	0.002%
84	10.485	2841	2844	2845	rBV	325	202	0.01%	0.002%
85	10.774	2921	2934	2950	rBV	560167	903196	51.77%	6.752%
86	11.134	3043	3046	3049	rBV	565	391	0.02%	0.003%
87	11.742	3233	3235	3236	rBV2	951	405	0.02%	0.003%
88	11.829	3249	3262	3284	rVB	643771	1070631	61.37%	8.003%
89	12.208	3367	3380	3397	rBV	746642	1212339	69.49%	9.063%
90	13.237	3696	3700	3709	rVB5	3465	4464	0.26%	0.033%


Sum of corrected areas: 13377307

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031220\
Data File : VU037205.D
Acq On : 12 Mar 2020 21:56
Operator : JC/MD
Sample : VU0312WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

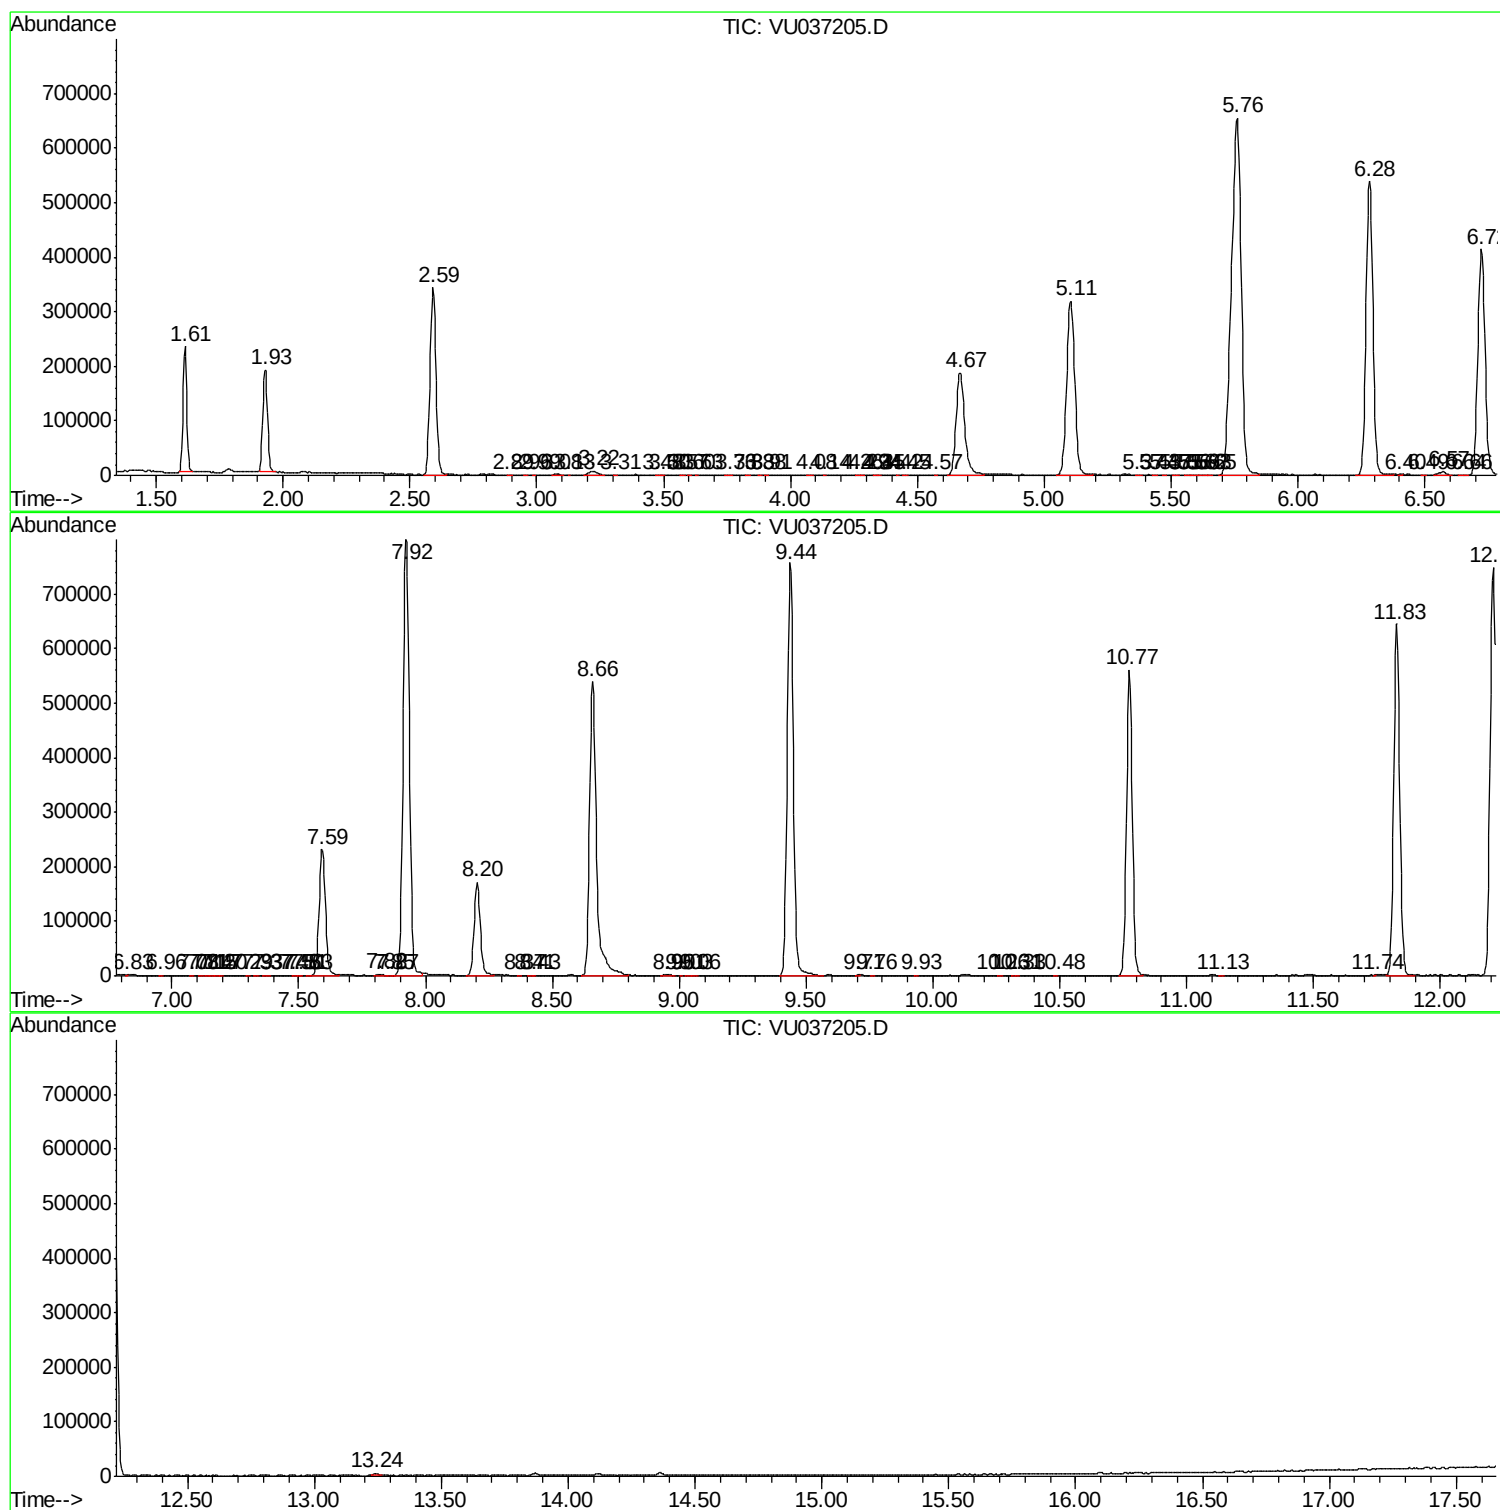

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031220\
Data File : VU037205.D
Acq On : 12 Mar 2020 21:56
Operator : JC/MD
Sample : VU0312WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031220\
Data File : VU037205.D
Acq On : 12 Mar 2020 21:56
Operator : JC/MD
Sample : VU0312WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc