


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031220\
 Data File : VU037183.D
 Acq On : 12 Mar 2020 12:05
 Operator : JC/MD
 Sample : BFB60
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031220WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 13 23:05:23 2020

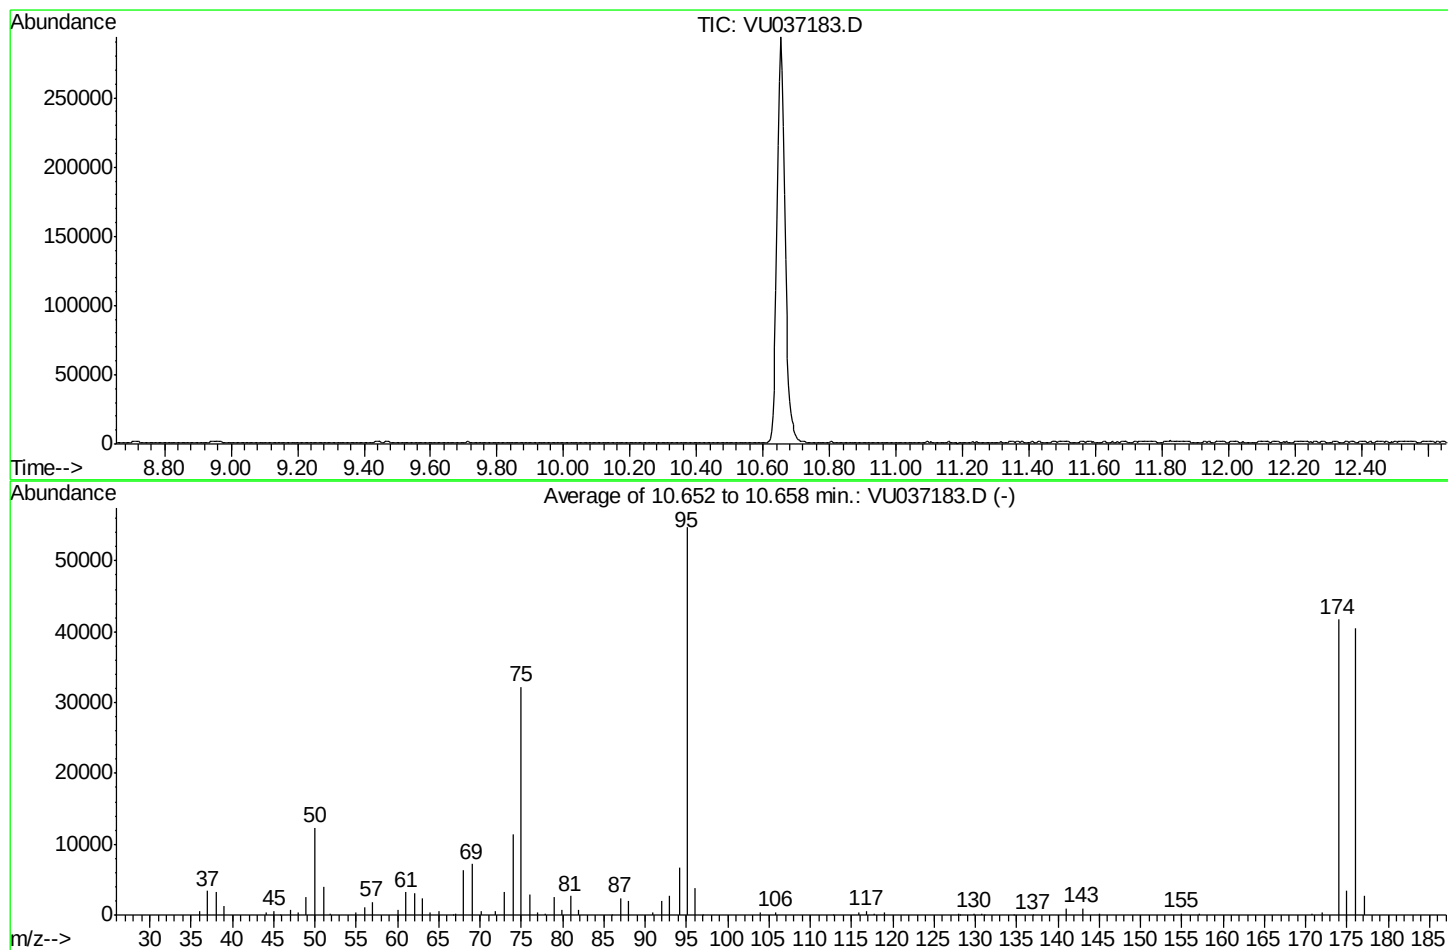

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	12357	PASS
75	95	30	80	58.9	32226	PASS
95	95	100	100	100.0	54738	PASS
96	95	5	9	7.0	3858	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.1	41674	PASS
175	174	5	9	8.4	3504	PASS
176	174	95	101	97.4	40573	PASS
177	176	5	9	6.6	2674	PASS

m/z	Abundance
36.00	585.0
37.00	3529.0
38.10	3328.0
39.00	1244.0
39.90	216.0
43.80	796.0
45.00	601.0
45.90	109.0
47.10	636.0
47.90	394.0
49.00	2508.0
50.00	12772.0
51.00	4009.0
51.90	158.0
54.90	395.0
56.00	1135.0
56.90	1935.0
60.10	762.0
61.00	3317.0
62.00	3180.0
63.00	2309.0
63.90	450.0
65.00	542.0
67.10	171.0
68.00	6399.0
69.00	7474.0
70.10	509.0
71.90	494.0
73.00	3510.0
74.00	11878.0
75.00	33208.0
76.10	3002.0
77.00	408.0
77.80	246.0
78.90	2630.0
79.90	742.0
80.90	2771.0
81.80	795.0
86.00	109.0
87.00	2445.0
87.90	2115.0
91.00	356.0
92.00	2020.0
93.00	2873.0
94.10	6880.0
95.00	56504.0
96.10	4038.0
104.00	364.0
105.90	361.0
112.90	115.0
116.00	302.0
116.80	642.0
117.80	285.0
119.00	430.0
127.90	244.0
129.90	203.0
130.70	139.0
134.70	109.0
137.00	133.0
141.00	912.0
143.00	1050.0
145.00	204.0
155.00	209.0
157.00	179.0
170.80	209.0
172.10	466.0
174.00	42872.0
175.00	3608.0
176.00	41744.0
177.10	2677.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	654.0
37.00	3619.0
38.10	3515.0
39.00	1261.0
40.00	203.0
44.10	834.0
45.00	575.0
45.80	126.0
47.10	658.0
47.90	321.0
48.90	2582.0
50.00	12761.0
51.00	4016.0
51.90	208.0
54.90	363.0
56.00	1222.0
56.90	1963.0
60.10	812.0
61.00	3430.0
62.00	3231.0
63.00	2403.0
63.90	474.0
65.00	598.0
66.80	187.0
68.00	6344.0
69.00	7526.0
70.10	487.0
71.90	487.0
73.00	3433.0
74.00	11561.0
75.00	33616.0
76.10	2840.0
77.10	401.0
77.90	211.0
78.90	2817.0
79.90	714.0
80.90	2762.0
81.90	802.0
86.00	129.0
87.00	2216.0
87.90	2039.0
91.00	336.0
92.00	2030.0
93.00	2942.0
94.10	6974.0
95.00	55272.0
96.10	4123.0
96.90	129.0
103.90	352.0
105.80	432.0
112.80	106.0
115.90	328.0
116.80	717.0
117.80	213.0
119.00	387.0
127.90	275.0
129.90	259.0
131.10	130.0
137.00	134.0
141.00	849.0
143.00	1006.0
145.00	199.0
154.90	201.0
157.10	169.0
170.80	172.0
172.00	405.0
174.00	41472.0
175.00	3525.0
176.00	40808.0
177.00	2838.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
35.90	531.0
37.00	3140.0
38.00	2787.0
39.00	1131.0
40.00	249.0
43.80	802.0
45.10	519.0
47.10	669.0
47.90	450.0
49.00	2424.0
50.00	11539.0
51.00	3656.0
54.90	282.0
56.00	1052.0
56.90	1684.0
60.10	630.0
61.00	2919.0
62.00	2895.0
63.00	2157.0
64.00	350.0
65.00	429.0
67.00	199.0
68.00	6099.0
69.00	6567.0
70.10	427.0
71.90	440.0
73.00	3178.0
74.00	10966.0
75.00	29856.0
76.10	2843.0
76.90	443.0
77.80	342.0
78.90	2271.0
79.90	707.0
81.00	2492.0
81.80	659.0
87.00	2417.0
87.90	1796.0
90.90	299.0
91.90	1820.0
93.00	2504.0
94.10	6285.0
95.10	52440.0
96.10	3415.0
104.00	365.0
105.90	304.0
116.00	207.0
116.90	488.0
117.80	315.0
119.00	418.0
128.10	218.0
129.90	142.0
130.70	163.0
134.70	147.0
140.90	912.0
143.00	932.0
145.00	143.0
155.10	210.0
157.00	182.0
170.80	165.0
172.10	407.0
174.00	40680.0
175.00	3381.0
176.00	39168.0
177.10	2508.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

Scan 2884 (10.613 min): VU037183.D
BFB60

m/z	Abundance
40.00	319.0
43.90	831.0
73.00	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60