

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048213.D
 Acq On : 22 Apr 2022 10:32
 Operator : SY/MD
 Sample : VU0422MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	157559	192802	16.71%	2.053%
2	1.916	170	179	200	rVB	115015	163999	14.21%	1.746%
3	2.568	370	382	408	rBV	259228	429311	37.20%	4.570%
4	2.732	428	433	434	rBV3	532	435	0.04%	0.005%
5	2.797	450	453	462	rVB3	669	695	0.06%	0.007%
6	2.861	469	473	475	rBV2	281	257	0.02%	0.003%
7	2.954	499	502	503	rBV	352	235	0.02%	0.003%
8	2.993	511	514	517	rVB2	384	184	0.02%	0.002%
9	3.012	518	520	523	rVB2	329	174	0.02%	0.002%
10	3.051	523	532	542	rBV4	2706	5078	0.44%	0.054%
11	3.186	568	574	579	rVV4	492	769	0.07%	0.008%
12	3.240	586	591	597	rVB2	379	414	0.04%	0.004%
13	3.298	607	609	613	rBV2	259	170	0.01%	0.002%
14	3.385	633	636	641	rVB2	180	173	0.01%	0.002%
15	3.424	646	648	653	rVV	248	221	0.02%	0.002%
16	3.498	665	671	677	rBV2	289	455	0.04%	0.005%
17	3.896	792	795	801	rVV2	225	245	0.02%	0.003%
18	3.951	809	812	817	rVV	216	188	0.02%	0.002%
19	3.990	820	824	828	rBV	298	328	0.03%	0.003%
20	4.051	837	843	844	rBV	344	240	0.02%	0.003%
21	4.189	880	886	889	rBV2	205	270	0.02%	0.003%
22	4.228	895	898	904	rVB	214	198	0.02%	0.002%
23	4.456	967	969	975	rVV2	294	232	0.02%	0.002%
24	4.626	1007	1022	1054	rBV	111596	284616	24.66%	3.030%
25	4.925	1112	1115	1127	rVB2	461	758	0.07%	0.008%
26	4.980	1127	1132	1134	rBV2	335	236	0.02%	0.003%
27	5.006	1134	1140	1142	rBV2	264	299	0.03%	0.003%
28	5.067	1142	1159	1179	rBV	204878	447163	38.75%	4.760%
29	5.199	1197	1200	1206	rVB2	272	267	0.02%	0.003%
30	5.256	1216	1218	1223	rVB3	443	203	0.02%	0.002%
31	5.285	1223	1227	1229	rBV2	425	370	0.03%	0.004%
32	5.729	1343	1365	1404	rVV2	427665	1154073	100.00%	12.286%
33	6.035	1456	1460	1462	rBV	239	222	0.02%	0.002%
34	6.047	1462	1464	1470	rVB3	372	313	0.03%	0.003%
35	6.105	1476	1482	1485	rBV3	437	487	0.04%	0.005%
36	6.121	1485	1487	1490	rVB4	304	179	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048213.D
 Acq On : 22 Apr 2022 10:32
 Operator : SY/MD
 Sample : VU0422MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1513	1527	1547	rBV	394361	748671	64.87%	7.970%
38	6.459	1590	1592	1596	rBV	314	266	0.02%	0.003%
39	6.530	1607	1614	1624	rBV5	1329	2428	0.21%	0.026%
40	6.694	1650	1665	1686	rBV	261721	510172	44.21%	5.431%
41	6.803	1696	1699	1701	rBV2	374	244	0.02%	0.003%
42	6.896	1726	1728	1732	rBV	304	191	0.02%	0.002%
43	6.973	1748	1752	1755	rBV2	192	185	0.02%	0.002%
44	7.044	1770	1774	1776	rBV2	433	305	0.03%	0.003%
45	7.096	1788	1790	1794	rVV2	359	218	0.02%	0.002%
46	7.186	1810	1818	1827	rVV5	1280	2249	0.19%	0.024%
47	7.247	1835	1837	1844	rVB3	357	291	0.03%	0.003%
48	7.362	1867	1873	1875	rBV	178	218	0.02%	0.002%
49	7.398	1880	1884	1885	rBV	326	193	0.02%	0.002%
50	7.568	1924	1937	1959	rBV	129747	235192	20.38%	2.504%
51	7.690	1970	1975	1986	rVB4	981	1470	0.13%	0.016%
52	7.793	1997	2007	2009	rBV4	1264	1355	0.12%	0.014%
53	7.899	2026	2040	2057	rBV	522518	895288	77.58%	9.531%
54	8.182	2114	2128	2145	rBV	93109	163981	14.21%	1.746%
55	8.555	2241	2244	2248	rBV2	366	352	0.03%	0.004%
56	8.636	2256	2269	2323	rBV	328500	638551	55.33%	6.798%
57	8.925	2357	2359	2361	rBV2	310	193	0.02%	0.002%
58	9.115	2416	2418	2421	rBV3	230	186	0.02%	0.002%
59	9.263	2462	2464	2467	rBV	341	200	0.02%	0.002%
60	9.417	2498	2512	2547	rBV	575752	995445	86.25%	10.597%
61	9.597	2566	2568	2574	rBV2	286	234	0.02%	0.002%
62	9.636	2577	2580	2583	rBV2	288	178	0.02%	0.002%
63	9.694	2593	2598	2599	rBV2	617	440	0.04%	0.005%
64	9.931	2667	2672	2676	rBV3	283	278	0.02%	0.003%
65	10.112	2719	2728	2731	rBV5	549	693	0.06%	0.007%
66	10.224	2760	2763	2766	rVB2	325	229	0.02%	0.002%
67	10.247	2766	2770	2778	rBV2	330	541	0.05%	0.006%
68	10.340	2790	2799	2801	rBV2	238	342	0.03%	0.004%
69	10.475	2838	2841	2844	rBV2	248	197	0.02%	0.002%
70	10.513	2850	2853	2858	rVB3	232	172	0.01%	0.002%
71	10.555	2864	2866	2871	rVB	255	176	0.02%	0.002%
72	10.581	2871	2874	2878	rBV	250	219	0.02%	0.002%
73	10.668	2895	2901	2912	rBV5	2555	3739	0.32%	0.040%
74	10.758	2915	2929	2952	rBV	381439	617227	53.48%	6.571%
75	10.896	2968	2972	2977	rVB4	708	668	0.06%	0.007%
76	10.999	3001	3004	3009	rBV3	336	308	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048213.D
 Acq On : 22 Apr 2022 10:32
 Operator : SY/MD
 Sample : VU0422MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.086	3027	3031	3033	rBV2	373	282	0.02%	0.003%
78	11.115	3038	3040	3047	rVB3	314	327	0.03%	0.003%
79	11.324	3101	3105	3107	rBV2	305	262	0.02%	0.003%
80	11.465	3140	3149	3159	rVB8	1933	3557	0.31%	0.038%
81	11.581	3183	3185	3190	rVB3	256	197	0.02%	0.002%
82	11.626	3196	3199	3202	rBV2	311	197	0.02%	0.002%
83	11.674	3211	3214	3216	rBV	413	213	0.02%	0.002%
84	11.697	3216	3221	3222	rBV3	653	446	0.04%	0.005%
85	11.745	3230	3236	3244	rBV5	2006	2580	0.22%	0.027%
86	11.812	3244	3257	3278	rBV	620253	998027	86.48%	10.625%
87	11.941	3292	3297	3303	rBV5	1007	1516	0.13%	0.016%
88	11.973	3304	3307	3313	rVB5	2195	2044	0.18%	0.022%
89	12.195	3358	3376	3396	rBV	501560	842319	72.99%	8.967%
90	12.404	3439	3441	3447	rVB2	411	354	0.03%	0.004%
91	12.433	3447	3450	3453	rBV2	445	244	0.02%	0.003%
92	12.610	3502	3505	3508	rBV3	387	299	0.03%	0.003%
93	12.989	3620	3623	3625	rBV2	272	177	0.02%	0.002%
94	13.195	3684	3687	3690	rBV	358	267	0.02%	0.003%
95	13.227	3690	3697	3707	rVV5	1343	2147	0.19%	0.023%
96	13.844	3881	3889	3901	rVB3	5612	8696	0.75%	0.093%
97	14.092	3957	3966	3975	rBV	6817	11173	0.97%	0.119%
98	14.333	4034	4041	4050	rVB5	4599	7177	0.62%	0.076%
99	15.018	4252	4254	4260	rVB3	794	663	0.06%	0.007%
100	15.349	4352	4357	4359	rBV3	604	589	0.05%	0.006%


Sum of corrected areas: 9393497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048213.D
Acq On : 22 Apr 2022 10:32
Operator : SY/MD
Sample : VU0422MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

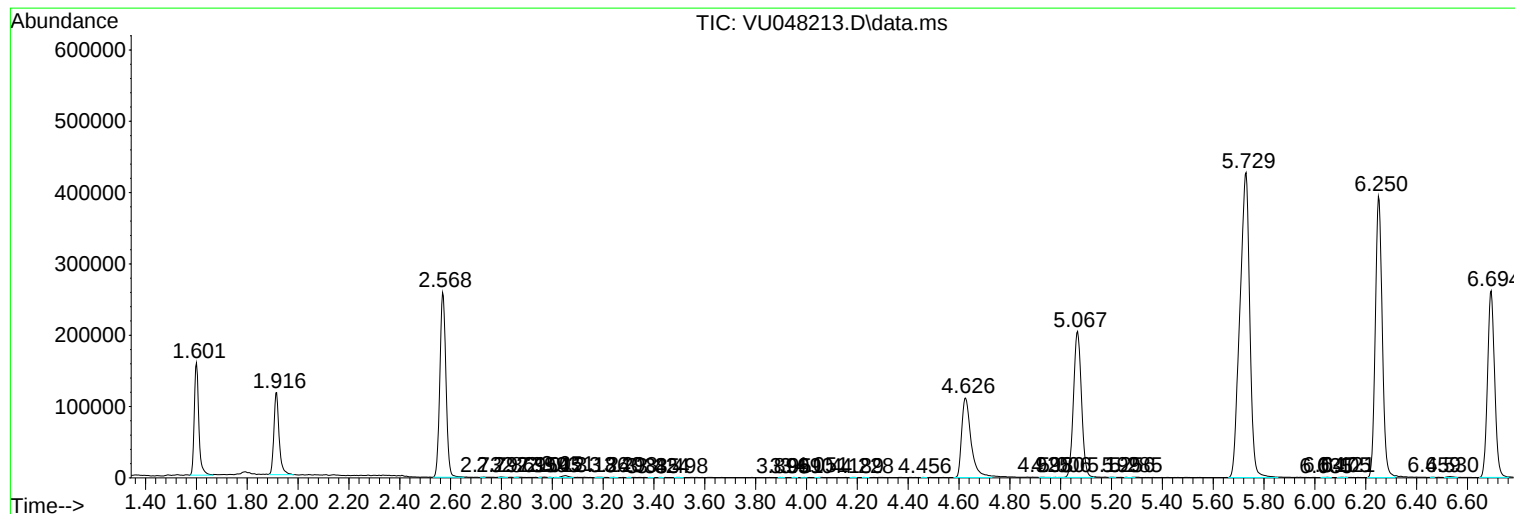

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048213.D
Acq On : 22 Apr 2022 10:32
Operator : SY/MD
Sample : VU0422MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048213.D
Acq On : 22 Apr 2022 10:32
Operator : SY/MD
Sample : VU0422MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc