

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048214.D
 Acq On : 22 Apr 2022 10:55
 Operator : SY/MD
 Sample : VU0422WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	156258	185880	16.07%	2.005%
2	1.916	171	179	201	rVB	115455	163130	14.10%	1.760%
3	2.568	370	382	412	rVB	255185	424541	36.70%	4.579%
4	2.983	507	511	515	rBV3	339	240	0.02%	0.003%
5	3.002	515	517	518	rBV3	221	92	0.01%	0.001%
6	3.047	524	531	541	rBV4	2546	4988	0.43%	0.054%
7	3.144	558	561	563	rBV2	180	131	0.01%	0.001%
8	3.176	568	571	575	rBV2	807	759	0.07%	0.008%
9	3.231	586	588	590	rBV	217	125	0.01%	0.001%
10	3.324	613	617	619	rBV2	306	175	0.02%	0.002%
11	3.362	628	629	631	rBV2	115	47	0.00%	0.001%
12	3.378	631	634	637	rBV3	313	254	0.02%	0.003%
13	3.430	646	650	656	rVB3	326	246	0.02%	0.003%
14	3.456	656	658	661	rBV	200	92	0.01%	0.001%
15	3.507	672	674	677	rBV	170	139	0.01%	0.001%
16	3.555	686	689	690	rBV	142	79	0.01%	0.001%
17	3.597	699	702	706	rVB3	321	240	0.02%	0.003%
18	3.620	706	709	712	rBV2	282	183	0.02%	0.002%
19	3.674	723	726	728	rBV	137	101	0.01%	0.001%
20	3.764	751	754	755	rBV	168	82	0.01%	0.001%
21	3.800	763	765	768	rVB	248	98	0.01%	0.001%
22	3.819	768	771	772	rBV	208	103	0.01%	0.001%
23	3.841	777	778	779	rBV	89	26	0.00%	0.000%
24	3.851	779	781	783	rVB	139	48	0.00%	0.001%
25	3.861	783	784	786	rBV	150	63	0.01%	0.001%
26	3.919	799	802	805	rBV2	115	82	0.01%	0.001%
27	3.960	810	815	819	rBV	261	247	0.02%	0.003%
28	3.983	819	822	824	rBV	143	106	0.01%	0.001%
29	4.034	835	838	841	rVB	264	102	0.01%	0.001%
30	4.131	865	868	871	rBV	112	91	0.01%	0.001%
31	4.192	883	887	891	rBV	184	172	0.01%	0.002%
32	4.263	906	909	911	rBV2	221	125	0.01%	0.001%
33	4.295	916	919	922	rVB2	237	154	0.01%	0.002%
34	4.436	957	963	966	rBV2	172	207	0.02%	0.002%
35	4.568	1001	1004	1005	rBV	124	71	0.01%	0.001%
36	4.626	1009	1022	1063	rBV	112980	299478	25.89%	3.230%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048214.D
 Acq On : 22 Apr 2022 10:55
 Operator : SY/MD
 Sample : VU0422WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.067	1142	1159	1184	rBV	205897	450492	38.94%	4.859%
38	5.276	1222	1224	1226	rBV	436	254	0.02%	0.003%
39	5.414	1264	1267	1272	rBV2	166	159	0.01%	0.002%
40	5.501	1290	1294	1299	rVB2	190	159	0.01%	0.002%
41	5.729	1343	1365	1401	rBV2	425504	1156778	100.00%	12.477%
42	6.038	1457	1461	1463	rBV3	381	260	0.02%	0.003%
43	6.118	1481	1486	1490	rBV	261	314	0.03%	0.003%
44	6.153	1494	1497	1498	rBV2	296	132	0.01%	0.001%
45	6.250	1506	1527	1554	rBV	368362	707920	61.20%	7.636%
46	6.533	1605	1615	1622	rBV4	1266	2154	0.19%	0.023%
47	6.613	1637	1640	1641	rBV	128	78	0.01%	0.001%
48	6.623	1641	1643	1644	rVV	143	61	0.01%	0.001%
49	6.693	1650	1665	1685	rBV	261377	514684	44.49%	5.551%
50	6.861	1713	1717	1722	rBV2	195	187	0.02%	0.002%
51	7.009	1762	1763	1764	rVB2	116	22	0.00%	0.000%
52	7.021	1764	1767	1771	rBV2	210	146	0.01%	0.002%
53	7.054	1771	1777	1780	rBV2	241	336	0.03%	0.004%
54	7.108	1791	1794	1800	rBV2	283	256	0.02%	0.003%
55	7.144	1800	1805	1810	rBV2	342	329	0.03%	0.004%
56	7.185	1810	1818	1819	rBV3	1225	1070	0.09%	0.012%
57	7.292	1849	1851	1854	rBV	200	111	0.01%	0.001%
58	7.378	1877	1878	1879	rBV	124	27	0.00%	0.000%
59	7.423	1889	1892	1895	rBV2	163	151	0.01%	0.002%
60	7.468	1904	1906	1909	rBV	100	45	0.00%	0.000%
61	7.491	1911	1913	1915	rVB	148	40	0.00%	0.000%
62	7.507	1915	1918	1919	rBV	102	63	0.01%	0.001%
63	7.568	1923	1937	1956	rBV	134602	240230	20.77%	2.591%
64	7.674	1966	1970	1972	rBV3	795	620	0.05%	0.007%
65	7.738	1987	1990	1993	rBV4	359	255	0.02%	0.003%
66	7.787	2001	2005	2015	rBV2	859	1213	0.10%	0.013%
67	7.899	2026	2040	2056	rBV	517079	897081	77.55%	9.676%
68	8.179	2116	2127	2146	rBV	94963	163999	14.18%	1.769%
69	8.427	2202	2204	2208	rBV3	254	207	0.02%	0.002%
70	8.520	2231	2233	2234	rBV3	130	60	0.01%	0.001%
71	8.526	2234	2235	2241	rVB3	394	305	0.03%	0.003%
72	8.636	2256	2269	2302	rBV	343558	661701	57.20%	7.137%
73	8.954	2365	2368	2373	rVB	207	133	0.01%	0.001%
74	8.976	2373	2375	2379	rBV	321	149	0.01%	0.002%
75	9.002	2381	2383	2385	rBV	211	88	0.01%	0.001%
76	9.147	2419	2428	2432	rBV2	519	755	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048214.D
 Acq On : 22 Apr 2022 10:55
 Operator : SY/MD
 Sample : VU0422WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.417	2499	2512	2535	rBV	568643	960047	82.99%	10.355%
78	9.639	2577	2581	2584	rBV3	359	317	0.03%	0.003%
79	9.693	2593	2598	2606	rVB4	868	1086	0.09%	0.012%
80	9.796	2628	2630	2631	rBV	245	94	0.01%	0.001%
81	9.883	2653	2657	2661	rBV2	274	225	0.02%	0.002%
82	9.918	2666	2668	2671	rBV	151	77	0.01%	0.001%
83	10.095	2720	2723	2727	rBV2	351	345	0.03%	0.004%
84	10.237	2765	2767	2768	rBV2	186	67	0.01%	0.001%
85	10.600	2878	2880	2881	rBV2	141	42	0.00%	0.000%
86	10.629	2886	2889	2894	rBV	315	317	0.03%	0.003%
87	10.671	2895	2902	2916	rVB6	2493	3758	0.32%	0.041%
88	10.758	2916	2929	2946	rBV	383164	628278	54.31%	6.777%
89	10.860	2958	2961	2964	rBV2	464	386	0.03%	0.004%
90	11.150	3049	3051	3054	rBV2	292	190	0.02%	0.002%
91	11.410	3128	3132	3134	rBV	220	182	0.02%	0.002%
92	11.812	3244	3257	3280	rBV	581291	943106	81.53%	10.173%
93	12.195	3361	3376	3397	rBV	508052	838837	72.51%	9.048%
94	14.092	3962	3966	3976	rVB3	3013	4144	0.36%	0.045%
95	14.336	4036	4042	4050	rVB4	2873	3884	0.34%	0.042%




Sum of corrected areas: 9271103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048214.D
Acq On : 22 Apr 2022 10:55
Operator : SY/MD
Sample : VU0422WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

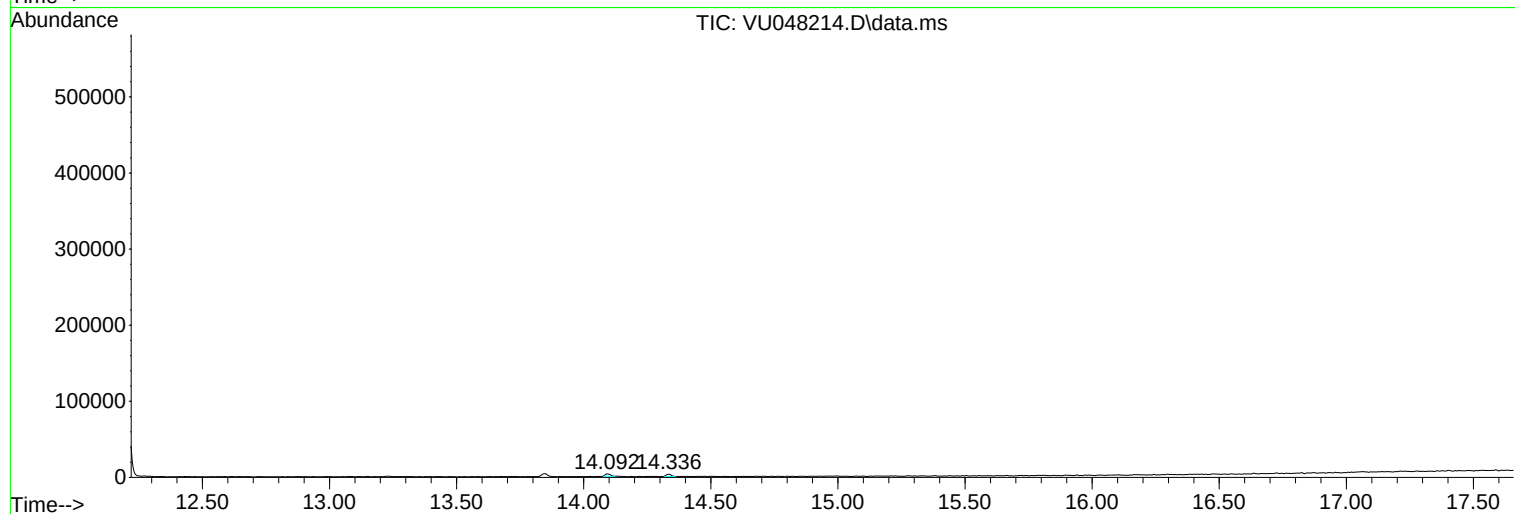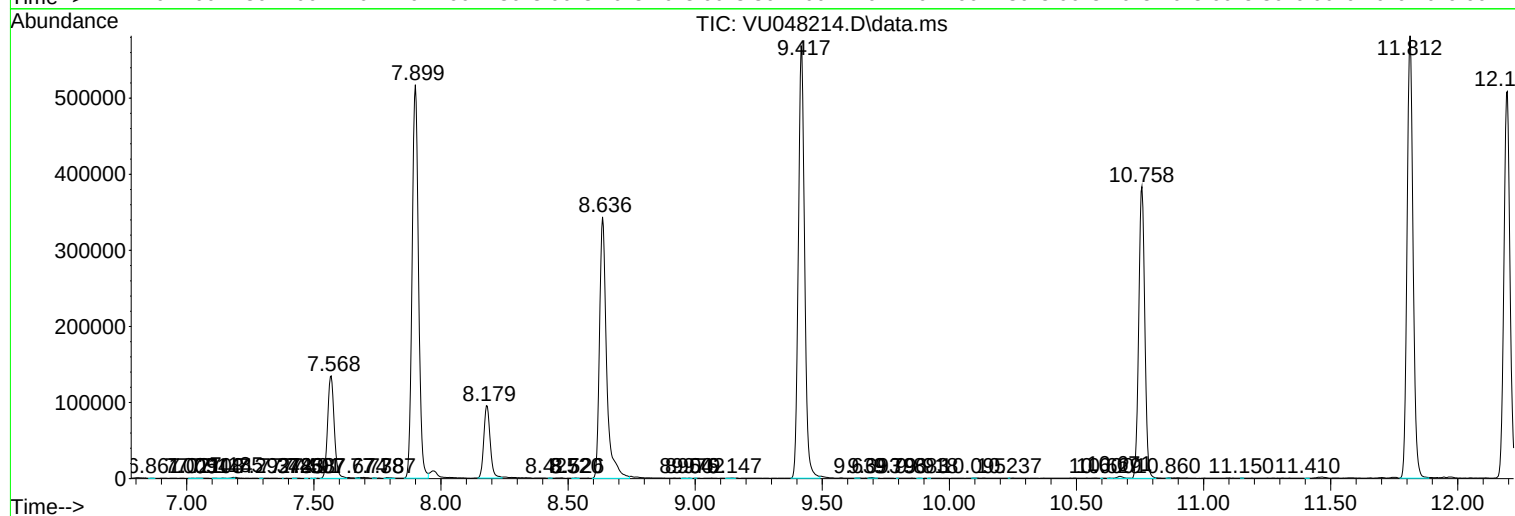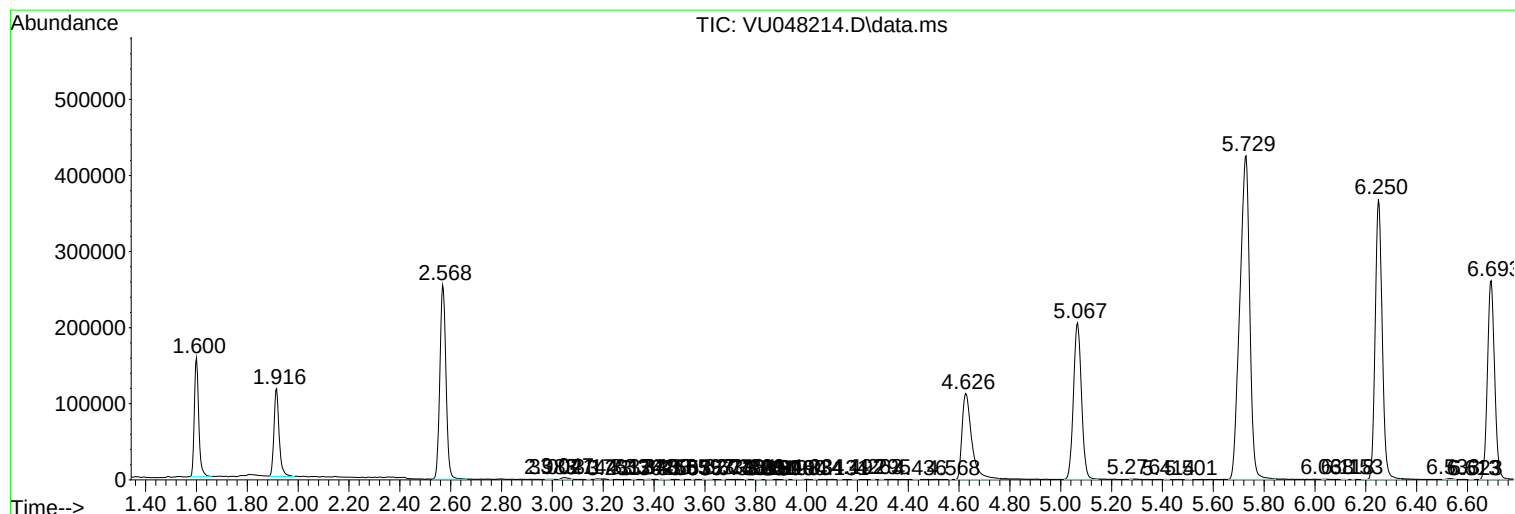

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048214.D
Acq On : 22 Apr 2022 10:55
Operator : SY/MD
Sample : VU0422WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048214.D
Acq On : 22 Apr 2022 10:55
Operator : SY/MD
Sample : VU0422WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc