

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048215.D
 Acq On : 22 Apr 2022 11:19
 Operator : SY/MD
 Sample : N2485-15DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	102	rBV	155469	188367	1.38%	0.553%
2	1.913	170	178	203	rVB	114666	164629	1.21%	0.483%
3	2.568	370	382	398	rBV	255458	418978	3.07%	1.229%
4	2.687	416	419	423	rVB3	507	304	0.00%	0.001%
5	2.765	433	443	461	rVB2	9529	20222	0.15%	0.059%
6	2.855	467	471	476	rVB3	459	442	0.00%	0.001%
7	2.941	496	498	500	rBV2	288	161	0.00%	0.000%
8	2.957	500	503	505	rVV2	311	204	0.00%	0.001%
9	2.990	509	513	517	rVB2	302	193	0.00%	0.001%
10	3.048	521	531	542	rBV3	4852	9379	0.07%	0.028%
11	3.134	554	558	564	rBV3	803	1038	0.01%	0.003%
12	3.183	565	573	590	rVB	3912	9006	0.07%	0.026%
13	3.404	639	642	646	rBV2	193	179	0.00%	0.001%
14	3.443	646	654	656	rVV2	267	366	0.00%	0.001%
15	3.453	656	657	663	rVV	272	189	0.00%	0.001%
16	3.668	716	724	726	rBV	384	412	0.00%	0.001%
17	3.771	753	756	759	rBV	217	172	0.00%	0.001%
18	3.877	785	789	796	rVB2	206	301	0.00%	0.001%
19	4.533	988	993	994	rBV2	345	272	0.00%	0.001%
20	4.623	1008	1021	1051	rBV	120451	304068	2.23%	0.892%
21	5.067	1141	1159	1183	rBV	205992	464660	3.41%	1.363%
22	5.215	1202	1205	1208	rVB2	396	293	0.00%	0.001%
23	5.292	1223	1229	1236	rVB4	659	919	0.01%	0.003%
24	5.340	1241	1244	1249	rVB2	309	197	0.00%	0.001%
25	5.398	1259	1262	1266	rVB2	401	288	0.00%	0.001%
26	5.433	1270	1273	1279	rVB2	208	256	0.00%	0.001%
27	5.469	1281	1284	1293	rVB2	233	283	0.00%	0.001%
28	5.504	1293	1295	1297	rBV	258	178	0.00%	0.001%
29	5.623	1329	1332	1336	rBV2	199	199	0.00%	0.001%
30	5.729	1343	1365	1369	rBV2	431275	1040724	7.63%	3.053%
31	5.777	1370	1380	1416	rVB	2629713	5370246	39.35%	15.753%
32	6.250	1512	1527	1550	rBV	384092	722424	5.29%	2.119%
33	6.382	1567	1568	1573	rVB2	359	185	0.00%	0.001%
34	6.404	1573	1575	1580	rVB3	267	168	0.00%	0.000%
35	6.523	1608	1612	1614	rBV2	1253	910	0.01%	0.003%
36	6.694	1650	1665	1691	rBV	261676	513318	3.76%	1.506%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048215.D
 Acq On : 22 Apr 2022 11:19
 Operator : SY/MD
 Sample : N2485-15DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.893	1723	1727	1733	rVB2	289	345	0.00%	0.001%
38	7.041	1768	1773	1774	rBV2	477	331	0.00%	0.001%
39	7.070	1780	1782	1786	rVB2	302	167	0.00%	0.000%
40	7.186	1810	1818	1827	rBV4	1731	2632	0.02%	0.008%
41	7.285	1846	1849	1850	rBV2	278	199	0.00%	0.001%
42	7.456	1898	1902	1905	rBV2	156	166	0.00%	0.000%
43	7.568	1923	1937	1952	rBV	135647	238839	1.75%	0.701%
44	7.755	1991	1995	1999	rBV2	391	306	0.00%	0.001%
45	7.793	2002	2007	2009	rBV3	687	505	0.00%	0.001%
46	7.899	2025	2040	2055	rBV	502174	855145	6.27%	2.508%
47	8.073	2091	2094	2097	rBV3	281	212	0.00%	0.001%
48	8.096	2100	2101	2105	rVB	547	230	0.00%	0.001%
49	8.179	2112	2127	2145	rBV	95252	161556	1.18%	0.474%
50	8.298	2161	2164	2170	rVB4	773	634	0.00%	0.002%
51	8.469	2215	2217	2221	rVB2	286	185	0.00%	0.001%
52	8.488	2221	2223	2228	rVB2	328	233	0.00%	0.001%
53	8.517	2228	2232	2236	rVB3	465	361	0.00%	0.001%
54	8.562	2241	2246	2249	rBV	309	244	0.00%	0.001%
55	8.633	2251	2268	2310	rBV	332176	637033	4.67%	1.869%
56	8.796	2317	2319	2321	rVB3	532	235	0.00%	0.001%
57	8.870	2338	2342	2344	rBV2	223	178	0.00%	0.001%
58	8.909	2351	2354	2355	rBV	376	212	0.00%	0.001%
59	8.944	2362	2365	2367	rVB3	332	186	0.00%	0.001%
60	8.973	2371	2374	2377	rBV2	236	201	0.00%	0.001%
61	9.063	2397	2402	2408	rVB2	385	416	0.00%	0.001%
62	9.131	2414	2423	2426	rBV3	361	477	0.00%	0.001%
63	9.449	2498	2522	2566	rBV	7901341	13645901	100.00%	40.028%
64	9.697	2591	2599	2606	rVV5	1500	1919	0.01%	0.006%
65	9.739	2608	2612	2614	rBV2	329	278	0.00%	0.001%
66	9.851	2644	2647	2652	rVB2	336	328	0.00%	0.001%
67	9.906	2660	2664	2666	rBV3	574	400	0.00%	0.001%
68	9.941	2672	2675	2679	rVB	427	369	0.00%	0.001%
69	9.960	2679	2681	2685	rBV2	331	200	0.00%	0.001%
70	10.054	2705	2710	2716	rBV2	801	1137	0.01%	0.003%
71	10.356	2800	2804	2806	rBV2	208	162	0.00%	0.000%
72	10.391	2811	2815	2819	rBV2	185	180	0.00%	0.001%
73	10.443	2828	2831	2836	rBV2	177	173	0.00%	0.001%
74	10.468	2836	2839	2840	rBV	346	197	0.00%	0.001%
75	10.668	2896	2901	2915	rVB4	2186	3146	0.02%	0.009%
76	10.758	2915	2929	2948	rBV	378630	612488	4.49%	1.797%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048215.D
 Acq On : 22 Apr 2022 11:19
 Operator : SY/MD
 Sample : N2485-15DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.919	2977	2979	2986	rVB3	386	336	0.00%	0.001%
78	11.089	3029	3032	3036	rVB3	424	308	0.00%	0.001%
79	11.121	3038	3042	3046	rVB3	343	276	0.00%	0.001%
80	11.292	3090	3095	3098	rBV	251	292	0.00%	0.001%
81	11.456	3142	3146	3148	rBV2	1060	816	0.01%	0.002%
82	11.693	3216	3220	3225	rVB2	698	716	0.01%	0.002%
83	11.745	3225	3236	3246	rBV	91071	145646	1.07%	0.427%
84	11.835	3246	3264	3289	rVB2	2129521	4158043	30.47%	12.197%
85	12.086	3338	3342	3344	rBV3	241	202	0.00%	0.001%
86	12.211	3362	3381	3402	rVV2	2256780	4246330	31.12%	12.456%
87	12.632	3509	3512	3514	rBV3	317	253	0.00%	0.001%
88	12.912	3596	3599	3602	rBV	431	354	0.00%	0.001%
89	12.976	3616	3619	3623	rVB3	869	695	0.01%	0.002%
90	13.012	3628	3630	3633	rVB2	301	165	0.00%	0.000%
91	13.047	3638	3641	3642	rBV2	267	162	0.00%	0.000%
92	13.095	3653	3656	3660	rVB2	295	199	0.00%	0.001%
93	13.205	3688	3690	3692	rBV	377	246	0.00%	0.001%
94	13.327	3725	3728	3730	rBV2	355	201	0.00%	0.001%
95	13.594	3808	3811	3814	rBV2	320	225	0.00%	0.001%
96	13.841	3877	3888	3902	rBV	66339	103709	0.76%	0.304%
97	14.092	3960	3966	3974	rVB	3082	4162	0.03%	0.012%
98	14.330	4031	4040	4054	rVB2	15868	24968	0.18%	0.073%
99	14.565	4110	4113	4115	rBV2	401	277	0.00%	0.001%
100	15.044	4259	4262	4264	rBV2	615	407	0.00%	0.001%




Sum of corrected areas: 34091224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048215.D
Acq On : 22 Apr 2022 11:19
Operator : SY/MD
Sample : N2485-15DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

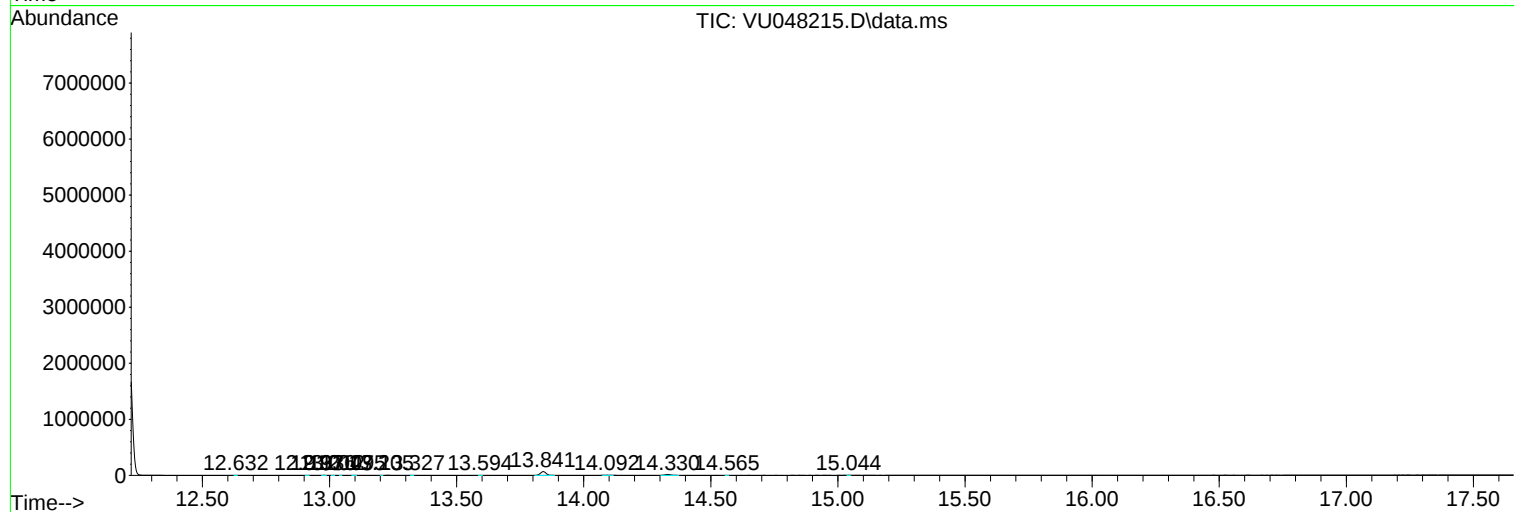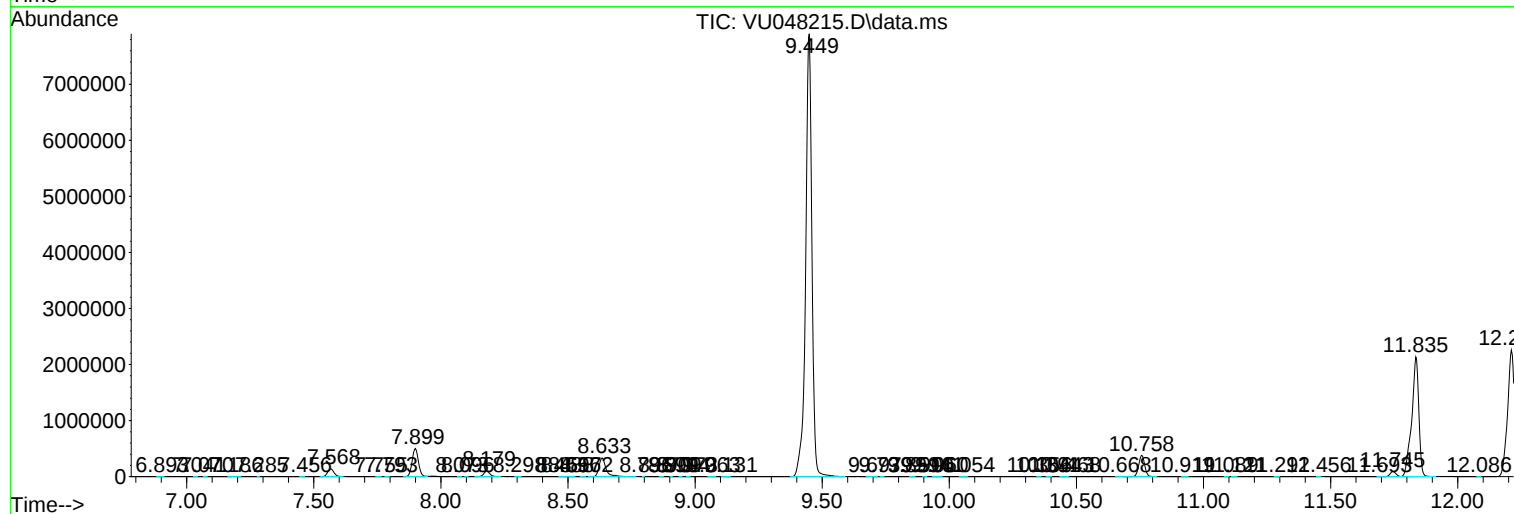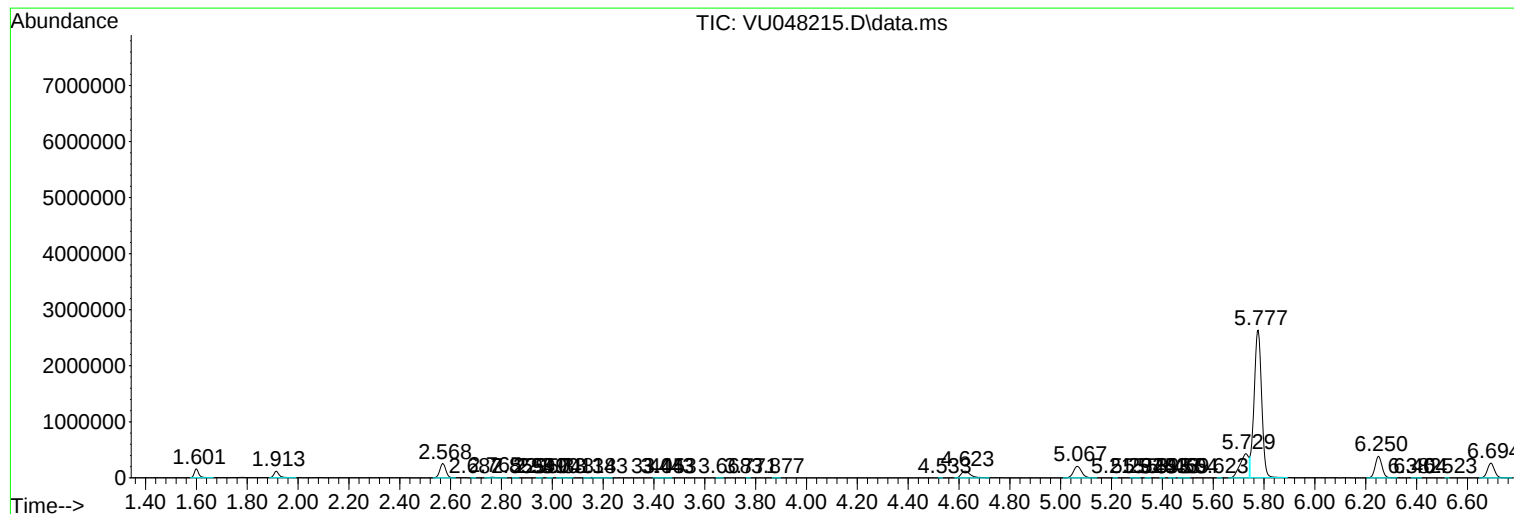

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048215.D
Acq On : 22 Apr 2022 11:19
Operator : SY/MD
Sample : N2485-15DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048215.D
Acq On : 22 Apr 2022 11:19
Operator : SY/MD
Sample : N2485-15DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------