

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048216.D
 Acq On : 22 Apr 2022 11:42
 Operator : SY/MD
 Sample : N2485-16DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	100	rBV	158853	188930	1.43%	0.567%
2	1.915	170	179	194	rBV	114261	161188	1.22%	0.484%
3	2.568	370	382	396	rBV	252856	417416	3.16%	1.252%
4	2.774	431	446	461	rBV2	8910	21781	0.16%	0.065%
5	2.935	494	496	498	rBV2	351	183	0.00%	0.001%
6	2.996	511	515	517	rBV	312	225	0.00%	0.001%
7	3.050	521	532	543	rBV3	4718	9344	0.07%	0.028%
8	3.134	553	558	560	rBV4	523	471	0.00%	0.001%
9	3.182	564	573	574	rBV3	2896	2868	0.02%	0.009%
10	3.234	587	589	592	rVB2	617	300	0.00%	0.001%
11	3.417	639	646	647	rBV	249	278	0.00%	0.001%
12	3.497	665	671	678	rBV2	296	350	0.00%	0.001%
13	3.607	700	705	707	rBV2	246	245	0.00%	0.001%
14	3.636	712	714	717	rVV2	270	214	0.00%	0.001%
15	3.668	721	724	729	rVB	262	200	0.00%	0.001%
16	3.864	781	785	789	rBV3	215	185	0.00%	0.001%
17	4.018	830	833	835	rBV	256	169	0.00%	0.001%
18	4.060	841	846	851	rVB2	258	233	0.00%	0.001%
19	4.169	876	880	883	rBV2	242	165	0.00%	0.000%
20	4.259	903	908	911	rBV	187	165	0.00%	0.000%
21	4.626	1008	1022	1051	rBV	120799	305915	2.31%	0.918%
22	4.986	1131	1134	1137	rBV2	331	273	0.00%	0.001%
23	5.066	1139	1159	1181	rVV	204780	464348	3.51%	1.393%
24	5.198	1198	1200	1202	rVB2	379	171	0.00%	0.001%
25	5.221	1202	1207	1209	rBV3	332	245	0.00%	0.001%
26	5.269	1214	1222	1224	rBV	308	346	0.00%	0.001%
27	5.362	1248	1251	1256	rBV	315	240	0.00%	0.001%
28	5.394	1257	1261	1268	rVB3	317	359	0.00%	0.001%
29	5.529	1296	1303	1304	rBV3	382	418	0.00%	0.001%
30	5.729	1343	1365	1369	rBV2	439044	1038773	7.85%	3.117%
31	5.777	1370	1380	1423	rVB	2523649	5149523	38.93%	15.450%
32	6.089	1474	1477	1479	rBV3	616	383	0.00%	0.001%
33	6.140	1490	1493	1496	rBV4	531	412	0.00%	0.001%
34	6.250	1513	1527	1545	rBV	388449	731749	5.53%	2.196%
35	6.520	1609	1611	1612	rBV	808	369	0.00%	0.001%
36	6.693	1649	1665	1684	rBV	261522	512575	3.88%	1.538%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048216.D
 Acq On : 22 Apr 2022 11:42
 Operator : SY/MD
 Sample : N2485-16DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.828	1706	1707	1712	rVB2	385	173	0.00%	0.001%
38	6.996	1752	1759	1762	rVB2	179	217	0.00%	0.001%
39	7.054	1774	1777	1781	rVB2	310	257	0.00%	0.001%
40	7.189	1809	1819	1828	rBV4	1467	2433	0.02%	0.007%
41	7.263	1836	1842	1844	rBV2	291	281	0.00%	0.001%
42	7.382	1876	1879	1882	rVB2	231	173	0.00%	0.001%
43	7.407	1882	1887	1889	rBV	237	273	0.00%	0.001%
44	7.568	1924	1937	1955	rBV	133071	237862	1.80%	0.714%
45	7.780	2000	2003	2005	rBV2	213	165	0.00%	0.000%
46	7.799	2005	2009	2012	rVV4	622	606	0.00%	0.002%
47	7.816	2012	2014	2018	rVB2	418	245	0.00%	0.001%
48	7.899	2027	2040	2055	rBV	521268	896169	6.78%	2.689%
49	8.179	2112	2127	2148	rBV	93652	161794	1.22%	0.485%
50	8.471	2214	2218	2219	rBV3	240	181	0.00%	0.001%
51	8.491	2219	2224	2228	rVV2	358	398	0.00%	0.001%
52	8.635	2256	2269	2300	rBV	337143	638737	4.83%	1.916%
53	8.838	2329	2332	2335	rBV3	299	197	0.00%	0.001%
54	8.909	2351	2354	2359	rBV2	378	367	0.00%	0.001%
55	8.979	2372	2376	2379	rVB2	361	215	0.00%	0.001%
56	9.166	2430	2434	2439	rVB2	399	458	0.00%	0.001%
57	9.211	2439	2448	2454	rBV2	241	373	0.00%	0.001%
58	9.446	2499	2521	2558	rBV	7462262	13226268	100.00%	39.684%
59	9.693	2594	2598	2609	rVB5	1215	1534	0.01%	0.005%
60	9.819	2635	2637	2645	rVB4	413	406	0.00%	0.001%
61	9.970	2681	2684	2688	rVB3	338	289	0.00%	0.001%
62	10.047	2705	2708	2711	rVV2	454	295	0.00%	0.001%
63	10.098	2720	2724	2729	rVV3	560	564	0.00%	0.002%
64	10.121	2729	2731	2735	rVB	281	184	0.00%	0.001%
65	10.179	2745	2749	2754	rBV2	226	289	0.00%	0.001%
66	10.208	2755	2758	2762	rVB2	284	204	0.00%	0.001%
67	10.378	2808	2811	2817	rVB	245	212	0.00%	0.001%
68	10.417	2820	2823	2827	rVB2	265	202	0.00%	0.001%
69	10.513	2850	2853	2857	rBV2	234	160	0.00%	0.000%
70	10.632	2888	2890	2893	rVB2	298	209	0.00%	0.001%
71	10.671	2894	2902	2910	rVV3	2621	3375	0.03%	0.010%
72	10.758	2916	2929	2949	rBV	371363	605953	4.58%	1.818%
73	10.857	2957	2960	2963	rBV3	227	215	0.00%	0.001%
74	11.092	3029	3033	3034	rBV	371	215	0.00%	0.001%
75	11.256	3081	3084	3086	rBV	365	188	0.00%	0.001%
76	11.433	3136	3139	3141	rBV2	409	258	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
 Data File : VU048216.D
 Acq On : 22 Apr 2022 11:42
 Operator : SY/MD
 Sample : N2485-16DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.465	3141	3149	3157	rVB4	1488	2515	0.02%	0.008%
78	11.696	3215	3221	3225	rBV3	744	781	0.01%	0.002%
79	11.745	3226	3236	3246	rBV	92597	143564	1.09%	0.431%
80	11.835	3246	3264	3284	rVB2	2059540	4114213	31.11%	12.344%
81	12.005	3315	3317	3320	rVB3	539	241	0.00%	0.001%
82	12.105	3345	3348	3350	rBV	329	208	0.00%	0.001%
83	12.211	3362	3381	3404	rBV2	2170100	4137478	31.28%	12.414%
84	12.362	3426	3428	3434	rVB4	489	424	0.00%	0.001%
85	12.410	3440	3443	3450	rBV3	634	641	0.00%	0.002%
86	12.574	3491	3494	3497	rBV2	270	229	0.00%	0.001%
87	12.696	3528	3532	3534	rBV3	404	310	0.00%	0.001%
88	12.876	3585	3588	3592	rVB3	328	251	0.00%	0.001%
89	13.005	3626	3628	3631	rBV	332	181	0.00%	0.001%
90	13.057	3642	3644	3648	rBV2	257	210	0.00%	0.001%
91	13.169	3676	3679	3682	rBV2	407	355	0.00%	0.001%
92	13.262	3706	3708	3714	rVB2	252	203	0.00%	0.001%
93	13.372	3739	3742	3745	rVB2	517	372	0.00%	0.001%
94	13.394	3745	3749	3752	rBV2	368	403	0.00%	0.001%
95	13.716	3846	3849	3852	rBB2	305	178	0.00%	0.001%
96	13.841	3877	3888	3900	rBV	65954	104824	0.79%	0.315%
97	14.015	3939	3942	3943	rBV	319	167	0.00%	0.001%
98	14.095	3960	3967	3970	rBV3	2088	2547	0.02%	0.008%
99	14.333	4032	4041	4050	rBV2	16155	24963	0.19%	0.075%
100	14.970	4236	4239	4243	rBV3	482	366	0.00%	0.001%




Sum of corrected areas: 33329227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048216.D
Acq On : 22 Apr 2022 11:42
Operator : SY/MD
Sample : N2485-16DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

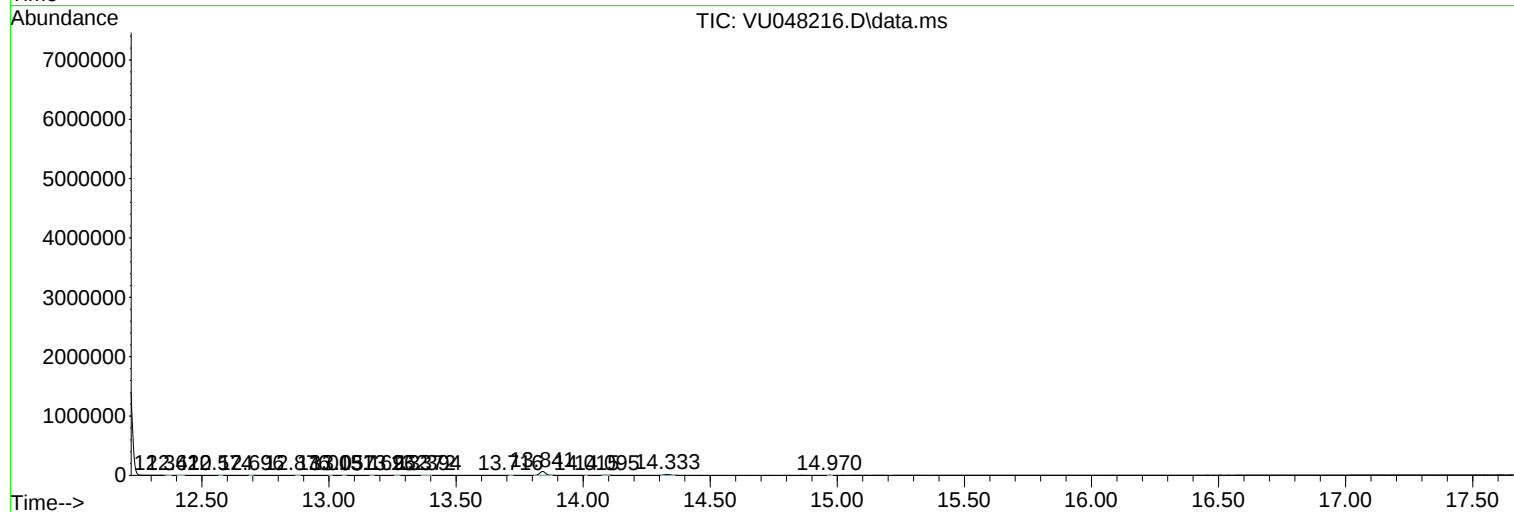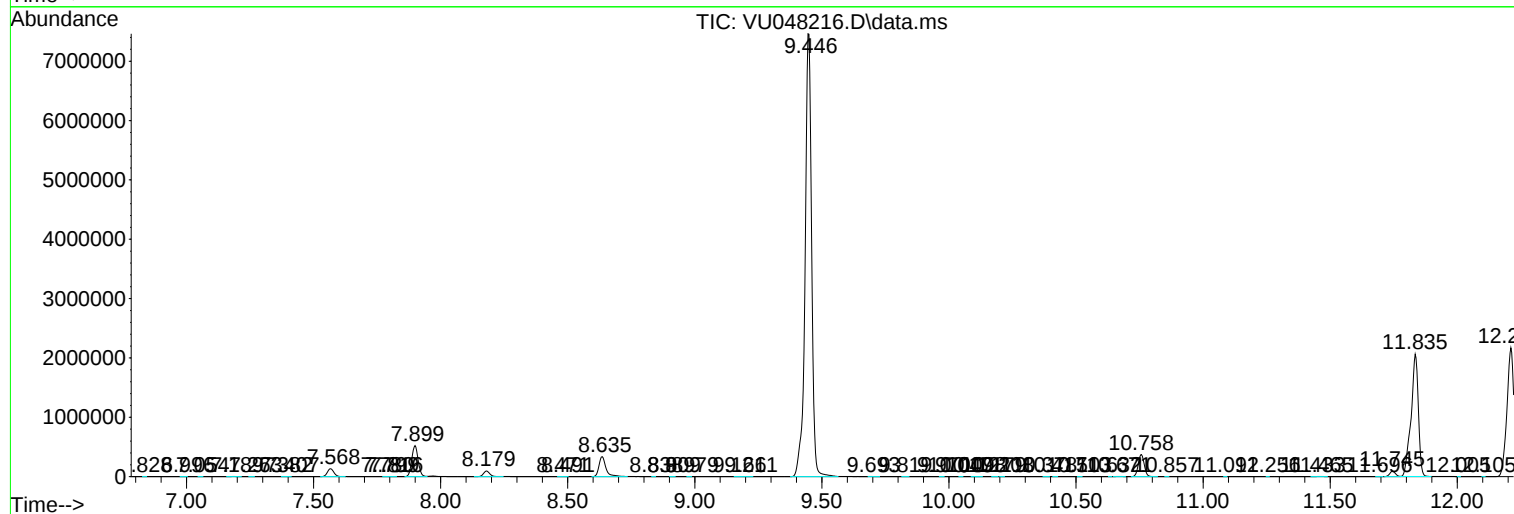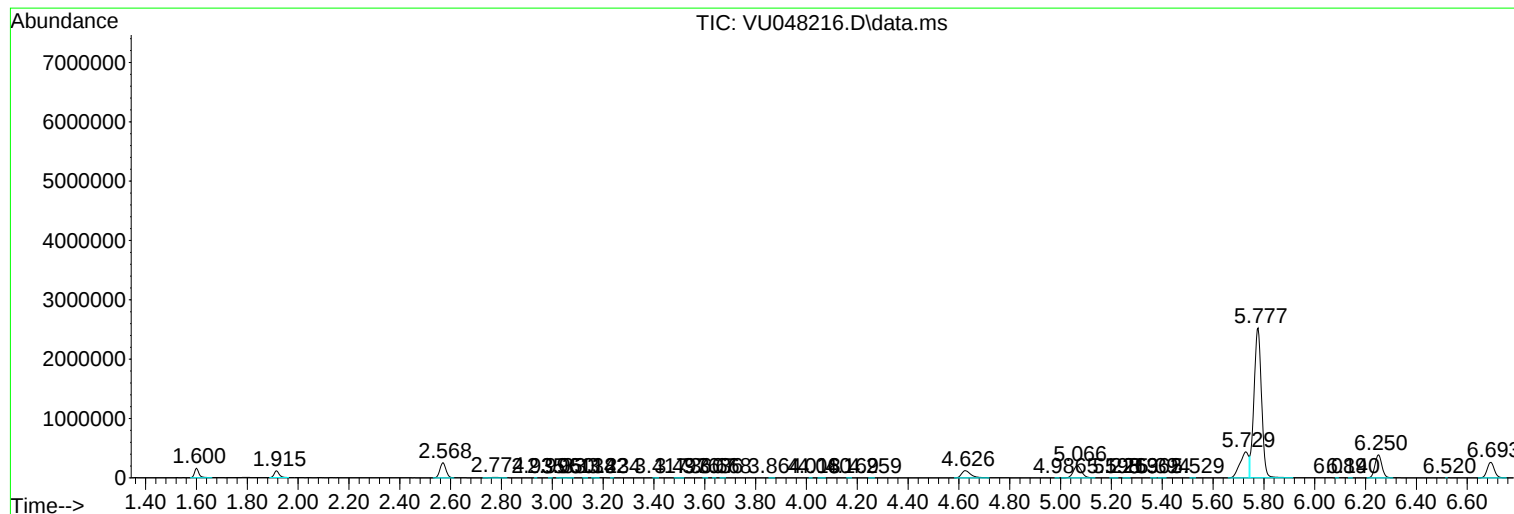

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048216.D
Acq On : 22 Apr 2022 11:42
Operator : SY/MD
Sample : N2485-16DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042222\
Data File : VU048216.D
Acq On : 22 Apr 2022 11:42
Operator : SY/MD
Sample : N2485-16DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
